

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063022\
 Data File : BP010915.D
 Acq On : 30 Jun 2022 12:04
 Operator : CG/JU
 Sample : N3523-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0JW3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010915.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	16	19	29	rVB	108358	145574	1.69%	0.185%
2	3.475	63	66	73	rBV	31410	45951	0.53%	0.058%
3	3.617	87	90	105	rBV	366442	568099	6.59%	0.721%
4	3.834	121	127	132	rBV	43345	64464	0.75%	0.082%
5	3.928	138	143	147	rBV	53772	73009	0.85%	0.093%
6	3.964	147	149	154	rVB6	6497	8940	0.10%	0.011%
7	4.640	259	264	268	rVB5	6067	9714	0.11%	0.012%
8	4.840	293	298	302	rBV3	8494	15008	0.17%	0.019%
9	4.881	302	305	310	rVB2	6141	9682	0.11%	0.012%
10	5.422	393	397	403	rBV	14052	25456	0.30%	0.032%
11	5.811	459	463	468	rVB6	5930	10962	0.13%	0.014%
12	6.711	611	616	620	rBV7	7872	13973	0.16%	0.018%
13	6.881	634	645	657	rVB	385882	614997	7.13%	0.780%
14	7.046	666	673	682	rBV	1458585	2180693	25.28%	2.766%
15	7.122	682	686	694	rVB	26809	42487	0.49%	0.054%
16	7.240	698	706	717	rBV	1390281	2132922	24.73%	2.706%
17	7.328	717	721	727	rVB7	8081	13199	0.15%	0.017%
18	7.705	777	785	793	rBV	1616866	2444210	28.34%	3.100%
19	7.775	793	797	803	rVB	13938	21015	0.24%	0.027%
20	8.052	839	844	848	rBV5	7370	13234	0.15%	0.017%
21	8.305	879	887	895	rVB5	6850	17245	0.20%	0.022%
22	8.416	900	906	918	rBV	1014984	1586923	18.40%	2.013%
23	8.863	975	982	993	rBV	1490956	2432136	28.20%	3.085%
24	8.987	998	1003	1007	rVV4	11008	20483	0.24%	0.026%
25	9.034	1007	1011	1020	rVB4	8744	16266	0.19%	0.021%
26	9.287	1047	1054	1061	rBV	58949	93015	1.08%	0.118%
27	9.587	1097	1105	1119	rBV	1053904	1685167	19.54%	2.138%
28	9.834	1142	1147	1151	rVB8	7717	15747	0.18%	0.020%
29	10.122	1186	1196	1206	rBV	1637660	2581394	29.93%	3.274%
30	10.299	1220	1226	1231	rVV10	6920	13358	0.15%	0.017%
31	10.499	1252	1260	1269	rBV	1984929	3298442	38.24%	4.184%
32	10.640	1277	1284	1300	rBV	1040957	1777262	20.61%	2.254%
33	10.881	1319	1325	1329	rBV9	5973	9965	0.12%	0.013%
34	11.316	1392	1399	1403	rBV10	11401	23345	0.27%	0.030%
35	11.793	1475	1480	1487	rVB	29895	45785	0.53%	0.058%
36	12.016	1513	1518	1522	rBV8	6450	12963	0.15%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063022\
 Data File : BP010915.D
 Acq On : 30 Jun 2022 12:04
 Operator : CG/JU
 Sample : N3523-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0JW3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

37	12.093	1525	1531	1539	rVB	33999	57284	0.66%	0.073%
38	12.716	1633	1637	1641	rBV5	7171	9167	0.11%	0.012%
39	12.975	1676	1681	1685	rVB5	10737	15657	0.18%	0.020%
40	13.193	1711	1718	1725	rVB5	17862	38105	0.44%	0.048%
41	13.263	1725	1730	1736	rBV5	12467	27188	0.32%	0.034%
42	13.328	1736	1741	1747	rVV10	10367	17020	0.20%	0.022%
43	13.581	1780	1784	1790	rBV8	6054	10252	0.12%	0.013%
44	13.781	1811	1818	1829	rBV	2605575	3667092	42.52%	4.652%
45	14.051	1855	1864	1881	rBV	3158760	4562864	52.91%	5.788%
46	14.357	1907	1916	1929	rBV	2454122	3689182	42.78%	4.680%
47	14.575	1947	1953	1965	rBV	211484	347166	4.03%	0.440%
48	14.792	1986	1990	1995	rBV8	12296	17607	0.20%	0.022%
49	15.116	2040	2045	2050	rBV	24619	36500	0.42%	0.046%
50	15.181	2051	2056	2062	rVB	31226	45820	0.53%	0.058%
51	15.357	2080	2086	2093	rBV	3969481	5823998	67.53%	7.388%
52	15.481	2101	2107	2122	rBV	775923	1098870	12.74%	1.394%
53	15.598	2122	2127	2134	rVB	47067	72303	0.84%	0.092%
54	15.934	2180	2184	2190	rBV8	7687	14319	0.17%	0.018%
55	16.151	2217	2221	2227	rVB3	23669	35367	0.41%	0.045%
56	16.275	2236	2242	2243	rBV6	7762	12235	0.14%	0.016%
57	16.904	2344	2349	2353	rBV6	11280	23036	0.27%	0.029%
58	17.122	2379	2386	2397	rBV	2761717	3942367	45.71%	5.001%
59	17.222	2397	2403	2422	rVB	4517548	6360879	73.75%	8.069%
60	17.504	2448	2451	2452	rBV3	9732	10227	0.12%	0.013%
61	17.528	2453	2455	2462	rVB5	27707	41930	0.49%	0.053%
62	17.822	2499	2505	2513	rBV	271399	338455	3.92%	0.429%
63	18.104	2551	2553	2557	rVB3	9108	9500	0.11%	0.012%
64	18.957	2694	2698	2702	rBV	370343	421212	4.88%	0.534%
65	19.051	2710	2714	2717	rBV2	60137	77462	0.90%	0.098%
66	19.092	2717	2721	2723	rVV	83210	97563	1.13%	0.124%
67	19.116	2723	2725	2729	rVB	53655	62663	0.73%	0.079%
68	19.475	2780	2786	2793	rBV	5883257	7453609	86.42%	9.455%
69	21.239	3081	3086	3091	rBV	3797126	4696820	54.46%	5.958%
70	23.445	3454	3461	3471	rBV2	4454535	8624614	100.00%	10.940%
71	23.598	3481	3487	3498	rVB2	2522286	4993698	57.90%	6.334%




Sum of corrected areas: 78835116

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063022\
Data File : BP010915.D
Acq On : 30 Jun 2022 12:04
Operator : CG/JU
Sample : N3523-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0JW3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

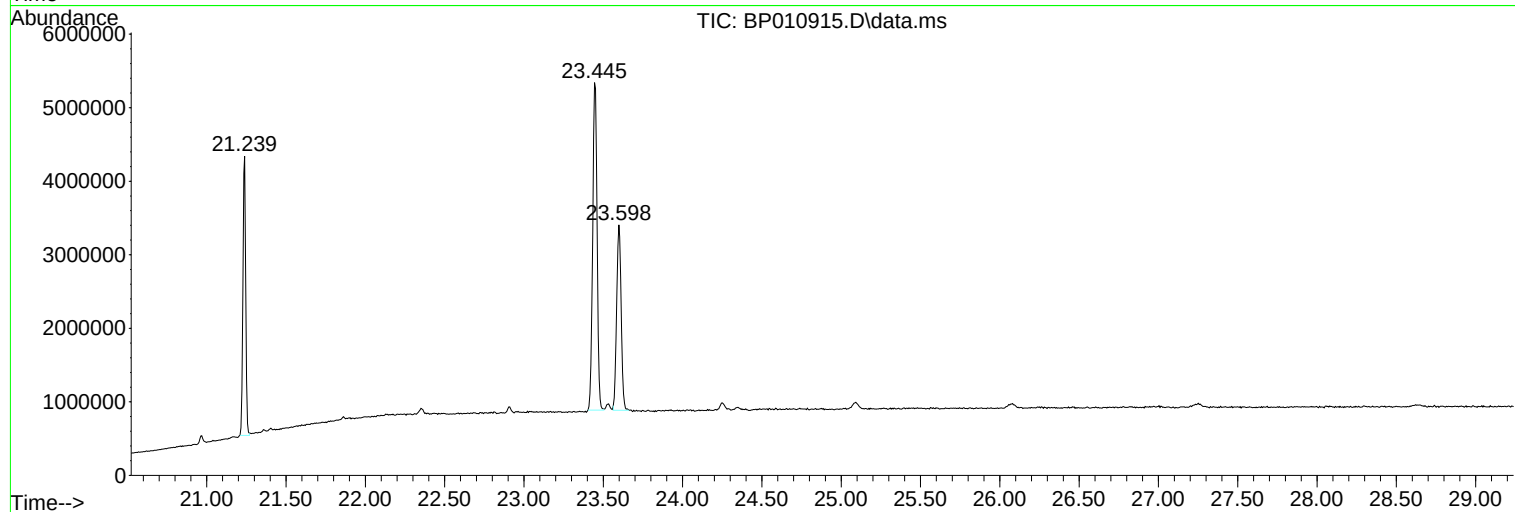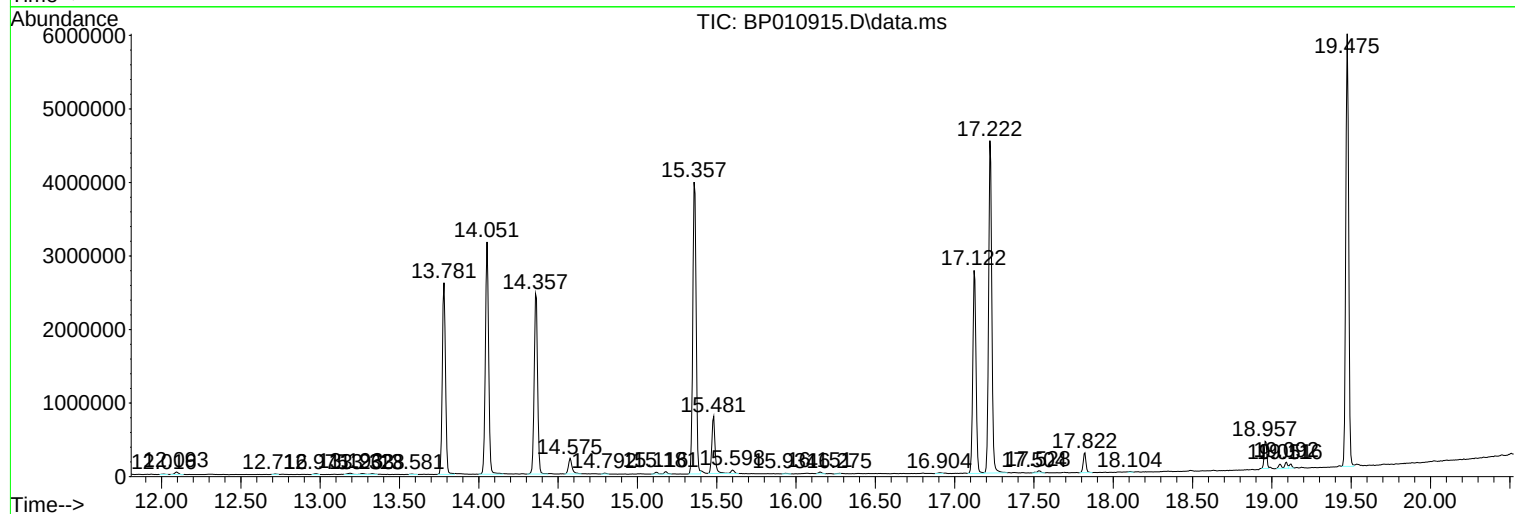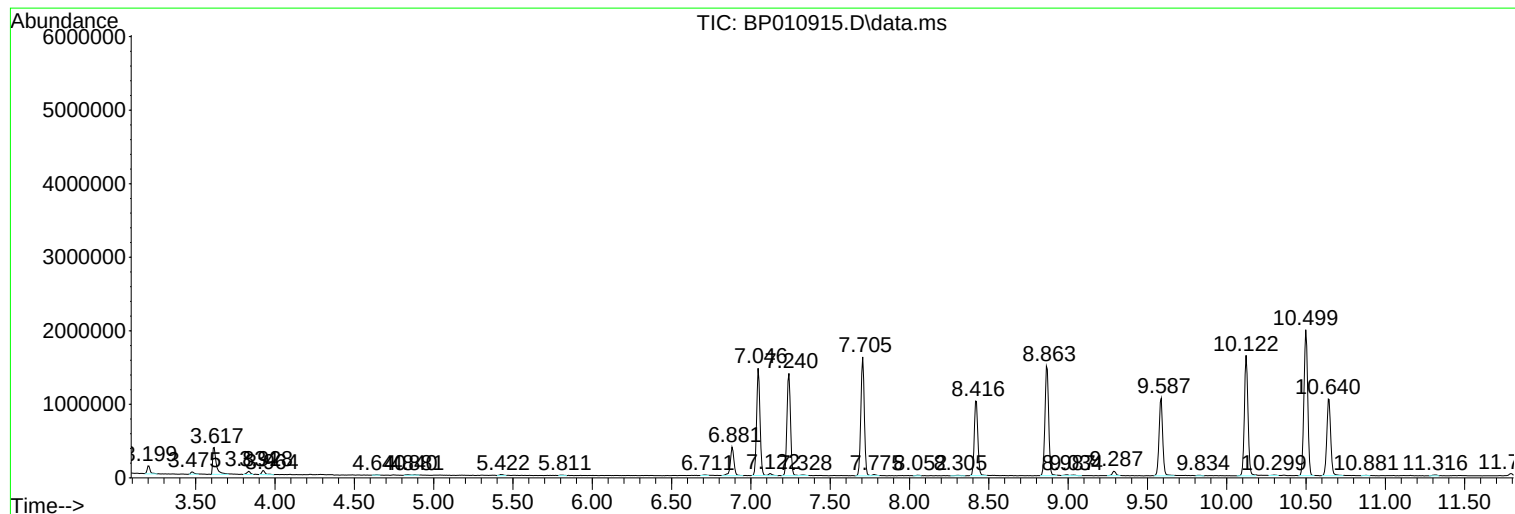

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063022\
Data File : BP010915.D
Acq On : 30 Jun 2022 12:04
Operator : CG/JU
Sample : N3523-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0JW3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 6-Octadecenoic acid, methyl... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
18.957	2.14 ng/ul	421212	Phenanthrene-d10	17.122

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			6-Octadecenoic acid, methyl ester	296	C19H36O2	052355-31-4	99
2			9-Octadecenoic acid (Z)-, methyl...	296	C19H36O2	000112-62-9	99
3			11-Octadecenoic acid, methyl ester	296	C19H36O2	052380-33-3	99
4			11-Octadecenoic acid, methyl ester	296	C19H36O2	052380-33-3	98
5			6-Octadecenoic acid, methyl este...	296	C19H36O2	002777-58-4	96

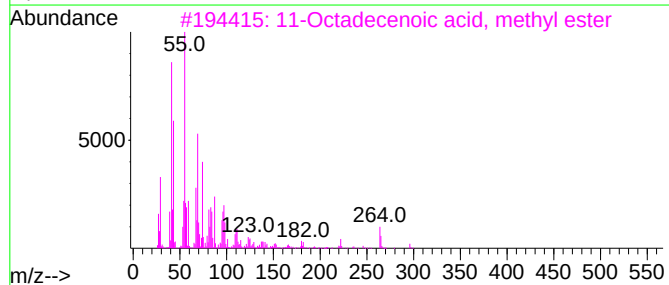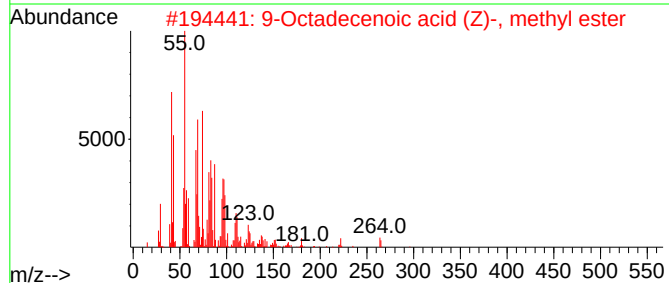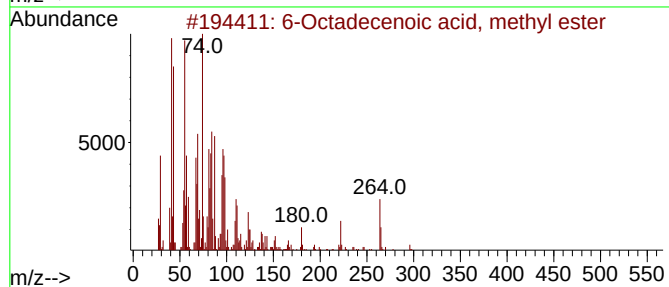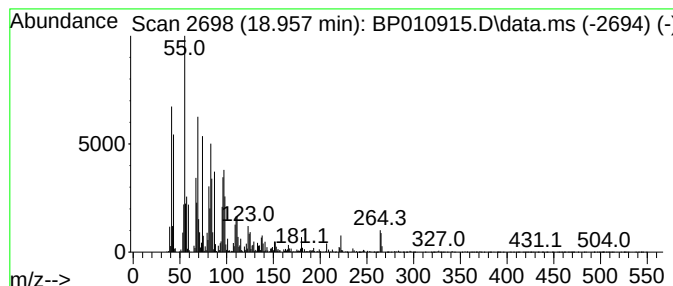

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063022\
Data File : BP010915.D
Acq On : 30 Jun 2022 12:04
Operator : CG/JU
Sample : N3523-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0JW3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
6-Octadecenoic ...	18.957	2.1	ng/ul	421212	4	17.122	3942370	20.0