

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063022\
 Data File : BP010916.D
 Acq On : 30 Jun 2022 12:37
 Operator : CG/JU
 Sample : N3523-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0JW9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010916.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	15	20	29	rVB	109313	141575	1.52%	0.178%
2	3.481	64	67	72	rBV	21771	33902	0.36%	0.043%
3	3.617	87	90	113	rVB	288920	428523	4.60%	0.540%
4	3.834	122	127	133	rVB	37693	57476	0.62%	0.072%
5	3.923	138	142	155	rVB	71827	105315	1.13%	0.133%
6	4.834	293	297	301	rBV3	10275	15154	0.16%	0.019%
7	5.358	382	386	388	rBV4	8685	10721	0.12%	0.013%
8	5.428	394	398	405	rVB2	10809	16228	0.17%	0.020%
9	5.722	444	448	452	rBV4	9719	13085	0.14%	0.016%
10	5.805	458	462	470	rBV	15294	22125	0.24%	0.028%
11	6.711	609	616	621	rBV	4795	11556	0.12%	0.015%
12	6.881	635	645	653	rVV	399142	624427	6.70%	0.786%
13	7.046	666	673	682	rBV	1521501	2283474	24.52%	2.875%
14	7.122	682	686	693	rVB	23174	37584	0.40%	0.047%
15	7.240	696	706	717	rBV	1436775	2248413	24.14%	2.831%
16	7.352	717	725	731	rVB2	16594	39544	0.42%	0.050%
17	7.705	778	785	793	rBV	1580841	2404576	25.82%	3.028%
18	7.775	793	797	802	rVV	15318	26060	0.28%	0.033%
19	7.958	820	828	835	rBV9	12216	27329	0.29%	0.034%
20	8.416	899	906	917	rBV	1061424	1671716	17.95%	2.105%
21	8.810	968	973	975	rBV6	6944	10120	0.11%	0.013%
22	8.863	975	982	993	rVV	1580633	2512210	26.97%	3.163%
23	8.981	998	1002	1007	rVB8	5059	9341	0.10%	0.012%
24	9.293	1049	1055	1060	rBV2	77020	116708	1.25%	0.147%
25	9.587	1097	1105	1122	rBV	1049283	1732147	18.60%	2.181%
26	9.734	1128	1130	1136	rVB7	5761	11229	0.12%	0.014%
27	10.122	1189	1196	1206	rBV	1645095	2673971	28.71%	3.367%
28	10.293	1222	1225	1234	rVB	3902	9495	0.10%	0.012%
29	10.499	1250	1260	1267	rBV	1984217	3254841	34.95%	4.098%
30	10.646	1274	1285	1297	rBV	1113686	1934316	20.77%	2.436%
31	10.869	1316	1323	1331	rBV	116086	212641	2.28%	0.268%
32	11.157	1368	1372	1378	rVB6	6048	9458	0.10%	0.012%
33	11.793	1473	1480	1488	rBV2	36497	58677	0.63%	0.074%
34	11.940	1501	1505	1511	rVB8	6900	10672	0.11%	0.013%
35	12.093	1525	1531	1539	rVV	36483	59681	0.64%	0.075%
36	12.169	1539	1544	1549	rVB5	7419	14756	0.16%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063022\
 Data File : BP010916.D
 Acq On : 30 Jun 2022 12:37
 Operator : CG/JU
 Sample : N3523-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0JW9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

37	12.310	1562	1568	1574	rBV9	4845	11682	0.13%	0.015%
38	12.975	1674	1681	1687	rBV10	9282	20194	0.22%	0.025%
39	13.193	1713	1718	1724	rBV2	18966	25025	0.27%	0.032%
40	13.263	1727	1730	1736	rVB7	5175	9473	0.10%	0.012%
41	13.328	1736	1741	1744	rBV6	7841	10893	0.12%	0.014%
42	13.781	1811	1818	1825	rBV	2728285	3680362	39.52%	4.634%
43	14.051	1854	1864	1875	rBV	3290238	4680329	50.25%	5.893%
44	14.275	1898	1902	1905	rVB6	8040	11609	0.12%	0.015%
45	14.357	1909	1916	1930	rBV	2379753	3538227	37.99%	4.455%
46	14.575	1947	1953	1964	rBV	222223	350944	3.77%	0.442%
47	14.798	1987	1991	1997	rVB7	9068	16103	0.17%	0.020%
48	15.175	2051	2055	2061	rBV	29688	43976	0.47%	0.055%
49	15.357	2079	2086	2100	rBV	4012095	5863562	62.96%	7.383%
50	15.481	2100	2107	2120	rVV	859785	1241091	13.33%	1.563%
51	15.598	2122	2127	2135	rVB	48468	79944	0.86%	0.101%
52	16.051	2198	2204	2206	rBV7	5912	10370	0.11%	0.013%
53	16.151	2216	2221	2225	rBV4	18327	25524	0.27%	0.032%
54	16.804	2327	2332	2336	rVB7	6976	10609	0.11%	0.013%
55	16.904	2345	2349	2352	rBV4	8813	12852	0.14%	0.016%
56	17.122	2380	2386	2397	rBV	2589165	3702398	39.75%	4.662%
57	17.222	2397	2403	2418	rVV2	4702808	6762451	72.61%	8.515%
58	17.816	2501	2504	2510	rVB	14523	17508	0.19%	0.022%
59	19.051	2710	2714	2718	rBV3	54912	79170	0.85%	0.100%
60	19.116	2722	2725	2729	rVV	52020	64979	0.70%	0.082%
61	19.475	2780	2786	2794	rBV	6245380	7851634	84.30%	9.886%
62	20.969	3037	3040	3044	rBV	83914	99644	1.07%	0.125%
63	21.239	3081	3086	3091	rBV	3462097	4330930	46.50%	5.453%
64	23.445	3454	3461	3471	rVB2	4946349	9313799	100.00%	11.727%
65	23.598	3481	3487	3499	rVB2	2460316	4706100	50.53%	5.926%




Sum of corrected areas: 79420428

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063022\
Data File : BP010916.D
Acq On : 30 Jun 2022 12:37
Operator : CG/JU
Sample : N3523-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0JW9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

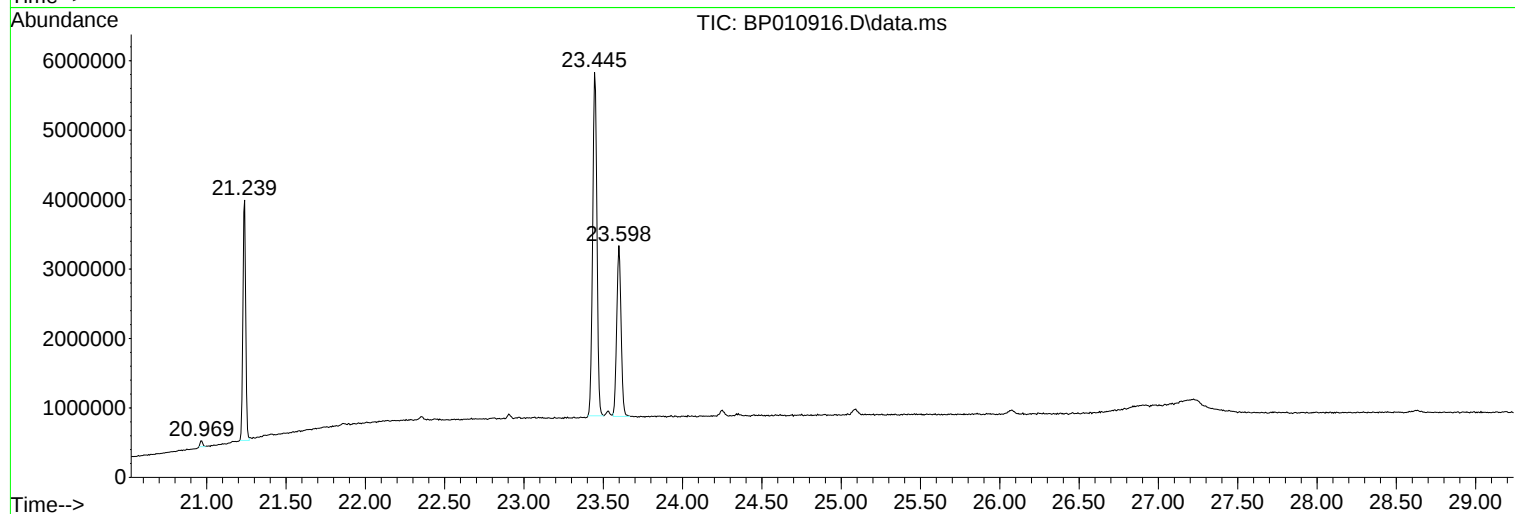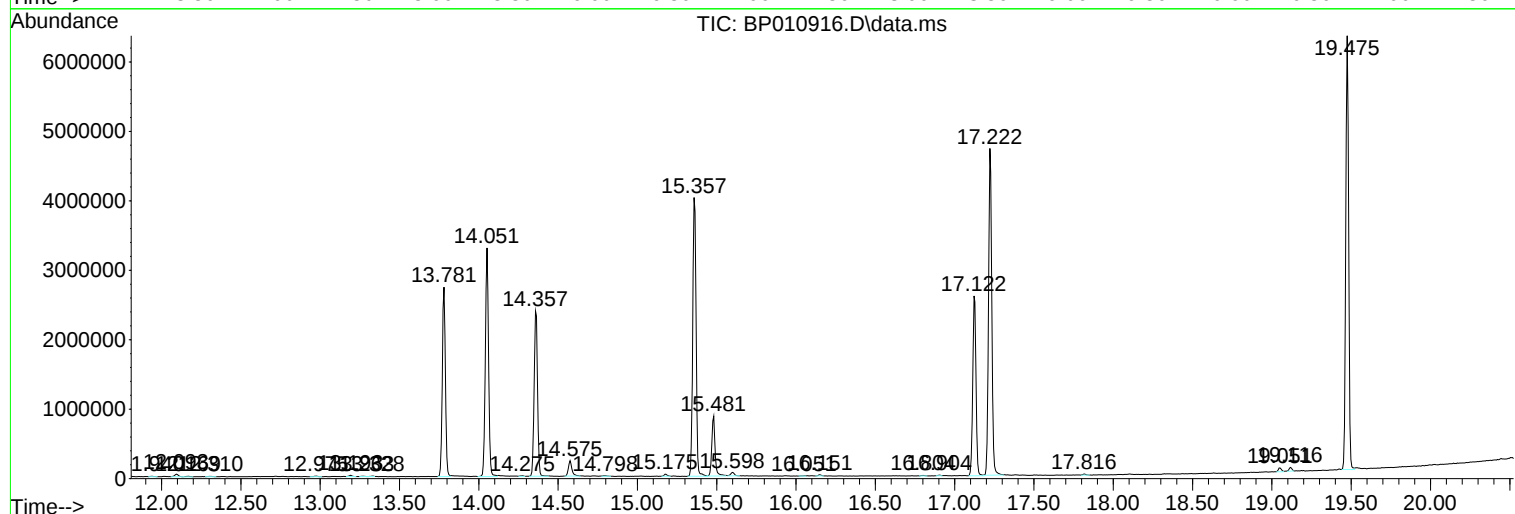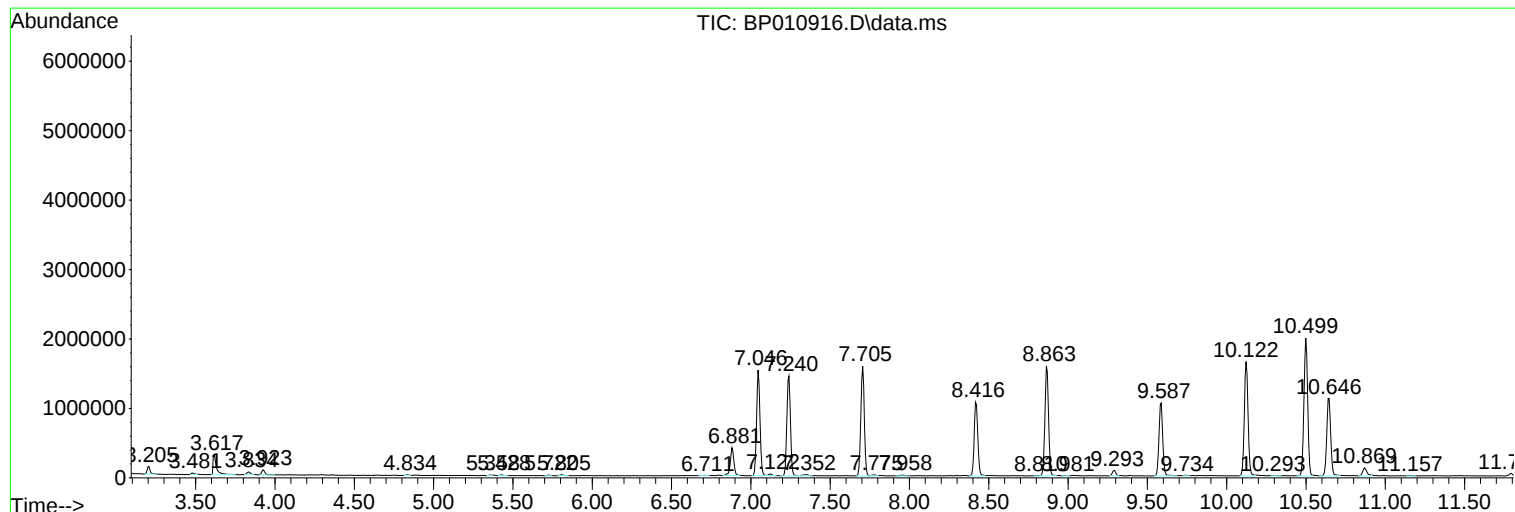

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063022\
Data File : BP010916.D
Acq On : 30 Jun 2022 12:37
Operator : CG/JU
Sample : N3523-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0JW9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063022\
Data File : BP010916.D
Acq On : 30 Jun 2022 12:37
Operator : CG/JU
Sample : N3523-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0JW9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc