

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063022\
 Data File : BP010917.D
 Acq On : 30 Jun 2022 13:11
 Operator : CG/JU
 Sample : N3523-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0JX5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010917.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	16	19	29	rVB	110870	149818	1.68%	0.181%
2	3.481	64	67	74	rVB	12461	20409	0.23%	0.025%
3	3.616	87	90	103	rBV	341395	520815	5.85%	0.628%
4	3.834	122	127	132	rVB	43153	60509	0.68%	0.073%
5	3.928	138	143	148	rVB	47297	63116	0.71%	0.076%
6	4.463	232	234	242	rVB9	7304	11722	0.13%	0.014%
7	4.640	259	264	269	rBV3	5877	9483	0.11%	0.011%
8	4.834	294	297	302	rVB3	8455	11308	0.13%	0.014%
9	4.893	302	307	310	rBV5	5849	11713	0.13%	0.014%
10	5.034	326	331	334	rBV4	8113	11763	0.13%	0.014%
11	5.381	385	390	394	rBV8	4791	10546	0.12%	0.013%
12	5.428	394	398	403	rVV	10255	12564	0.14%	0.015%
13	6.881	634	645	654	rBV	404346	636384	7.14%	0.767%
14	7.046	666	673	682	rBV	1642723	2445490	27.45%	2.949%
15	7.122	682	686	693	rVB	24234	36970	0.41%	0.045%
16	7.240	698	706	717	rBV	1507695	2326462	26.11%	2.805%
17	7.328	719	721	731	rVB8	9882	16433	0.18%	0.020%
18	7.705	777	785	794	rBV	1762679	2668751	29.95%	3.218%
19	7.775	794	797	803	rVB2	15423	24226	0.27%	0.029%
20	8.310	880	888	893	rBV2	7121	14700	0.16%	0.018%
21	8.416	899	906	917	rBV	1098701	1727491	19.39%	2.083%
22	8.863	973	982	990	rBV	1685101	2722378	30.55%	3.283%
23	8.987	999	1003	1008	rBV4	9243	14056	0.16%	0.017%
24	9.034	1008	1011	1017	rVB8	7876	12202	0.14%	0.015%
25	9.293	1048	1055	1060	rVB	96955	150622	1.69%	0.182%
26	9.587	1089	1105	1119	rBV	1155912	1929351	21.65%	2.326%
27	10.122	1186	1196	1215	rBV	1792005	2866320	32.17%	3.456%
28	10.363	1232	1237	1241	rVB8	5135	9800	0.11%	0.012%
29	10.498	1252	1260	1268	rBV	2240999	3613977	40.56%	4.358%
30	10.646	1276	1285	1299	rBV	1141088	1962511	22.03%	2.366%
31	11.316	1391	1399	1403	rBV	6713	12669	0.14%	0.015%
32	11.793	1472	1480	1486	rBV	66264	97726	1.10%	0.118%
33	11.940	1501	1505	1510	rBV4	8586	13310	0.15%	0.016%
34	12.093	1525	1531	1537	rBV	38672	65751	0.74%	0.079%
35	12.310	1561	1568	1575	rBV10	5738	10739	0.12%	0.013%
36	12.722	1632	1638	1642	rBV7	7600	12773	0.14%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063022\
 Data File : BP010917.D
 Acq On : 30 Jun 2022 13:11
 Operator : CG/JU
 Sample : N3523-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0JX5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

37	12.975	1676	1681	1685	rBV5	8787	15026	0.17%	0.018%
38	13.087	1692	1700	1705	rBV5	5912	11570	0.13%	0.014%
39	13.187	1713	1717	1723	rVB	25628	36638	0.41%	0.044%
40	13.269	1726	1731	1736	rBV7	7768	15575	0.17%	0.019%
41	13.328	1736	1741	1748	rVB7	28911	48109	0.54%	0.058%
42	13.781	1811	1818	1829	rBV	3006807	4030346	45.23%	4.860%
43	14.051	1854	1864	1874	rBV	3592640	5057953	56.77%	6.099%
44	14.269	1898	1901	1905	rVB2	23699	30997	0.35%	0.037%
45	14.363	1905	1917	1931	rBV	2658152	4186827	46.99%	5.048%
46	14.575	1947	1953	1963	rBV	203699	332587	3.73%	0.401%
47	14.792	1987	1990	1995	rVB6	7674	10646	0.12%	0.013%
48	14.898	2003	2008	2013	rVB9	6612	13145	0.15%	0.016%
49	15.116	2041	2045	2050	rBV6	7627	12792	0.14%	0.015%
50	15.175	2051	2055	2061	rVV	32966	51326	0.58%	0.062%
51	15.228	2061	2064	2068	rVB	39132	46532	0.52%	0.056%
52	15.357	2079	2086	2101	rBV	4293319	6303313	70.74%	7.600%
53	15.481	2101	2107	2121	rVV	824219	1224621	13.74%	1.477%
54	15.598	2123	2127	2133	rVV	52048	90392	1.01%	0.109%
55	15.645	2133	2135	2139	rVB4	12708	11744	0.13%	0.014%
56	15.804	2157	2162	2167	rVV9	7835	15168	0.17%	0.018%
57	15.933	2178	2184	2190	rBV10	9060	19792	0.22%	0.024%
58	16.098	2208	2212	2216	rBV	50922	73216	0.82%	0.088%
59	16.151	2218	2221	2229	rVB2	51396	77185	0.87%	0.093%
60	16.898	2344	2348	2352	rBV2	55883	74259	0.83%	0.090%
61	16.945	2354	2356	2361	rVB4	13932	20082	0.23%	0.024%
62	17.122	2379	2386	2395	rBV	2727751	3998840	44.88%	4.822%
63	17.222	2397	2403	2419	rVV2	4672073	6756671	75.83%	8.147%
64	17.375	2426	2429	2434	rVB2	23263	31008	0.35%	0.037%
65	17.645	2471	2475	2479	rBV2	41852	49410	0.55%	0.060%
66	18.322	2587	2590	2595	rVB2	38199	44554	0.50%	0.054%
67	18.939	2692	2695	2697	rBV2	28953	28766	0.32%	0.035%
68	19.051	2710	2714	2719	rBV3	56770	76710	0.86%	0.092%
69	19.116	2722	2725	2730	rVB	52360	65864	0.74%	0.079%
70	19.474	2780	2786	2793	rBV	6016203	7576120	85.03%	9.135%
71	21.239	3081	3086	3091	rBV	3515677	4408036	49.47%	5.315%
72	23.445	3454	3461	3469	rBV2	4609860	8909915	100.00%	10.744%
73	23.598	3481	3487	3498	rVB2	2500633	4892304	54.91%	5.899%




Sum of corrected areas: 82932897

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063022\
Data File : BP010917.D
Acq On : 30 Jun 2022 13:11
Operator : CG/JU
Sample : N3523-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0JX5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

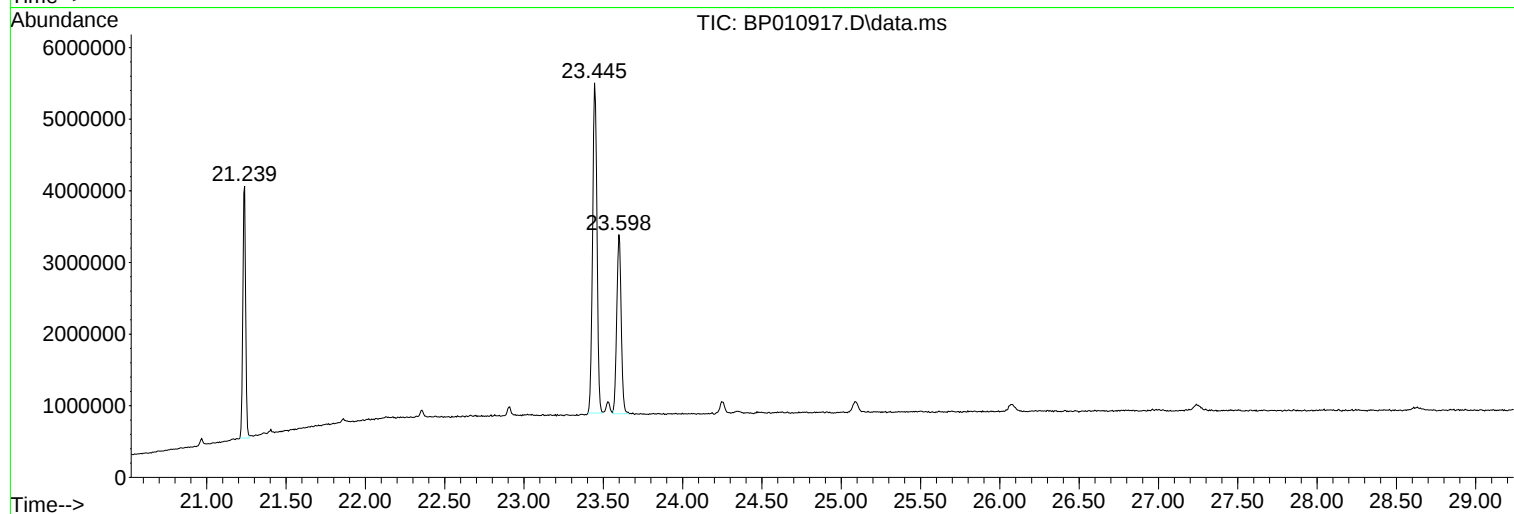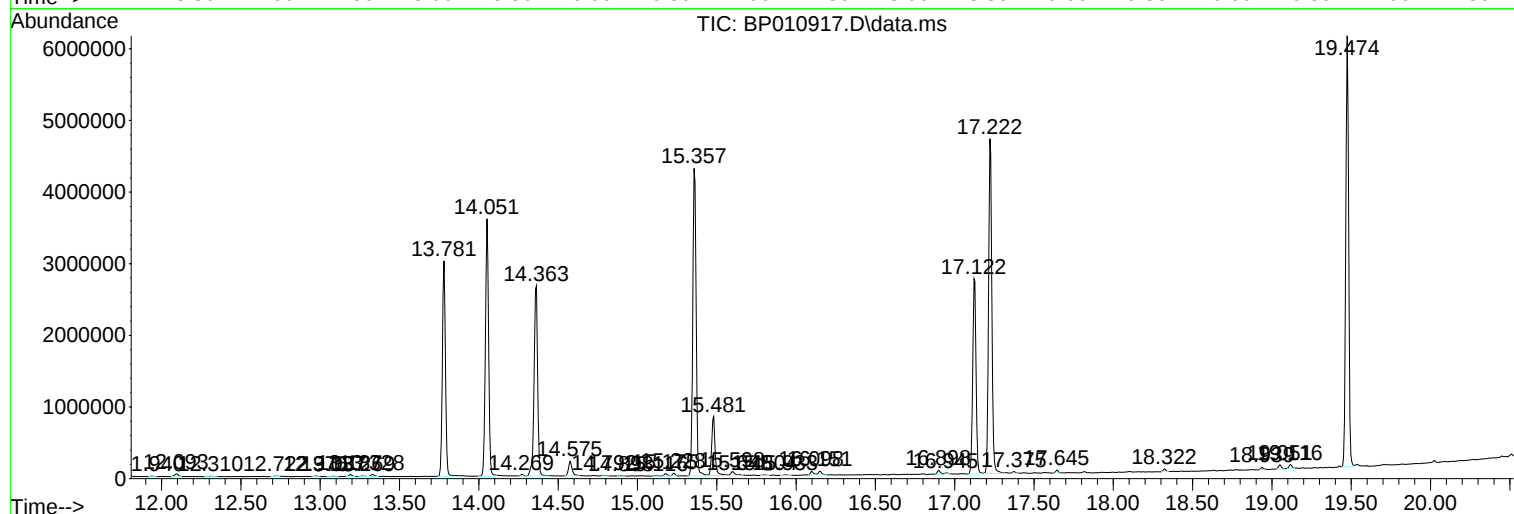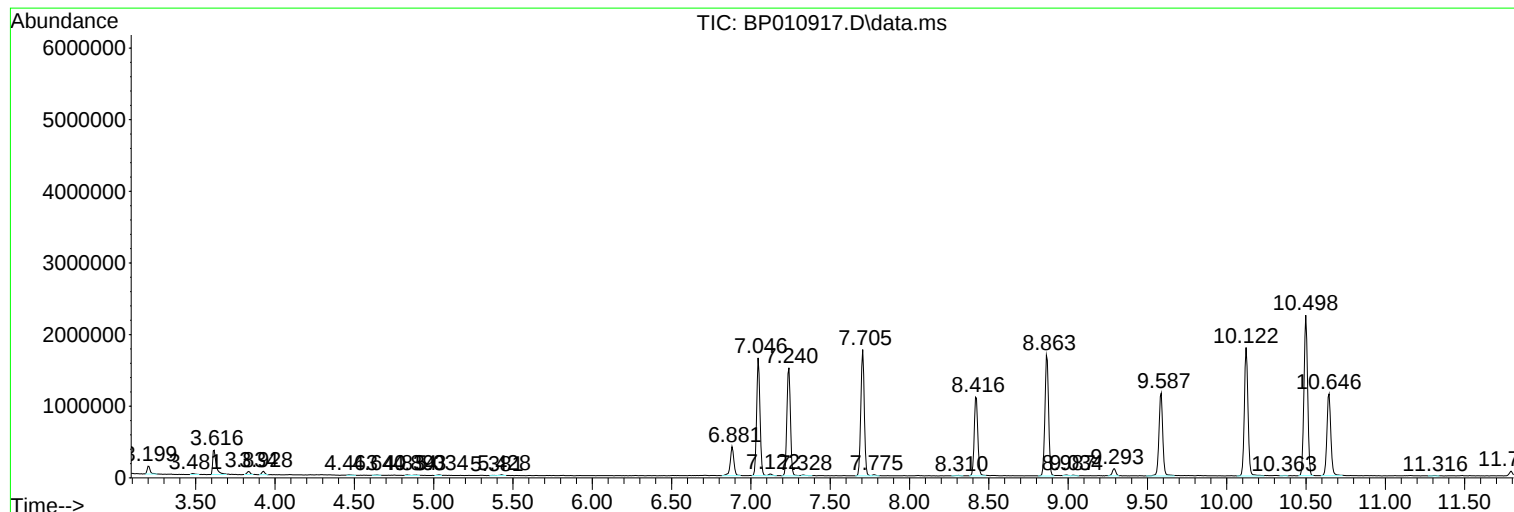

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063022\
Data File : BP010917.D
Acq On : 30 Jun 2022 13:11
Operator : CG/JU
Sample : N3523-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0JX5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063022\
Data File : BP010917.D
Acq On : 30 Jun 2022 13:11
Operator : CG/JU
Sample : N3523-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0JX5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
