


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063025\
Data File : BP025043.D
Acq On : 30 Jun 2025 15:21
Operator : RC/JU
Sample : DFTPP624
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP624

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP063025.MA.M
Title : SVOA CALIBRATION
Last Update : Tue Jul 01 11:17:33 2025

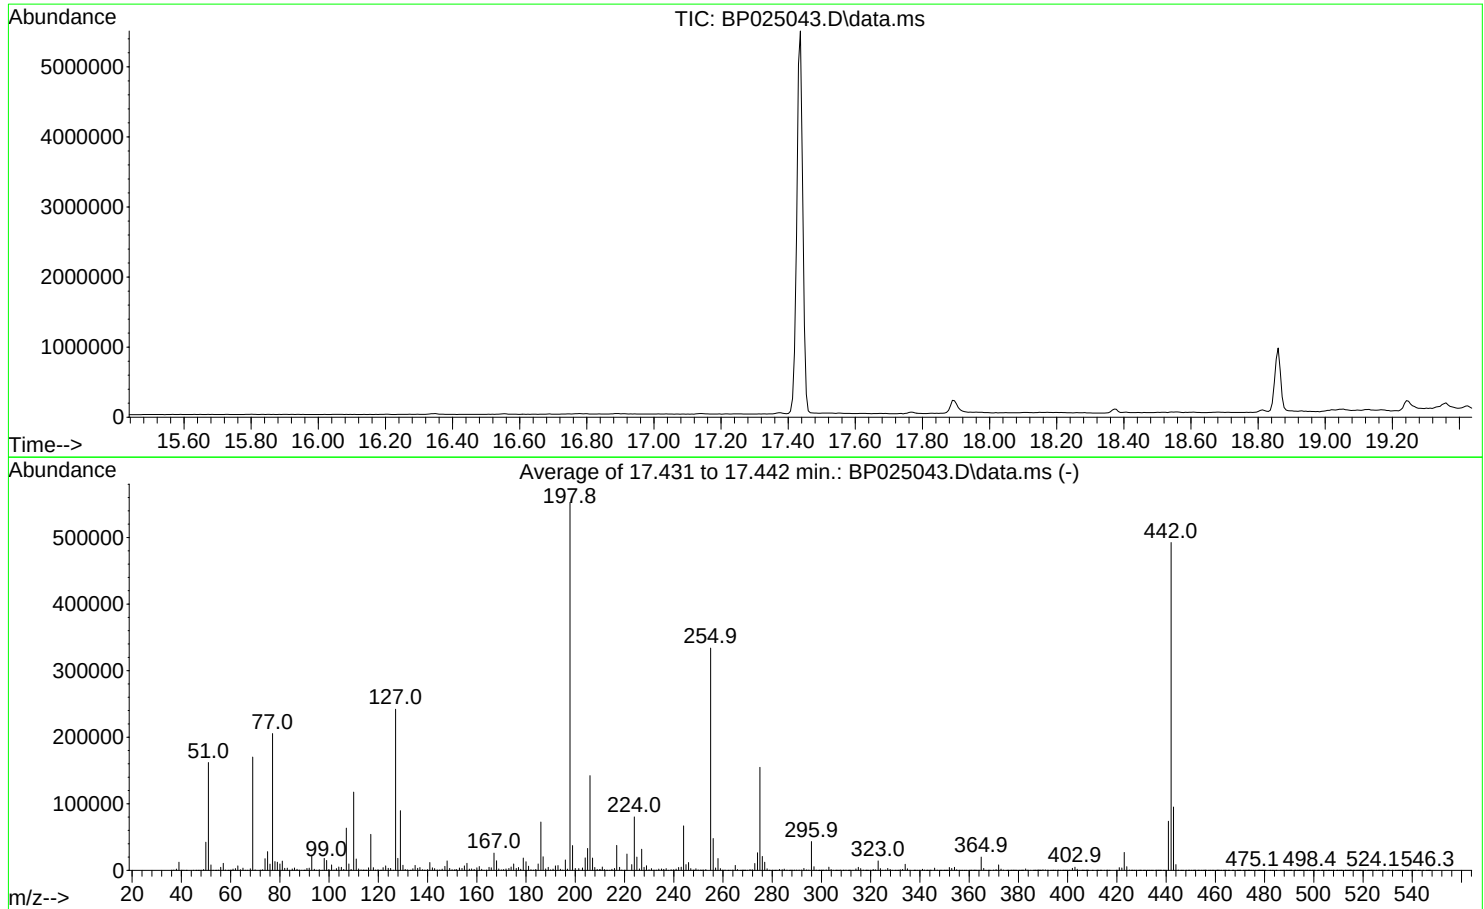

AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.3	161971	PASS
68	69	0.00	2	1.5	2480	PASS
69	198	0.00	100	30.8	170142	PASS
70	69	0.00	2	0.4	741	PASS
127	198	10	80	43.8	242074	PASS
197	198	0.00	2	0.4	1968	PASS
198	198	100	100	100.0	552551	PASS
199	198	5	9	6.7	37243	PASS
275	198	10	60	28.0	154771	PASS
365	198	1	100	3.6	20088	PASS
441	198	0.01	100	13.4	73897	PASS
442	198	50	100	89.1	492523	PASS
443	442	15	24	19.3	95088	PASS