

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP070120\
 Data File : BP002618.D
 Acq On : 01 Jul 2020 23:02
 Operator : CG/JU
 Sample : L2811-05 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 NB-7-063020

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.193	386	392	408	rBV	591640	971826	25.85%	3.801%
2	6.763	652	659	673	rBV	595440	1055948	28.09%	4.130%
3	6.875	673	678	687	rVB	39775	69870	1.86%	0.273%
4	7.569	788	796	807	rBV	1161623	1896740	50.46%	7.419%
5	7.887	843	850	861	rBV	560957	911639	24.25%	3.566%
6	8.716	983	991	1005	rBV	358403	632820	16.83%	2.475%
7	10.346	1259	1268	1284	rBV	1502609	2668800	71.00%	10.438%
8	12.834	1684	1691	1708	rBV	1039515	1589883	42.29%	6.218%
9	13.681	1826	1835	1843	rBV	110854	182142	4.85%	0.712%
10	14.222	1920	1927	1937	rBV	2330712	3425595	91.13%	13.398%
11	15.722	2176	2182	2193	rBV	679322	1008368	26.82%	3.944%
12	16.980	2390	2396	2407	rBV	2648689	3759087	100.00%	14.703%
13	18.645	2676	2679	2684	rVB	50220	56573	1.50%	0.221%
14	19.569	2831	2836	2842	rBV	1531919	1845610	49.10%	7.219%
15	21.086	3089	3094	3100	rBV	2390673	2920047	77.68%	11.421%
16	23.280	3462	3467	3476	rVB2	1395662	2572314	68.43%	10.061%


Sum of corrected areas: 25567262

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP070120\
Data File : BP002618.D
Acq On : 01 Jul 2020 23:02
Operator : CG/JU
Sample : L2811-05 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
NB-7-063020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP062920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

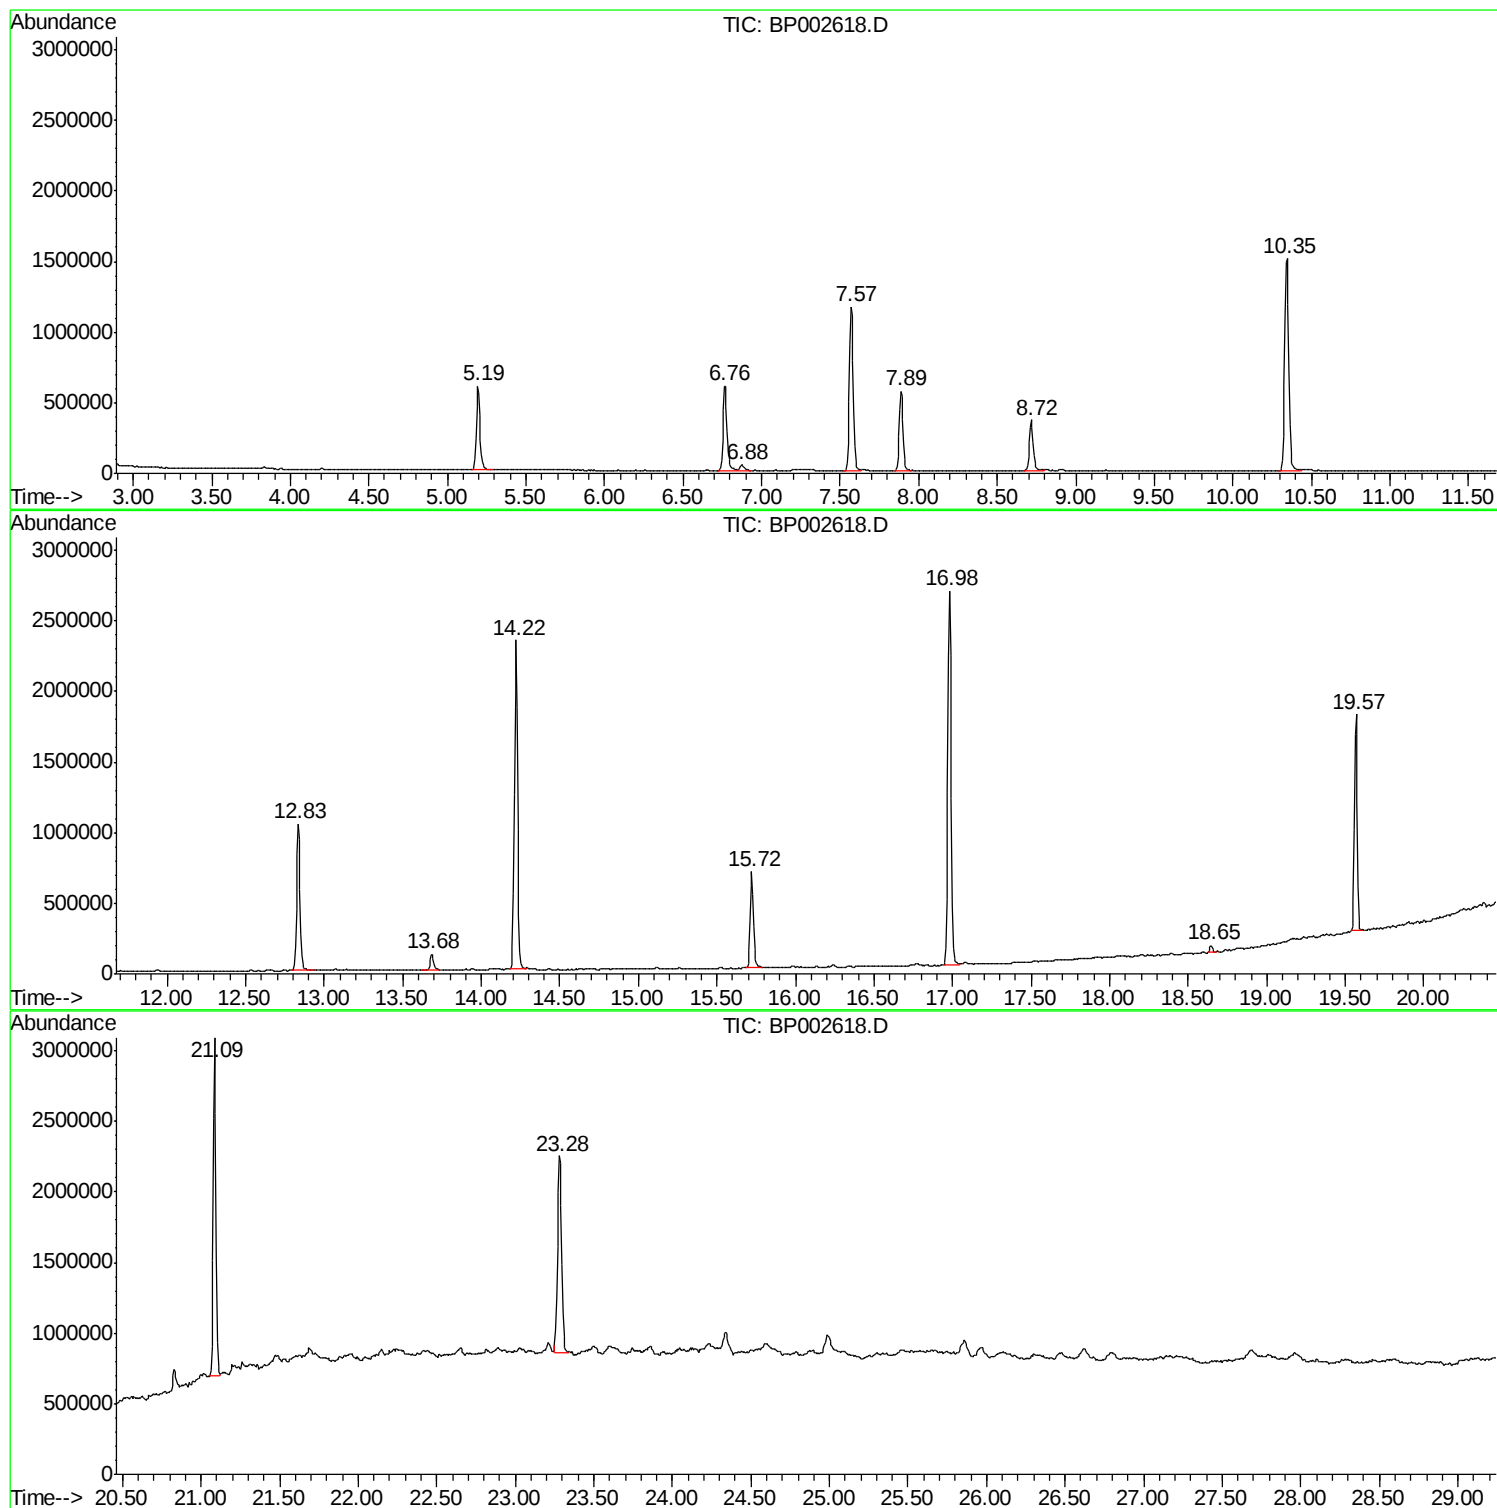

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP070120\
Data File : BP002618.D
Acq On : 01 Jul 2020 23:02
Operator : CG/JU
Sample : L2811-05 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
NB-7-063020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP070120\
Data File : BP002618.D
Acq On : 01 Jul 2020 23:02
Operator : CG/JU
Sample : L2811-05 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
NB-7-063020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc