


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP070120\
 Data File : BP002599.D
 Acq On : 01 Jul 2020 12:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 29 16:51:57 2020

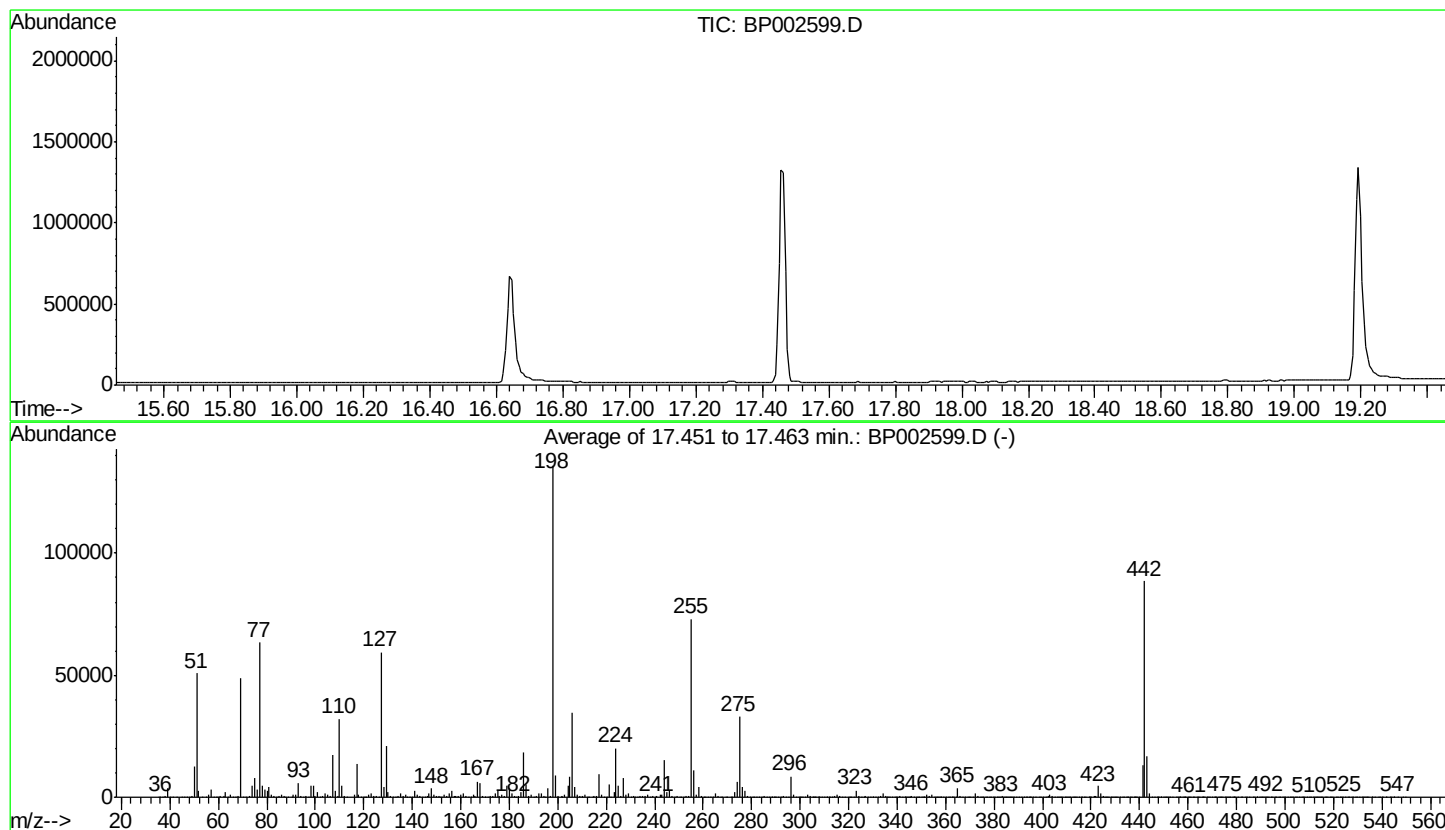

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	50763	PASS
68	69	0.00	2	1.5	748	PASS
69	198	0.00	100	35.9	48748	PASS
70	69	0.00	2	0.4	195	PASS
127	198	10	80	43.7	59382	PASS
197	198	0.00	2	0.4	550	PASS
198	198	100	100	100.0	135922	PASS
199	198	5	9	6.6	9035	PASS
275	198	10	60	24.2	32866	PASS
365	198	1	100	2.8	3752	PASS
441	198	0.01	100	9.8	13356	PASS
442	198	50	100	65.2	88588	PASS
443	442	15	24	18.7	16581	PASS