




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070124\
Data File : BP020718.D
Acq On : 01 Jul 2024 14:46
Operator : MA/JU
Sample : P2897-14DL2 50X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0T61DL2

Manual IntegrationsAPPROVED

Quant Time: Jul 01 15:19:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 25 18:30:06 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/02/2024
Supervised By :mohammad ahmed 07/04/2024

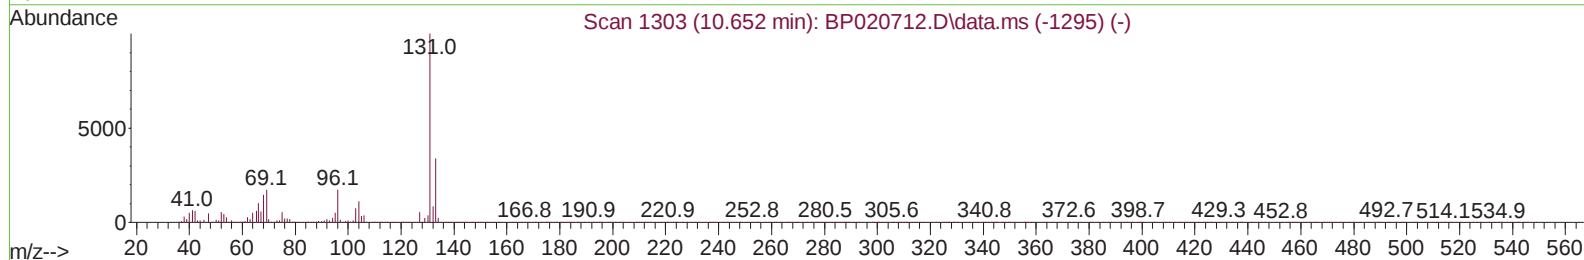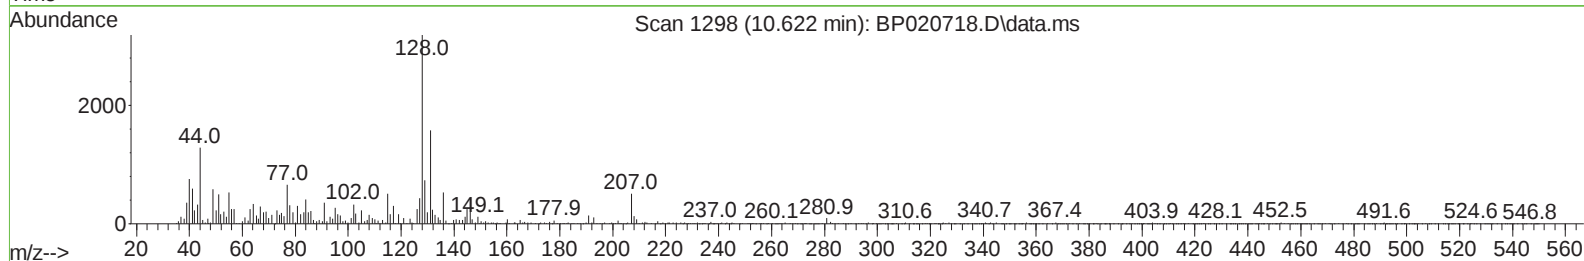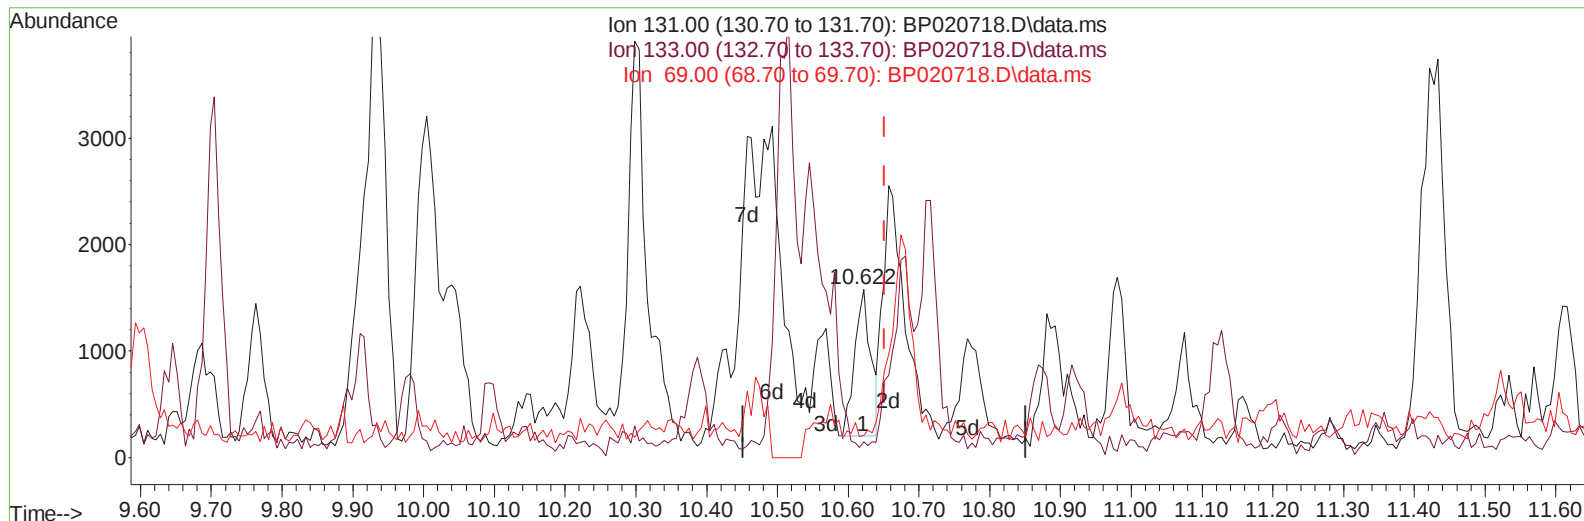

TIC: BP020718.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.622min (-0.030) 0.11 ng/u1

response 2196

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.40	9.37#
69.00	17.60	13.23#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070124\
Data File : BP020718.D
Acq On : 01 Jul 2024 14:46
Operator : MA/JU
Sample : P2897-14DL2 50X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0T61DL2

Manual IntegrationsAPPROVED

Quant Time: Jul 01 15:19:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 25 18:30:06 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/02/2024
Supervised By :mohammad ahmed 07/04/2024

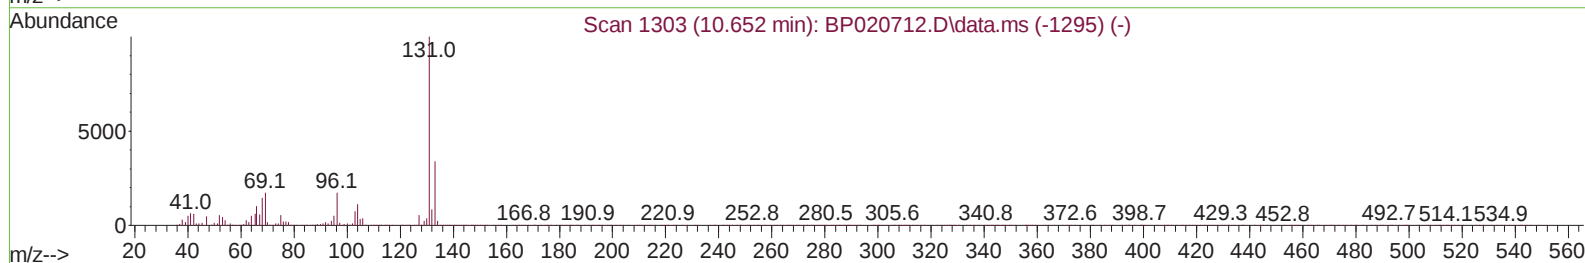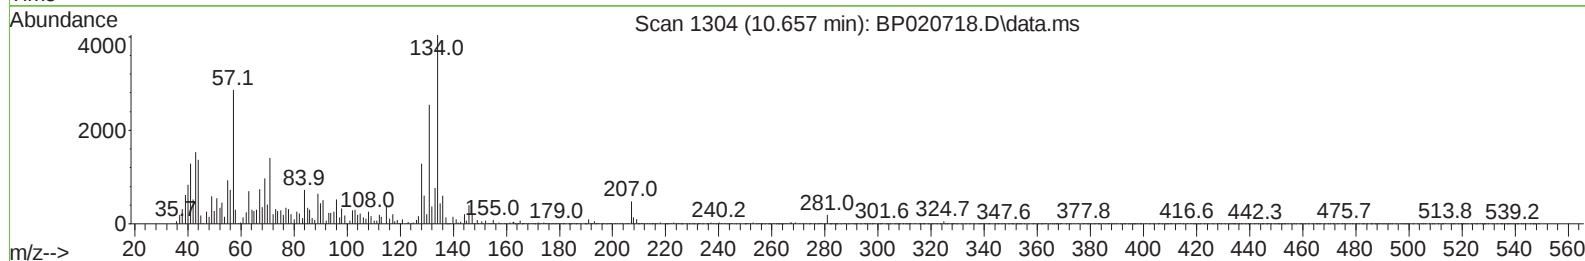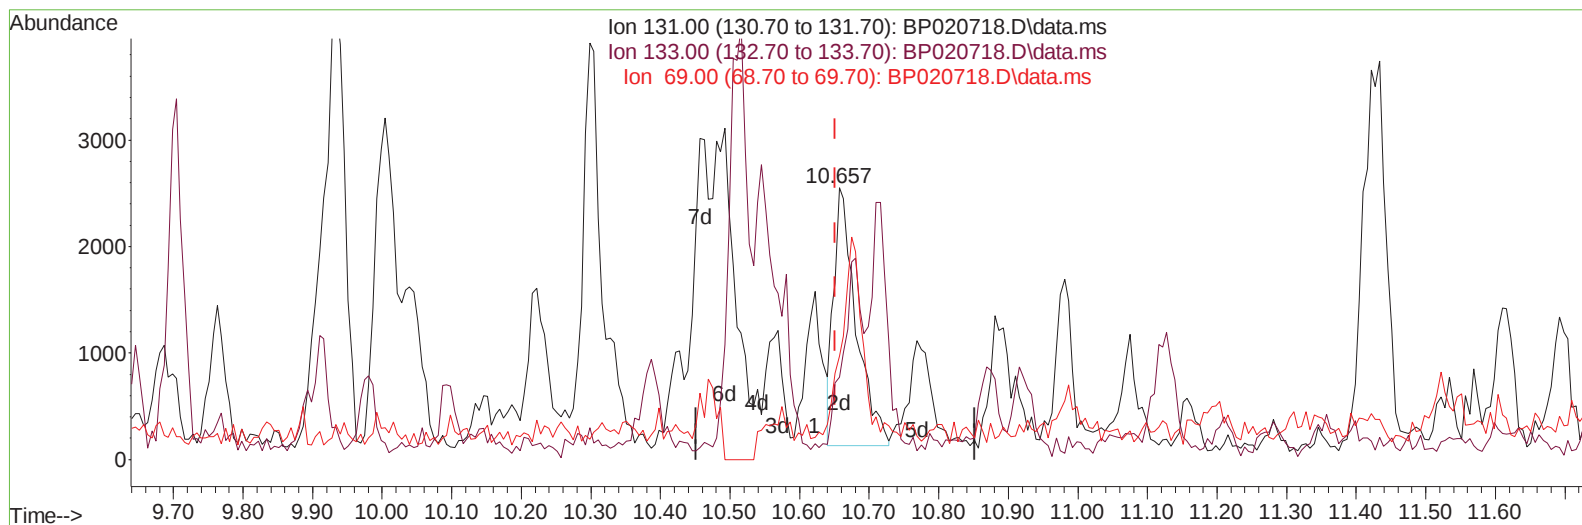

TIC: BP020718.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.657min (+ 0.006) 0.27 ng/ul m

response 5413

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.40	30.31
69.00	17.60	38.12#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070124\
 Data File : BP020718.D
 Acq On : 01 Jul 2024 14:46
 Operator : MA/JU
 Sample : P2897-14DL2 50X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0T61DL2

Manual IntegrationsAPPROVED

Quant Time: Jul 01 15:19:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 25 18:30:06 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/02/2024
 Supervised By :mohammad ahmed 07/04/2024

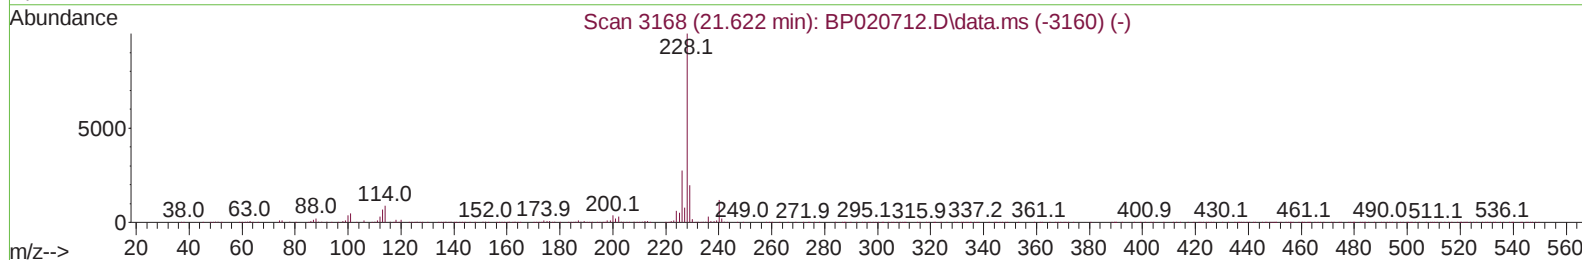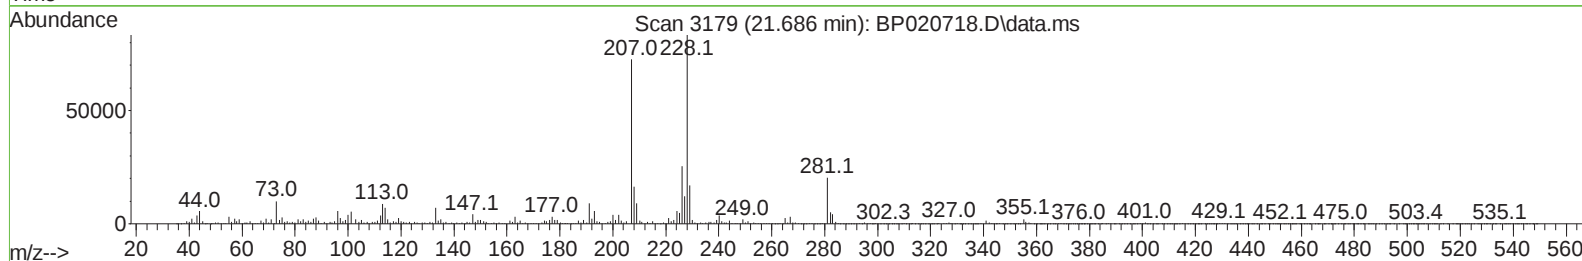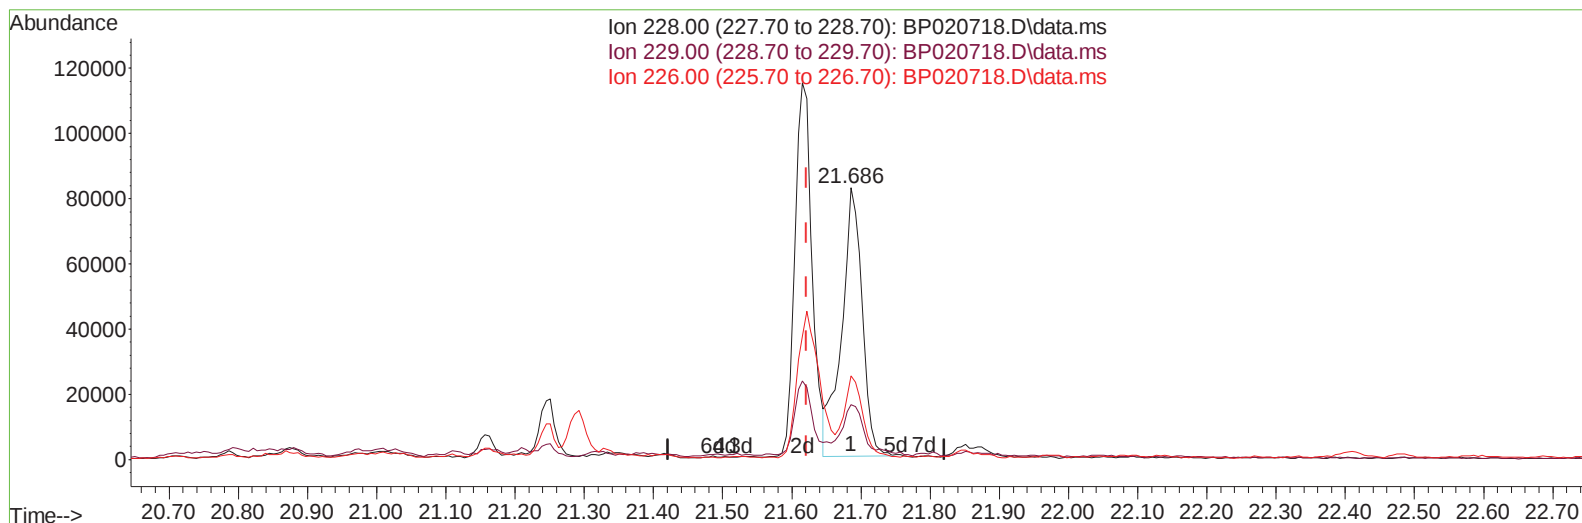

TIC: BP020718.D\data.ms

(85) Benzo(a)anthracene

21.686min (+ 0.064) 2.70 ng/u1

response 169250

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	19.00	20.29
226.00	26.40	30.67
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070124\
Data File : BP020718.D
Acq On : 01 Jul 2024 14:46
Operator : MA/JU
Sample : P2897-14DL2 50X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0T61DL2

Manual IntegrationsAPPROVED

Quant Time: Jul 01 15:19:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 25 18:30:06 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/02/2024
Supervised By :mohammad ahmed 07/04/2024

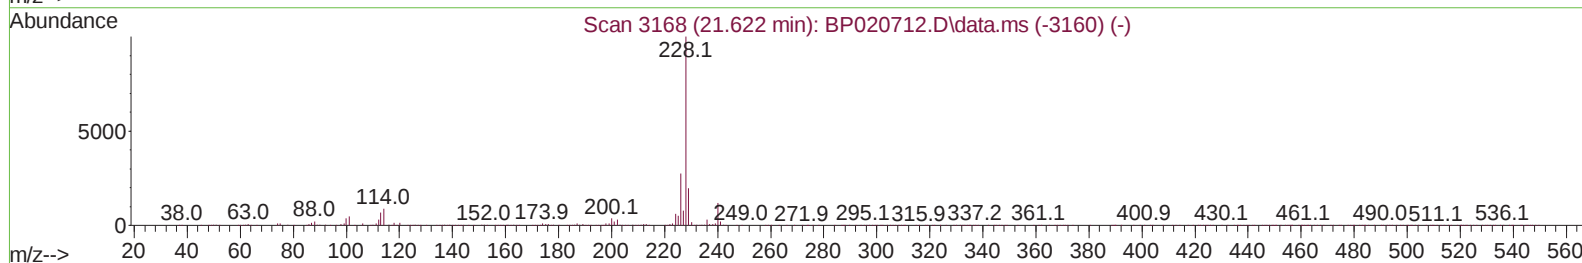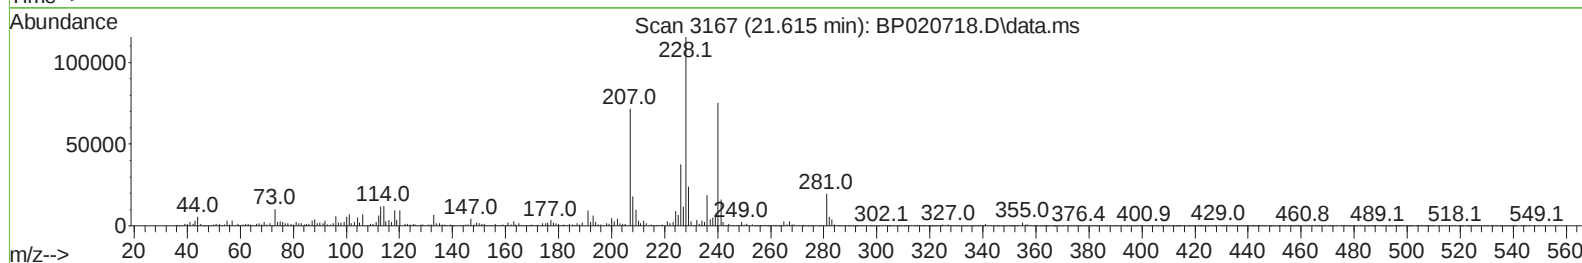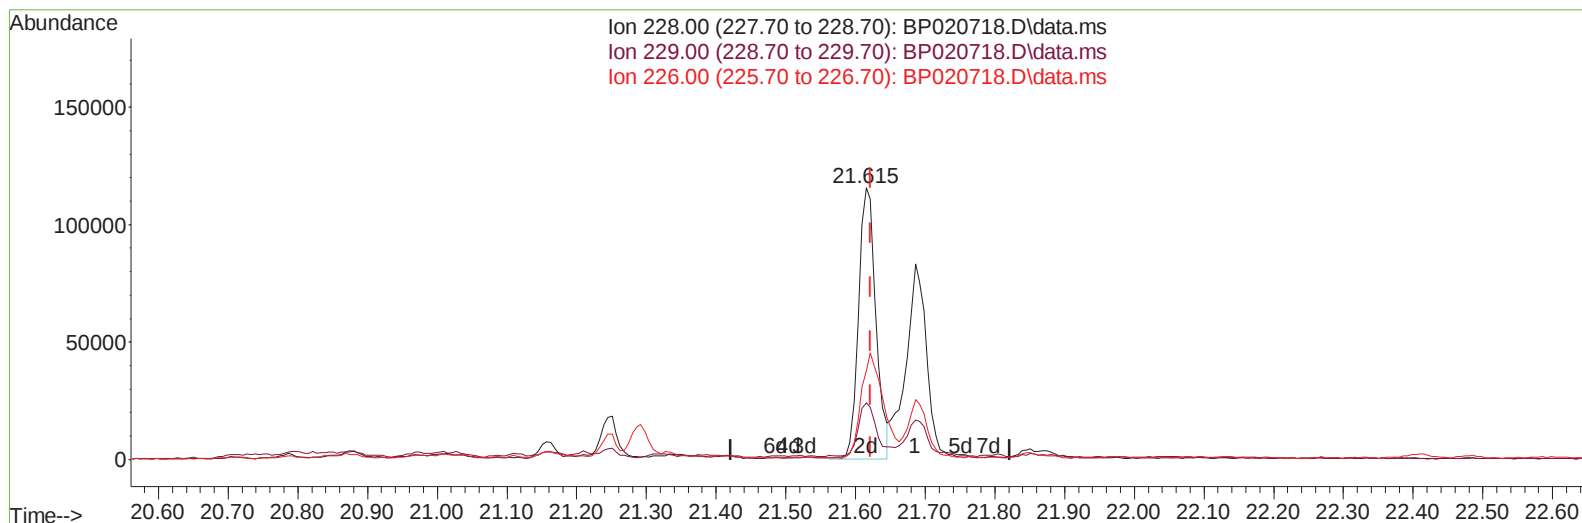

TIC: BP020718.D\data.ms

(85) Benzo(a)anthracene

21.615min (-0.006) 3.17 ng/ul m

response 198998

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	19.00	20.84
226.00	26.40	32.69#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070124\
 Data File : BP020718.D
 Acq On : 01 Jul 2024 14:46
 Operator : MA/JU
 Sample : P2897-14DL2 50X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0T61DL2

Manual IntegrationsAPPROVED

Quant Time: Jul 01 15:19:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 25 18:30:06 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/02/2024
 Supervised By :mohammad ahmed 07/04/2024

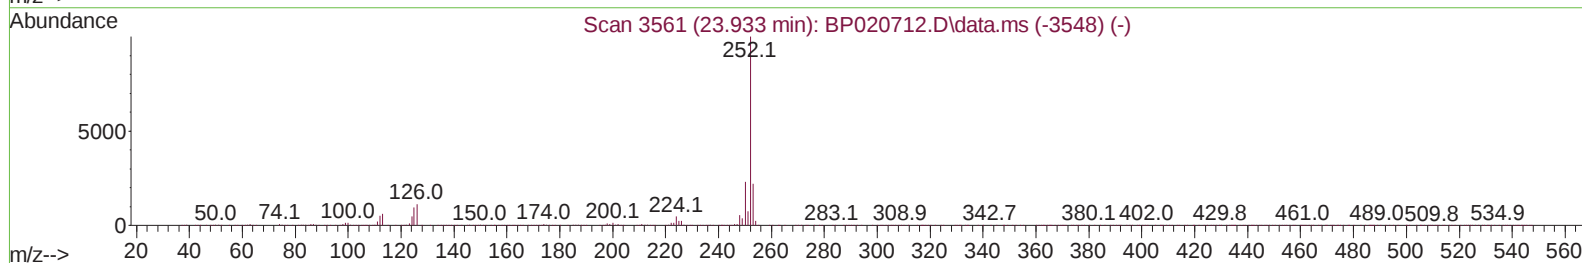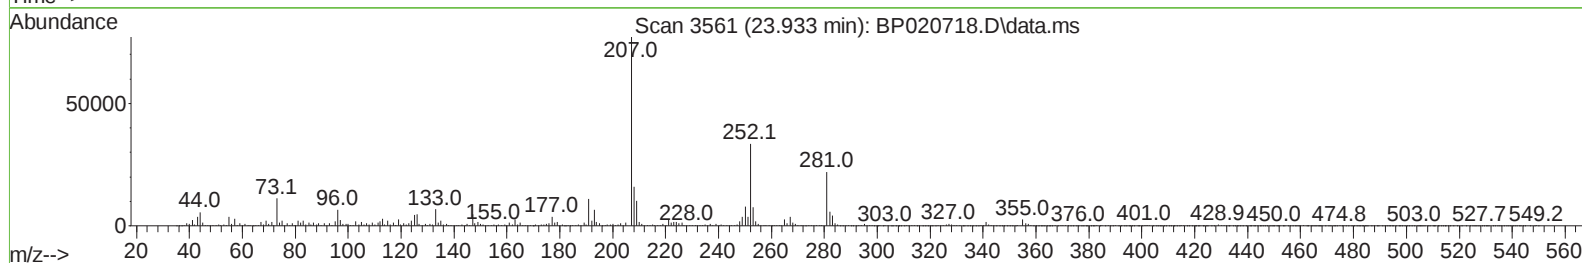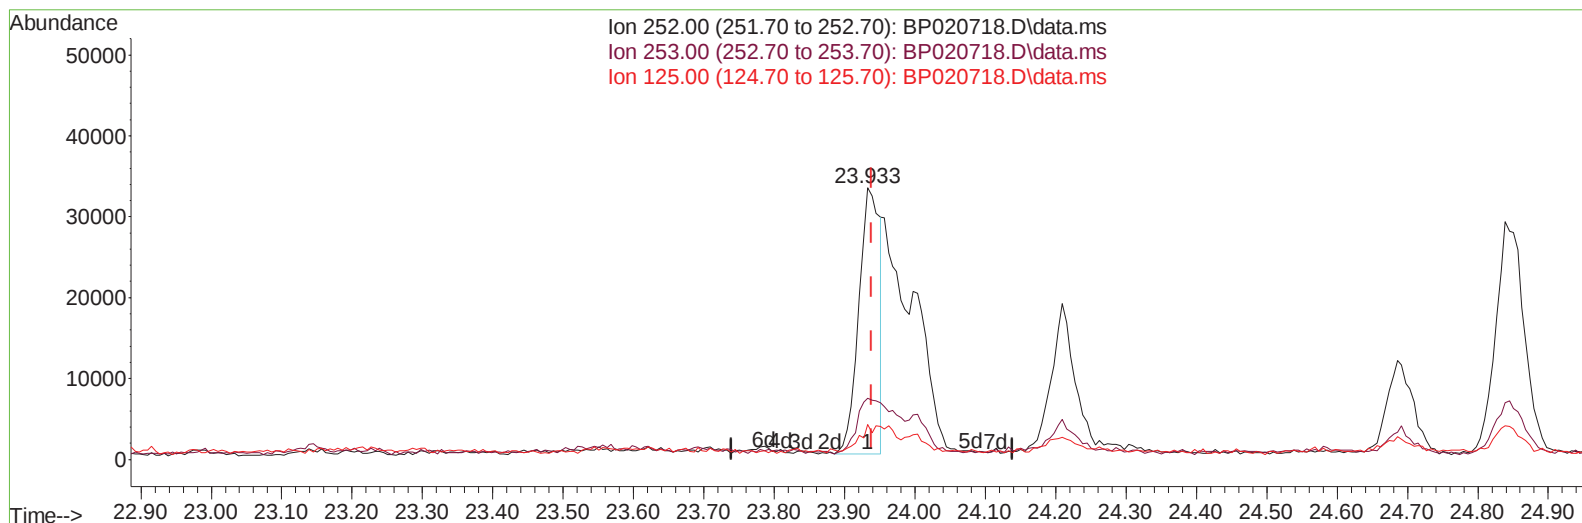

TIC: BP020718.D\data.ms

(90) Benzo(b)fluoranthene

23.933min (-0.006) 1.01 ng/u1

response 67882

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.90	22.43
125.00	9.90	12.92#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070124\
 Data File : BP020718.D
 Acq On : 01 Jul 2024 14:46
 Operator : MA/JU
 Sample : P2897-14DL2 50X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0T61DL2

Manual IntegrationsAPPROVED

Quant Time: Jul 01 15:19:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 25 18:30:06 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/02/2024
 Supervised By :mohammad ahmed 07/04/2024

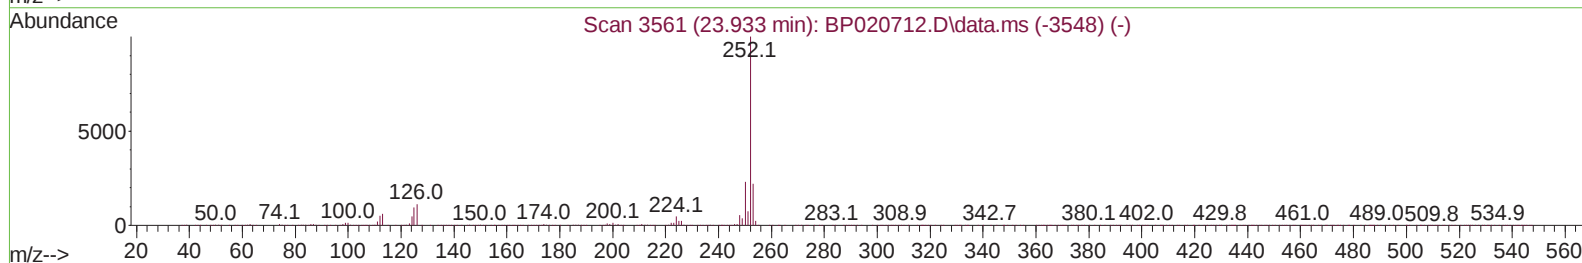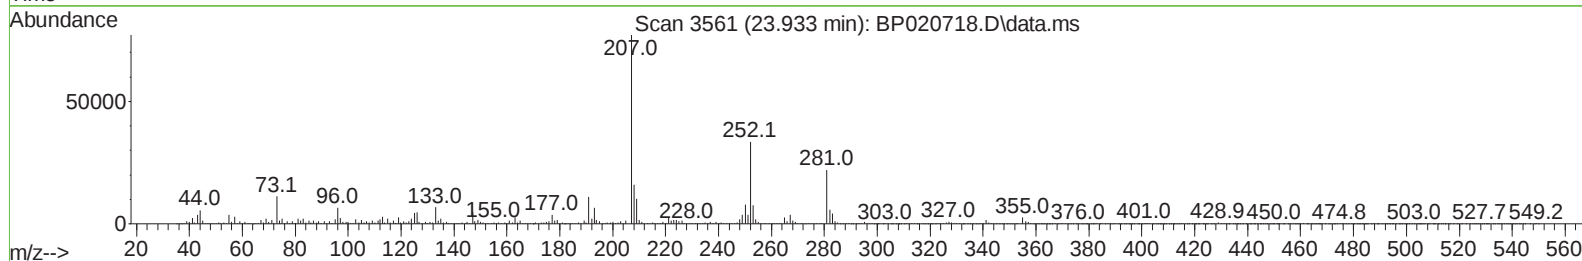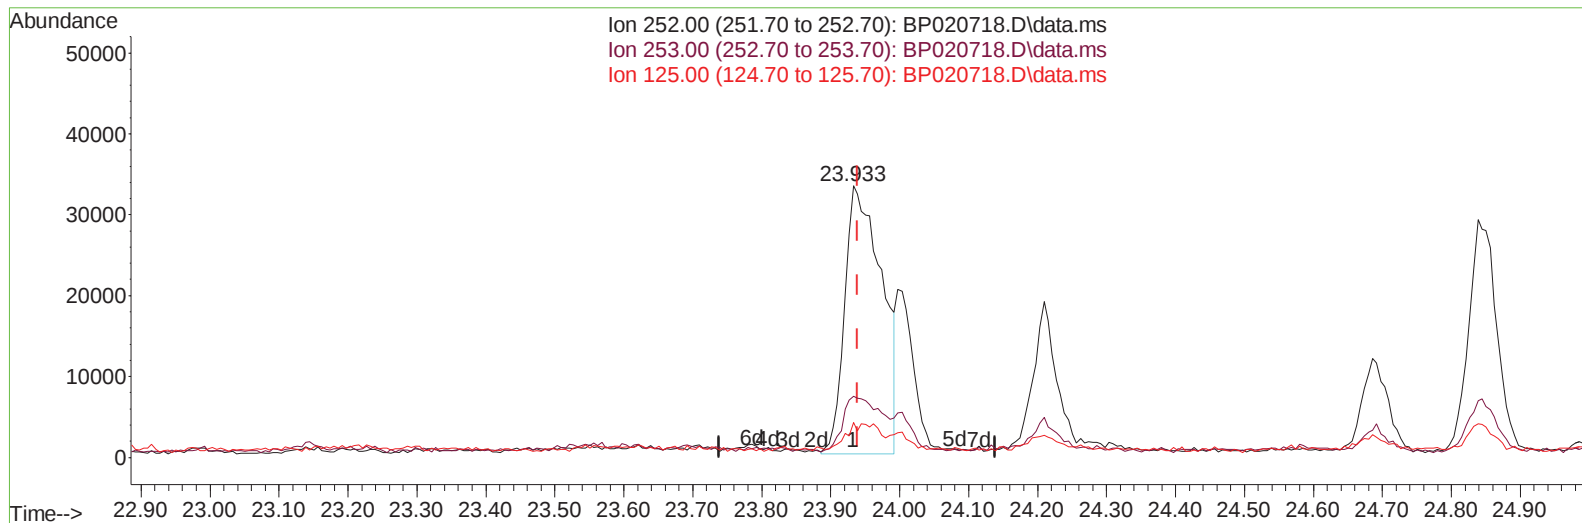

TIC: BP020718.D\data.ms

(90) Benzo(b)fluoranthene

23.933min (-0.006) 1.84 ng/ul m

response 123622

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.90	22.43
125.00	9.90	12.92#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070124\
Data File : BP020718.D
Acq On : 01 Jul 2024 14:46
Operator : MA/JU
Sample : P2897-14DL2 50X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0T61DL2

Manual IntegrationsAPPROVED

Quant Time: Jul 02 01:14:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 25 18:30:06 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/02/2024
Supervised By :mohammad ahmed 07/04/2024

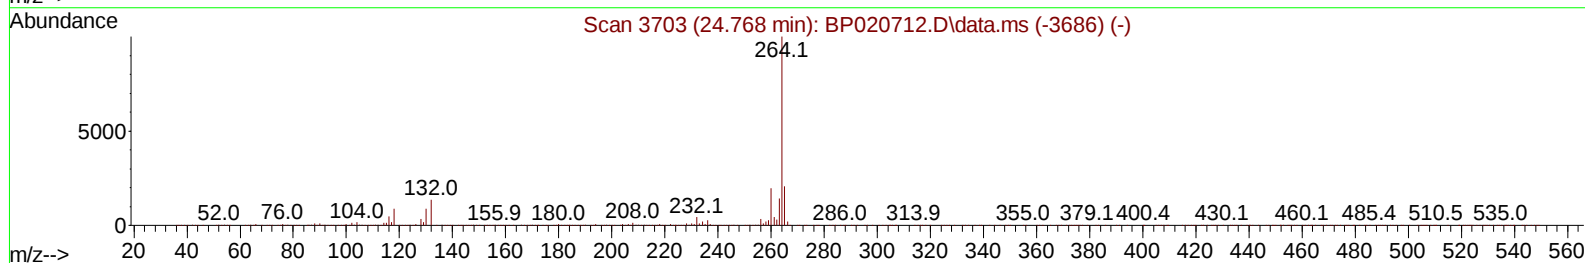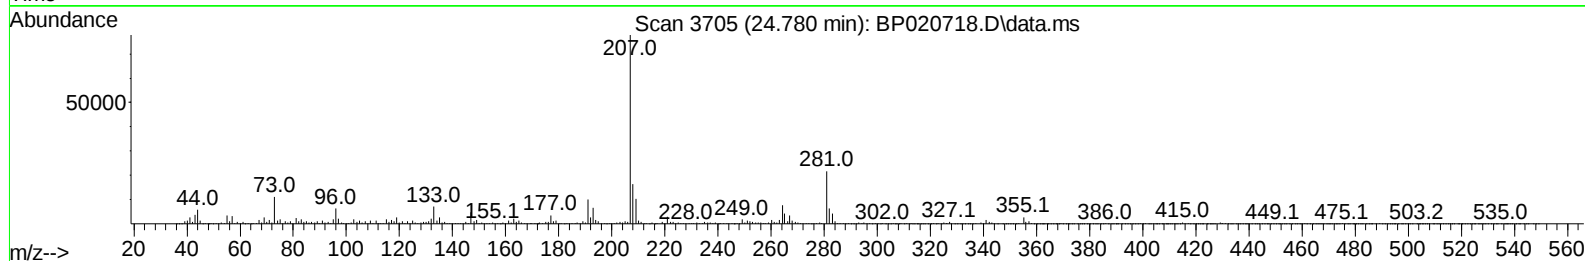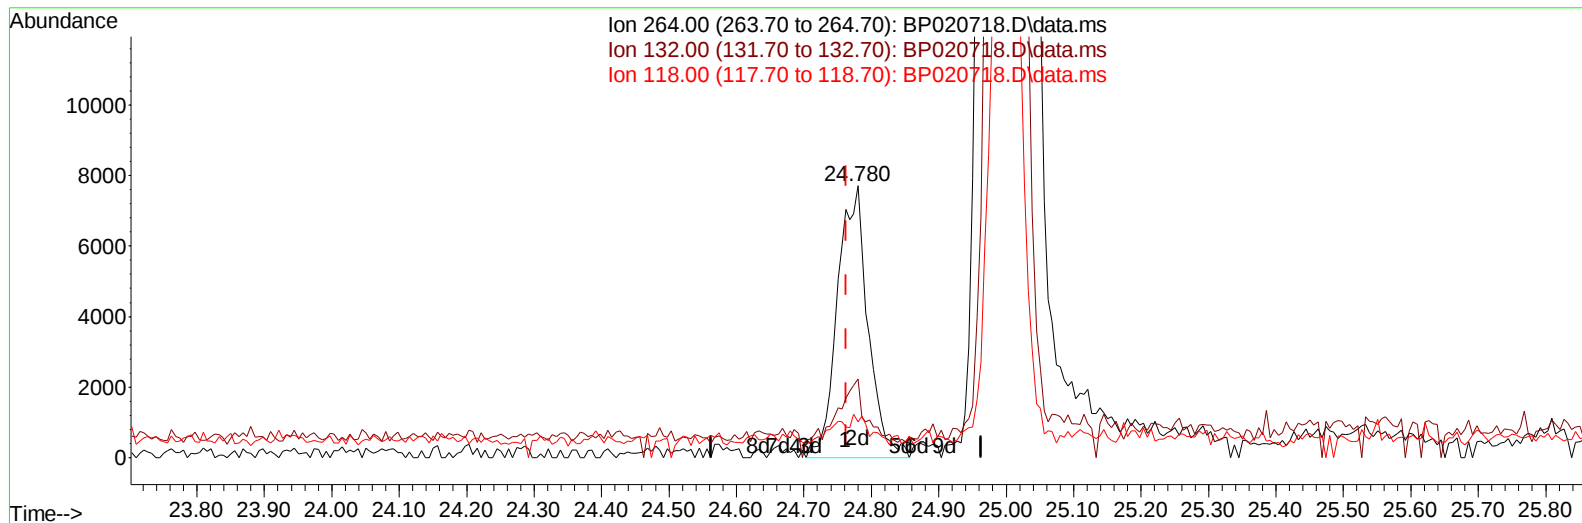

TIC: BP020718.D\data.ms

(92) Benzo(a)pyrene-d12 (S)

24.780min (+ 0.017) 0.45 ng/ul m

response 24141

Ion	Exp%	Act%
264.00	100.00	100.00
132.00	15.50	28.85#
118.00	9.80	13.09#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070124\
Data File : BP020718.D
Acq On : 01 Jul 2024 14:46
Operator : MA/JU
Sample : P2897-14DL2 50X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COT61DL2

Manual IntegrationsAPPROVED

Quant Time: Jul 01 15:22:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 25 18:30:06 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/02/2024
Supervised By :mohammad ahmed 07/04/2024

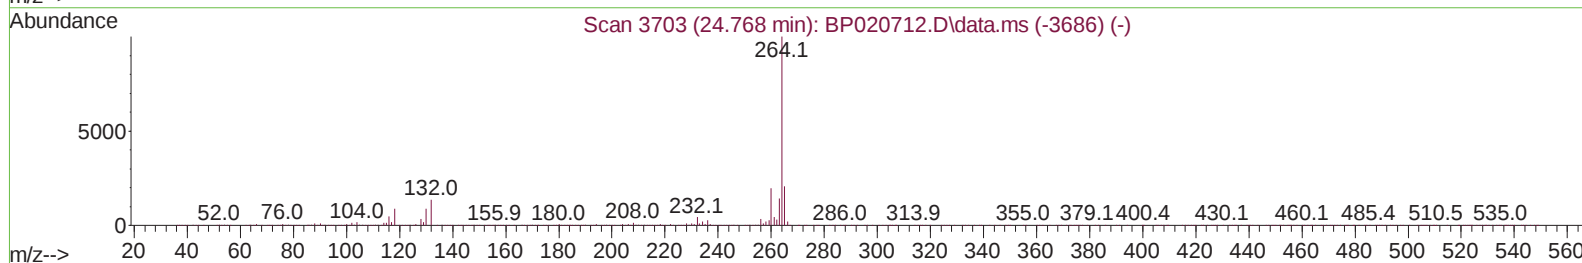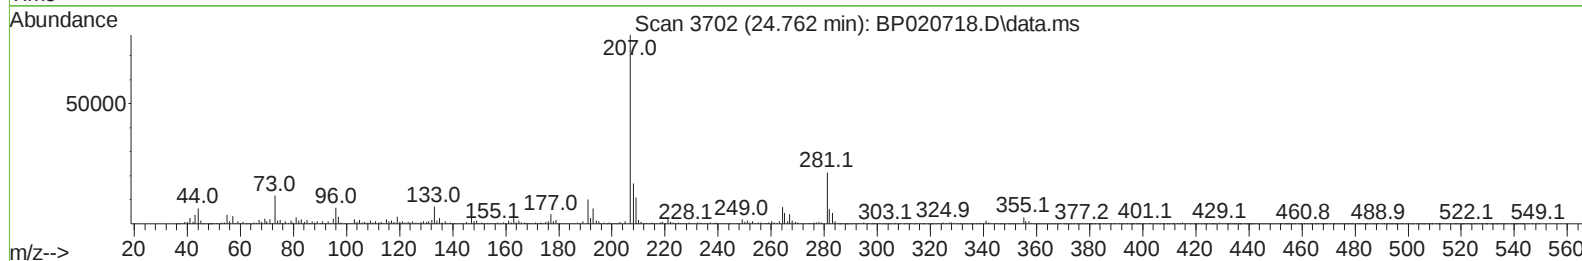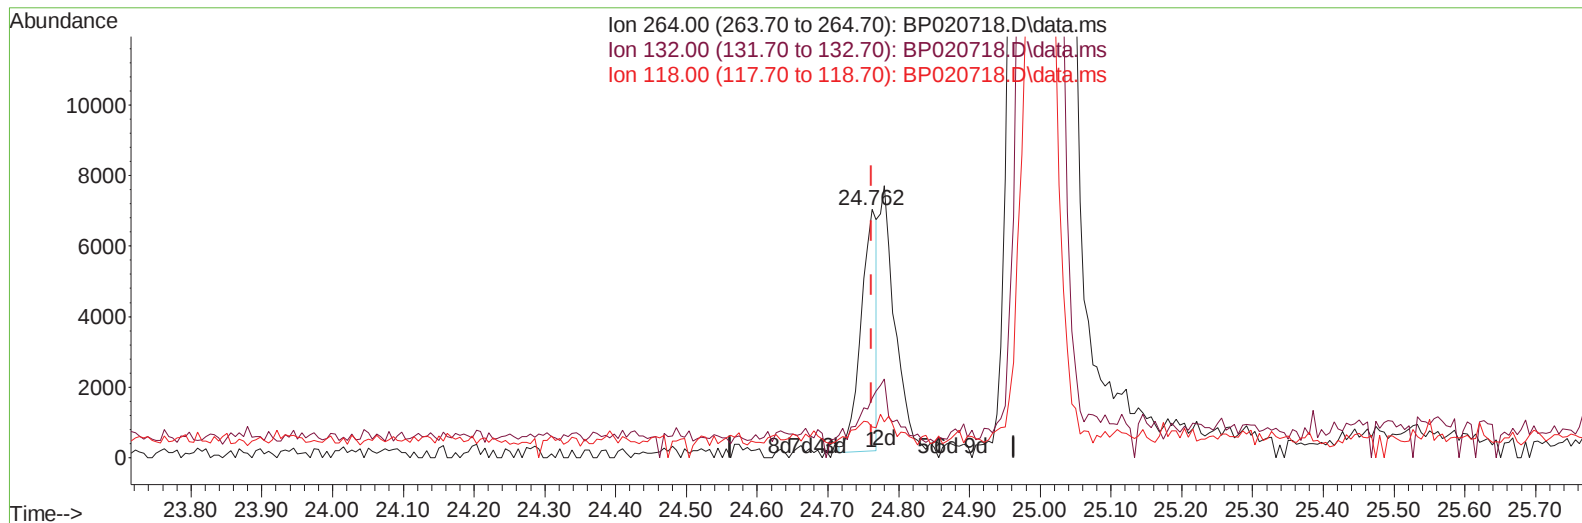

TIC: BP020718.D\data.ms

(92) Benzo(a)pyrene-d12 (S)

24.762min (-0.000) 0.20 ng/u1

response 10820

Ion	Exp%	Act%
264.00	100.00	100.00
132.00	15.50	24.00#
118.00	9.80	12.20#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070124\
 Data File : BP020718.D
 Acq On : 01 Jul 2024 14:46
 Operator : MA/JU
 Sample : P2897-14DL2 50X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0T61DL2

Manual IntegrationsAPPROVED

Quant Time: Jul 02 01:14:59 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 25 18:30:06 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/02/2024
 Supervised By :mohammad ahmed 07/04/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.740	152		225370	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.510	136		928650	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.369	164		573211	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.186	188		1049445	20.000	ng/ul	0.00
79) Chrysene-d12	21.639	240		894395	20.000	ng/ul	0.00
88) Perylene-d12	25.003	264		1110080	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	0.000	96		0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84		0d	0.000	ng/ul	
7) Phenol-d5	6.928	99		8975	0.486	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.081	67		6385	0.545	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.287	132		8061	0.534	ng/ul	0.00
15) 4-Methylphenol-d8	8.445	113		6445	0.429	ng/ul	0.00
21) Nitrobenzene-d5	8.893	128		3782	0.552	ng/ul	0.00
24) 2-Nitrophenol-d4	9.598	143		3707	0.540	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.145	165		6683	0.473	ng/ul	0.00
31) 4-Chloroaniline-d4	10.657	131		5413m	0.273	ng/ul	0.00
46) Dimethylphthalate-d6	13.775	166		27813	0.698	ng/ul	0.00
49) Acenaphthylene-d8	14.057	160		29358	0.617	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143		0d	0.000	ng/ul	
60) Fluorene-d10	15.380	176		23293	0.695	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200		0d	0.000	ng/ul	
73) Anthracene-d10	17.280	188		32002	0.679	ng/ul	0.00
81) Pyrene-d10	19.663	212		28922	0.538	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.780	264		24141m	0.447	ng/ul	0.02
Target Compounds							
						Qvalue	
30) Naphthalene	10.563	128		2731436	54.953	ng/ul	99
36) 2-Methylnaphthalene	12.169	142		950752	28.555	ng/ul	98
37) 1-Methylnaphthalene	12.392	142		581259	17.077	ng/ul	100
43) 1,1'-Biphenyl	13.186	154		129754	3.027	ng/ul	98
50) Acenaphthylene	14.086	152		114621	2.134	ng/ul#	91
52) Acenaphthene	14.428	153		366301	10.279	ng/ul	99
61) Fluorene	15.433	166		259450	6.725	ng/ul	98
72) Phenanthrene	17.227	178		1122879	20.433	ng/ul	100
74) Anthracene	17.316	178		289347	5.119	ng/ul	99
80) Fluoranthene	19.315	202		369325	5.627	ng/ul	99
82) Pyrene	19.692	202		469610	6.977	ng/ul	98
85) Benzo(a)anthracene	21.615	228		198998m	3.174	ng/ul	
87) Chrysene	21.686	228		166733	2.814	ng/ul	99
90) Benzo(b)fluoranthene	23.933	252		123622m	1.838	ng/ul	
93) Benzo(a)pyrene	24.839	252		80139	1.262	ng/ul#	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070124\
Data File : BP020718.D
Acq On : 01 Jul 2024 14:46
Operator : MA/JU
Sample : P2897-14DL2 50X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0T61DL2

Manual IntegrationsAPPROVED

Quant Time: Jul 02 01:14:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 25 18:30:06 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/02/2024
Supervised By :mohammad ahmed 07/04/2024

