

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070124\
 Data File : BP020734.D
 Acq On : 02 Jul 2024 02:17
 Operator : MA/JU
 Sample : P2962-09
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COT81

Quant Time: Jul 02 03:06:53 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 25 18:30:06 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.740	152	244163	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.504	136	959618	20.000	ng/u1	-0.02
38) Acenaphthene-d10	14.363	164	567654	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.180	188	1023567	20.000	ng/u1	0.00
79) Chrysene-d12	21.627	240	966839	20.000	ng/u1	-0.01
88) Perylene-d12	24.992	264	1147414	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	17957	3.158	ng/uL	0.00
4) Pyridine-d5	3.687	84	102908	6.210	ng/u1	0.00
7) Phenol-d5	6.916	99	375214	18.736	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.081	67	236501	18.629	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.275	132	313527	19.156	ng/u1	-0.01
15) 4-Methylphenol-d8	8.440	113	317719	19.534	ng/u1	0.00
21) Nitrobenzene-d5	8.893	128	156629	22.108	ng/u1	0.00
24) 2-Nitrophenol-d4	9.604	143	171554	24.197	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.134	165	298259	20.423	ng/u1	0.00
31) 4-Chloroaniline-d4	10.651	131	370012	18.079	ng/u1	0.00
46) Dimethylphthalate-d6	13.775	166	997074	25.263	ng/u1	0.00
49) Acenaphthylene-d8	14.051	160	1051302	22.323	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.592	143	111032	18.412	ng/u1	0.00
60) Fluorene-d10	15.381	176	779101	23.458	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.510	200	98253	19.048	ng/u1	0.00
73) Anthracene-d10	17.280	188	1120762	24.397	ng/u1	0.00
81) Pyrene-d10	19.669	212	1293129	22.263	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.751	264	1436833	25.743	ng/u1	-0.01
Target Compounds						
					Qvalue	
30) Naphthalene	10.557	128	409094	7.965	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070124\
Data File : BP020734.D
Acq On : 02 Jul 2024 02:17
Operator : MA/JU
Sample : P2962-09
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0T81

Quant Time: Jul 02 03:06:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 25 18:30:06 2024
Response via : Initial Calibration

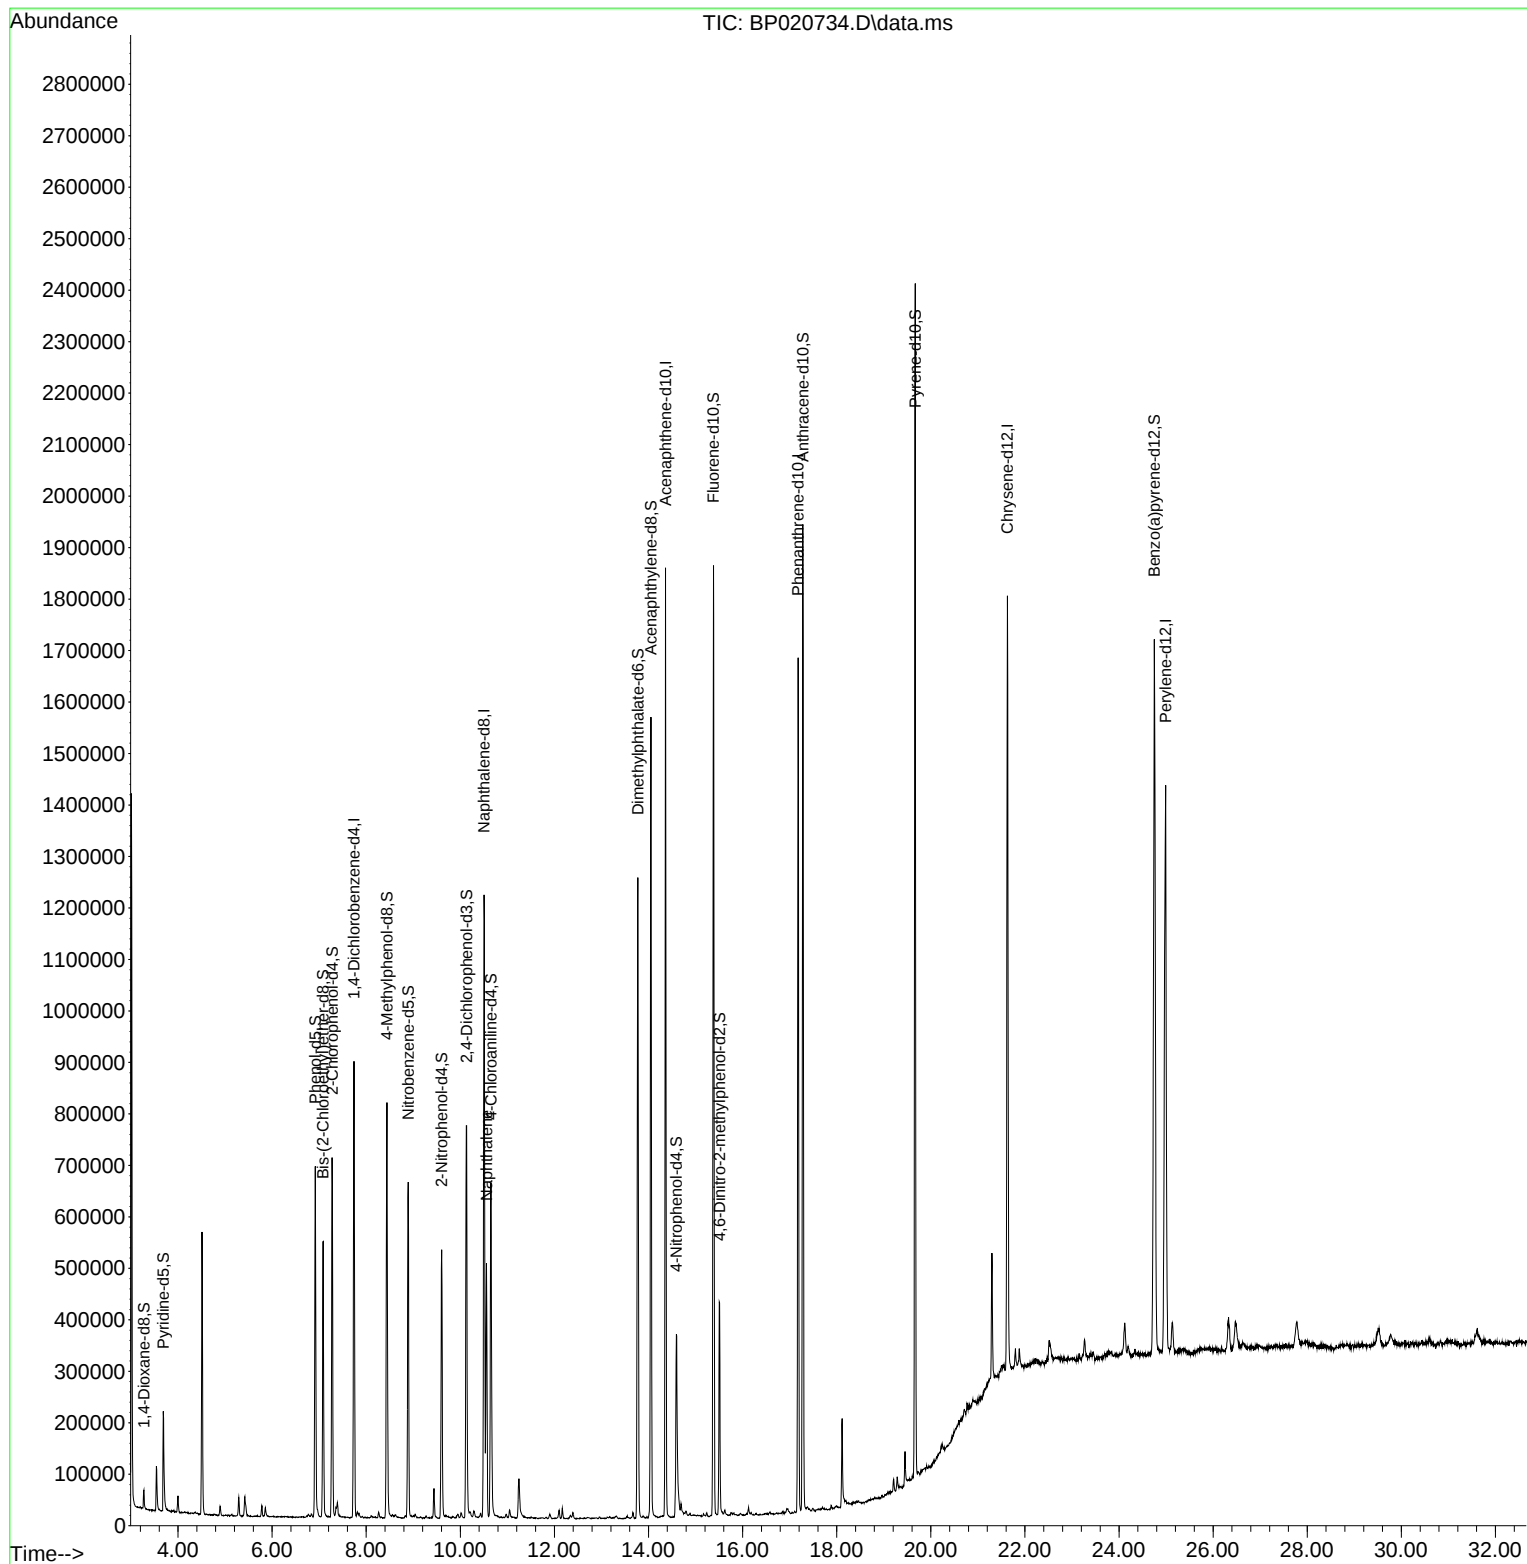

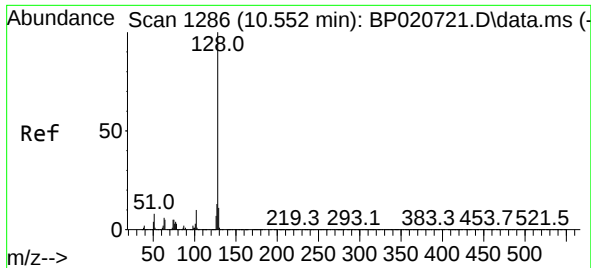

#30
Naphthalene
Concen: 7.965 ng/ul
RT: 10.557 min Scan# 11
Delta R.T. -0.012 min
Lab File: BP020734.D
Acq: 02 Jul 2024 02:17

Instrument :
BNA_P
ClientSampleId :
C0T81

Tgt Ion:128 Resp: 409094
Ion Ratio Lower Upper
128 100
129 10.7 8.7 13.1
127 13.5 10.6 15.8

