

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070124\
 Data File : BP020713.D
 Acq On : 01 Jul 2024 10:56
 Operator : MA/JU
 Sample : PB161602BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK602

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020713.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	43	47	55	rVB	54830	78714	1.75%	0.149%
2	3.670	113	116	136	rBV	784074	1134397	25.22%	2.140%
3	3.987	165	170	178	rVB	14509	22178	0.49%	0.042%
4	6.905	659	666	681	rBV	922820	1426667	31.71%	2.692%
5	7.069	687	694	704	rVB	710562	1098681	24.42%	2.073%
6	7.263	718	727	738	rBV	923245	1443213	32.08%	2.723%
7	7.722	797	805	815	rBV	690422	1205597	26.80%	2.274%
8	8.428	917	925	938	rBV	1108888	1852876	41.19%	3.496%
9	8.516	938	940	946	rVB7	3482	5593	0.12%	0.011%
10	8.875	991	1001	1014	rBV	879330	1487308	33.06%	2.806%
11	9.587	1113	1122	1133	rBV	741654	1261786	28.05%	2.381%
12	10.122	1205	1213	1222	rBV	1166408	1944964	43.24%	3.669%
13	10.222	1229	1230	1236	rVB6	5842	5180	0.12%	0.010%
14	10.499	1269	1277	1287	rBV	1190525	1849631	41.12%	3.490%
15	10.634	1292	1300	1320	rBV	1039704	2013685	44.76%	3.799%
16	12.093	1541	1548	1556	rBV2	16886	35454	0.79%	0.067%
17	13.322	1753	1757	1763	rVB4	4000	6244	0.14%	0.012%
18	13.775	1826	1834	1848	rBV	2164507	2981725	66.28%	5.625%
19	14.057	1874	1882	1894	rBV	2377091	3555861	79.04%	6.709%
20	14.369	1927	1935	1944	rBV	1889302	2616567	58.16%	4.936%
21	14.592	1966	1973	1979	rBV	667635	1085844	24.14%	2.049%
22	14.734	1992	1997	2003	rVB9	5177	11131	0.25%	0.021%
23	14.881	2018	2022	2026	rVB7	2745	4525	0.10%	0.009%
24	15.381	2100	2107	2122	rBV	3029065	4325514	96.15%	8.161%
25	15.504	2122	2128	2145	rVV	639119	1089889	24.23%	2.056%
26	15.628	2145	2149	2157	rVB3	16275	28004	0.62%	0.053%
27	16.186	2240	2244	2249	rVB5	8211	12056	0.27%	0.023%
28	16.857	2354	2358	2365	rVB8	6279	9389	0.21%	0.018%
29	16.969	2373	2377	2382	rBV4	4205	6825	0.15%	0.013%
30	17.192	2407	2415	2421	rBV	2101529	2984652	66.35%	5.631%
31	17.286	2424	2431	2450	rVB2	2842602	4498541	100.00%	8.487%
32	17.881	2529	2532	2534	rBV3	5665	7241	0.16%	0.014%
33	18.133	2570	2575	2576	rBV5	7380	9082	0.20%	0.017%
34	19.216	2755	2759	2765	rBV2	36236	53978	1.20%	0.102%
35	19.292	2769	2772	2778	rVB	28484	41566	0.92%	0.078%
36	19.675	2830	2837	2845	rBV	2772280	4416123	98.17%	8.332%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070124\
Data File : BP020713.D
Acq On : 01 Jul 2024 10:56
Operator : MA/JU
Sample : PB161602BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK602

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Title : SVOA CALIBRATION

37	21.651	3167	3173	3183	rVB2	1312079	2241189	49.82%	4.228%
38	24.792	3699	3707	3720	rVB2	1527619	3773888	83.89%	7.120%
39	25.015	3737	3745	3760	rVB	809581	2379277	52.89%	4.489%




Sum of corrected areas: 53005035

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070124\
Data File : BP020713.D
Acq On : 01 Jul 2024 10:56
Operator : MA/JU
Sample : PB161602BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK602

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

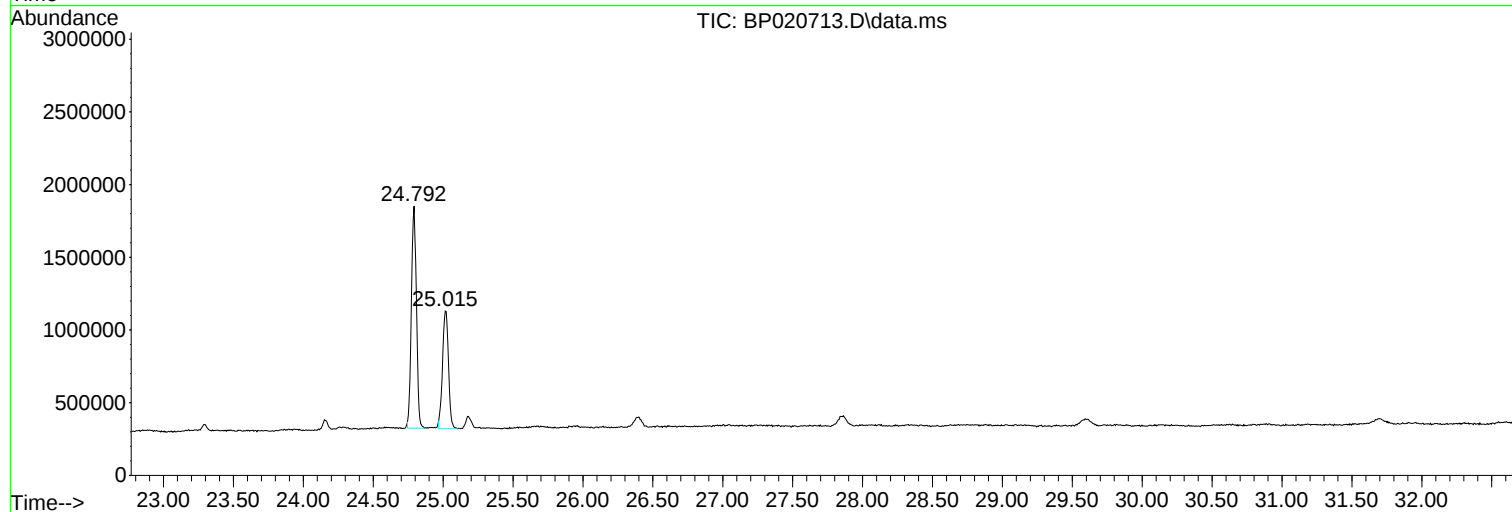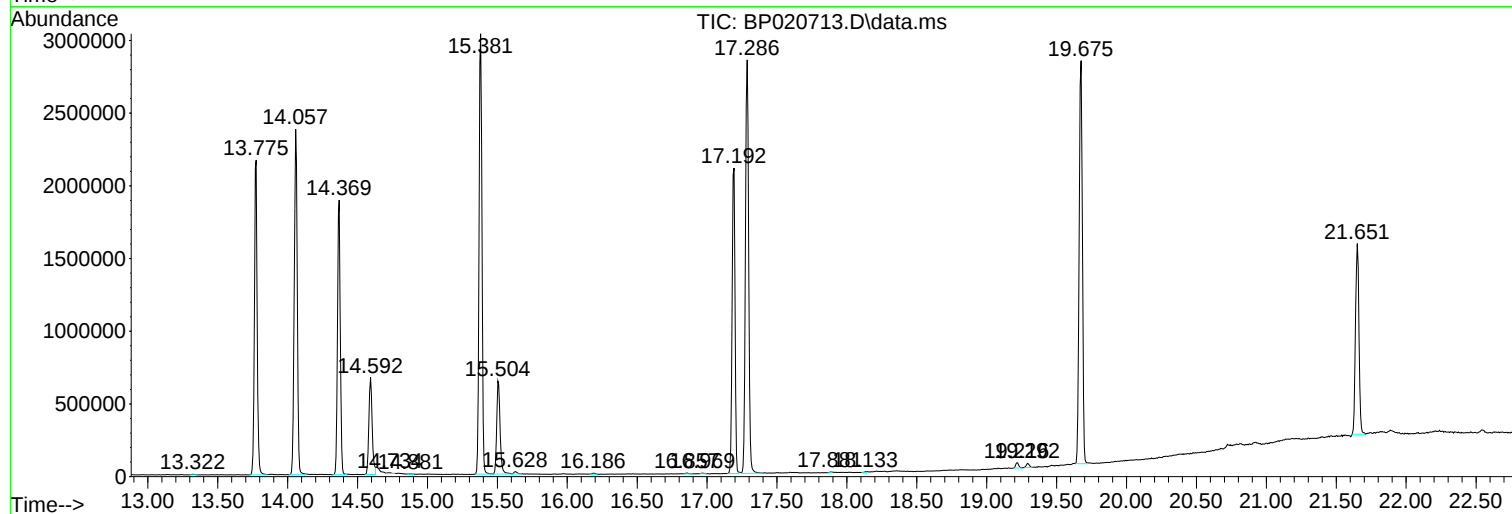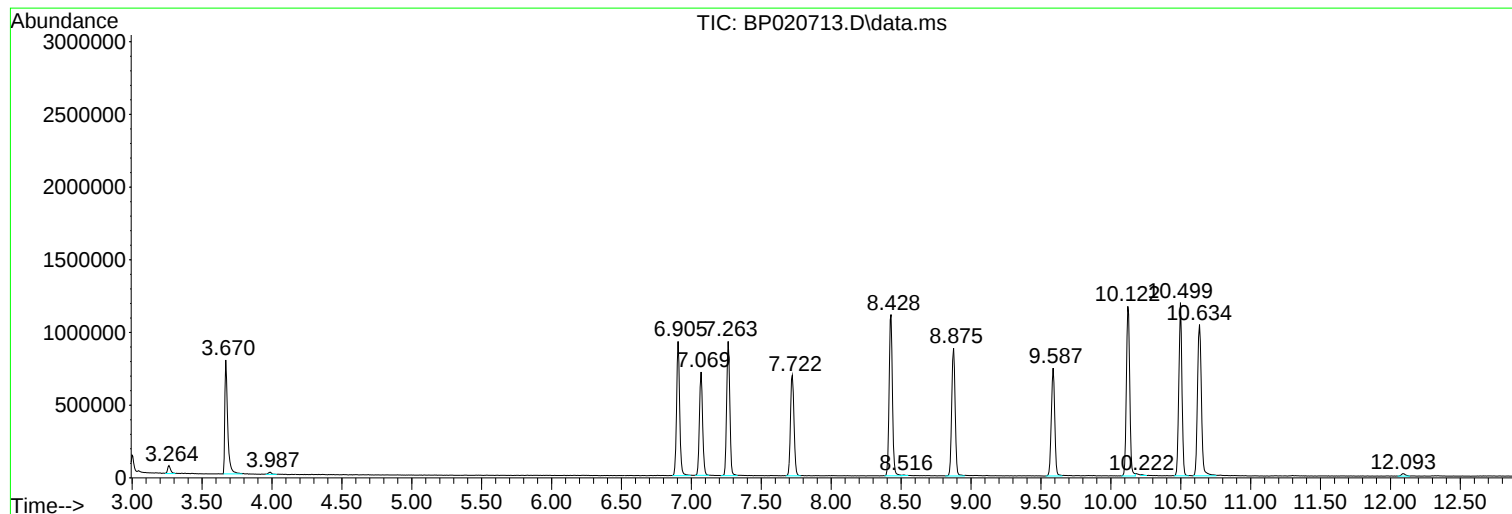

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070124\
Data File : BP020713.D
Acq On : 01 Jul 2024 10:56
Operator : MA/JU
Sample : PB161602BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK602

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070124\
Data File : BP020713.D
Acq On : 01 Jul 2024 10:56
Operator : MA/JU
Sample : PB161602BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK602

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------