

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070124\
 Data File : BP020737.D
 Acq On : 02 Jul 2024 05:09
 Operator : MA/JU
 Sample : PB161640BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK640

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020737.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	45	49	53	rBV	67253	84739	1.78%	0.158%
2	3.681	115	118	142	rBV	907539	1341550	28.13%	2.496%
3	3.999	168	172	177	rVB	15977	23633	0.50%	0.044%
4	6.922	662	669	679	rBV	1015186	1651939	34.64%	3.073%
5	7.087	690	697	709	rVB	851283	1318701	27.65%	2.453%
6	7.281	722	730	741	rBV	1089206	1708316	35.82%	3.178%
7	7.740	800	808	818	rVB	832140	1373872	28.81%	2.556%
8	8.440	919	927	941	rBV	1185899	2081291	43.64%	3.872%
9	8.893	995	1004	1018	rBV	941793	1666678	34.95%	3.100%
10	9.605	1117	1125	1139	rBV	855936	1410172	29.57%	2.623%
11	10.134	1207	1215	1238	rBV	1144791	2088364	43.79%	3.885%
12	10.505	1270	1278	1290	rVB	1046548	1904949	39.94%	3.544%
13	10.652	1294	1303	1320	rBV	1153870	2074882	43.51%	3.860%
14	11.328	1410	1418	1421	rBV9	2551	6236	0.13%	0.012%
15	12.110	1544	1551	1557	rBV2	18229	33576	0.70%	0.062%
16	13.316	1752	1756	1759	rBV5	3231	4944	0.10%	0.009%
17	13.781	1827	1835	1850	rBV	1730480	2816670	59.06%	5.240%
18	14.057	1873	1882	1900	rBV2	1995183	3331480	69.86%	6.197%
19	14.375	1928	1936	1948	rBV	1519429	2303279	48.30%	4.285%
20	14.598	1967	1974	1988	rBV	496033	1042857	21.87%	1.940%
21	14.698	1988	1991	1995	rVB5	11147	15704	0.33%	0.029%
22	15.387	2101	2108	2123	rBV	2813823	3867815	81.10%	7.195%
23	15.510	2123	2129	2144	rVV	548015	927942	19.46%	1.726%
24	15.634	2146	2150	2155	rVB2	10767	16464	0.35%	0.031%
25	16.187	2241	2244	2248	rVB5	8098	9641	0.20%	0.018%
26	16.851	2353	2357	2362	rVB7	4216	7657	0.16%	0.014%
27	17.187	2407	2414	2423	rBV	1548422	2367685	49.65%	4.404%
28	17.287	2424	2431	2443	rVV	2531215	3822585	80.16%	7.111%
29	17.881	2529	2532	2539	rBV9	4371	9022	0.19%	0.017%
30	18.122	2570	2573	2577	rBV5	5464	7213	0.15%	0.013%
31	19.216	2755	2759	2764	rBV3	34223	48700	1.02%	0.091%
32	19.292	2768	2772	2775	rVV	28191	38813	0.81%	0.072%
33	19.669	2830	2836	2844	rBV	3091327	4306337	90.30%	8.011%
34	21.633	3164	3170	3184	rVB2	1404225	2509636	52.62%	4.668%
35	24.768	3692	3703	3717	rVB2	1730124	4768939	100.00%	8.871%
36	24.992	3732	3741	3753	rVB	958341	2765134	57.98%	5.144%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070124\
Data File : BP020737.D
Acq On : 02 Jul 2024 05:09
Operator : MA/JU
Sample : PB161640BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK640

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 53757415

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070124\
Data File : BP020737.D
Acq On : 02 Jul 2024 05:09
Operator : MA/JU
Sample : PB161640BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK640

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

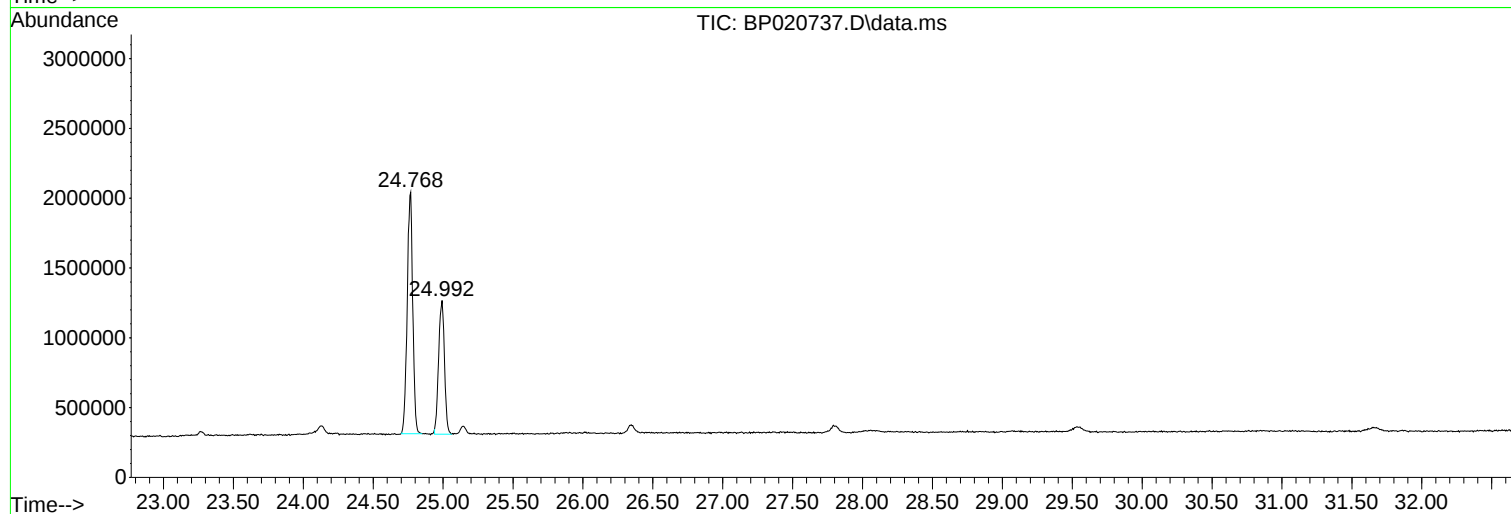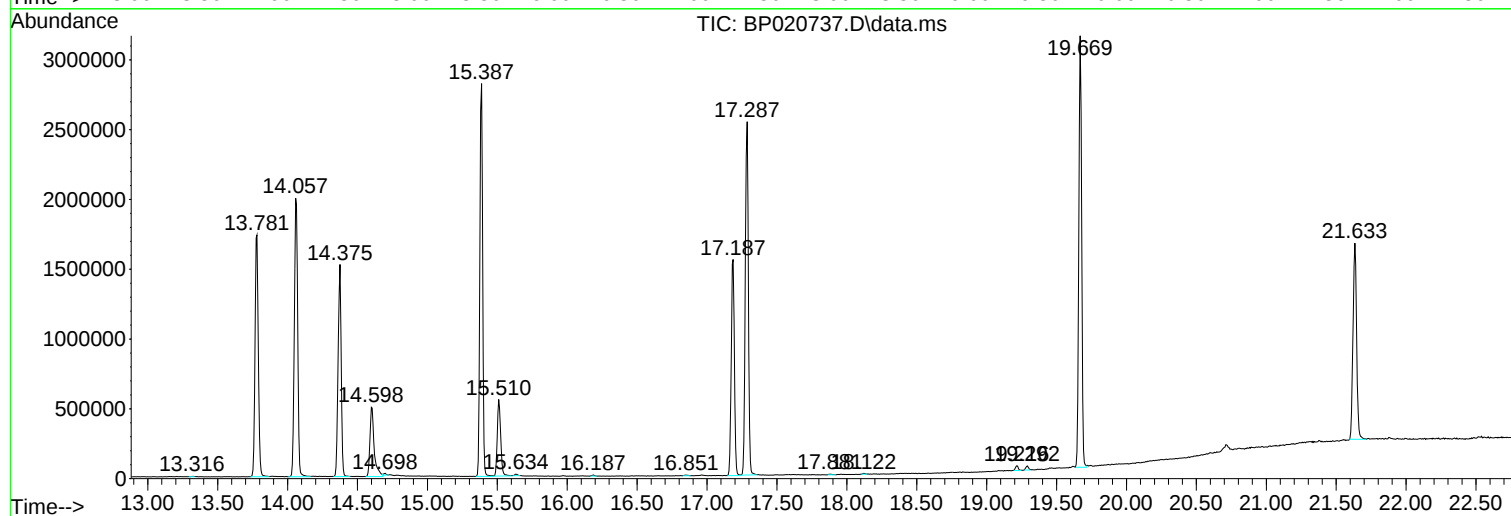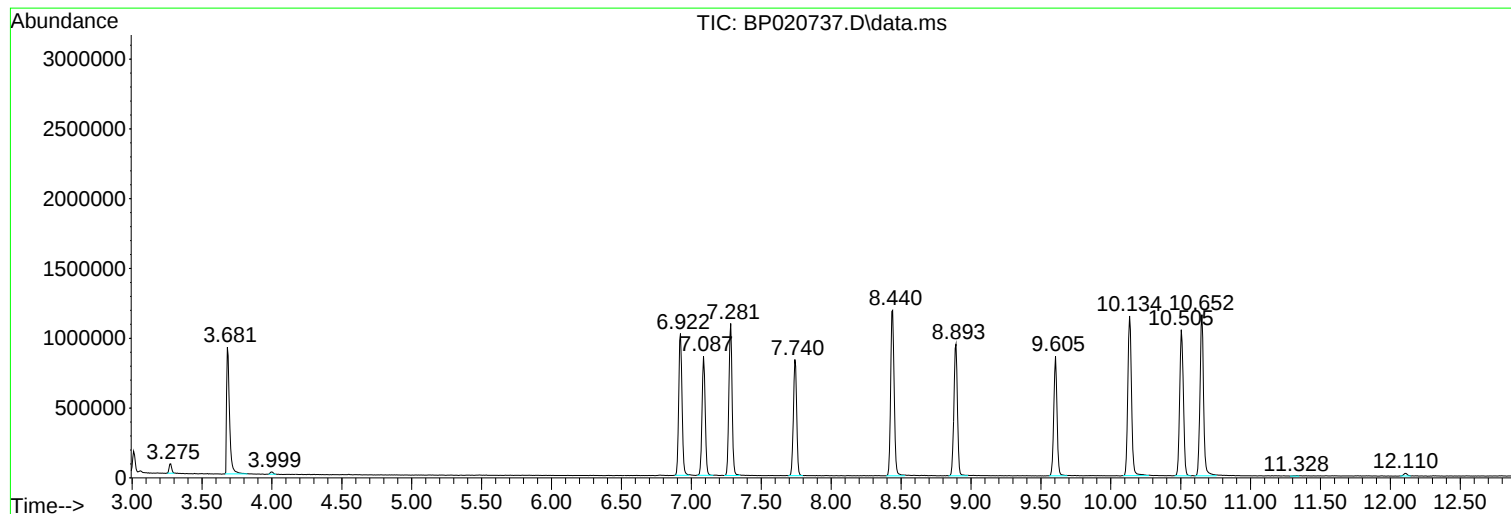

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070124\
Data File : BP020737.D
Acq On : 02 Jul 2024 05:09
Operator : MA/JU
Sample : PB161640BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK640

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070124\
Data File : BP020737.D
Acq On : 02 Jul 2024 05:09
Operator : MA/JU
Sample : PB161640BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK640

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc