

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070124\
 Data File : BP020752.D
 Acq On : 02 Jul 2024 15:51
 Operator : MA/JU
 Sample : PB161652BL
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK652

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020752.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	44	48	58	rVB	55043	77290	1.62%	0.143%
2	3.681	114	118	139	rBV	740081	1202760	25.29%	2.223%
3	3.993	167	171	181	rVB	16454	31520	0.66%	0.058%
4	6.922	662	669	686	rBV	945262	1500743	31.55%	2.774%
5	7.081	689	696	710	rVB	733865	1130024	23.76%	2.089%
6	7.281	722	730	741	rBV	945211	1524389	32.05%	2.818%
7	7.734	800	807	822	rBV	731187	1195044	25.12%	2.209%
8	8.434	917	926	939	rBV	1197421	1937691	40.74%	3.582%
9	8.887	995	1003	1015	rBV	876102	1526923	32.10%	2.822%
10	9.593	1115	1123	1139	rBV	767260	1308883	27.52%	2.419%
11	10.134	1207	1215	1227	rBV	1200126	2021568	42.50%	3.737%
12	10.510	1270	1279	1292	rBV	1174301	1805163	37.95%	3.337%
13	10.646	1292	1302	1322	rBV	1093721	2057358	43.25%	3.803%
14	11.322	1413	1417	1422	rBV8	2549	4813	0.10%	0.009%
15	12.099	1542	1549	1556	rBV	17832	35174	0.74%	0.065%
16	13.328	1753	1758	1764	rBV9	3736	7276	0.15%	0.013%
17	13.775	1827	1834	1849	rBV	2195105	2950767	62.04%	5.454%
18	14.057	1875	1882	1896	rBV	2271721	3579477	75.25%	6.616%
19	14.369	1927	1935	1943	rBV	1682580	2478778	52.11%	4.582%
20	14.593	1966	1973	1990	rBV	665666	1262769	26.55%	2.334%
21	15.381	2097	2107	2120	rBV	3058362	4380953	92.10%	8.098%
22	15.504	2123	2128	2144	rVV	728810	1055619	22.19%	1.951%
23	15.628	2144	2149	2154	rVB	14089	23899	0.50%	0.044%
24	16.087	2224	2227	2235	rVB10	3947	8067	0.17%	0.015%
25	16.181	2239	2243	2251	rVB7	7773	13144	0.28%	0.024%
26	16.851	2353	2357	2361	rVB6	5635	8479	0.18%	0.016%
27	16.963	2373	2376	2382	rVB6	5841	8801	0.19%	0.016%
28	17.181	2405	2413	2420	rBV	1985421	2841907	59.75%	5.253%
29	17.281	2423	2430	2446	rVB	3191509	4659538	97.96%	8.613%
30	18.134	2570	2575	2580	rBV8	6932	18703	0.39%	0.035%
31	19.216	2754	2759	2766	rVB2	40134	60431	1.27%	0.112%
32	19.292	2768	2772	2777	rVV2	29144	43393	0.91%	0.080%
33	19.669	2829	2836	2844	rBV	3145767	4756581	100.00%	8.792%
34	21.639	3165	3171	3180	rBV	1398441	2256765	47.45%	4.171%
35	24.769	3693	3703	3715	rVB3	1437299	3905694	82.11%	7.219%
36	24.992	3734	3741	3757	rVB	852644	2421145	50.90%	4.475%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070124\
Data File : BP020752.D
Acq On : 02 Jul 2024 15:51
Operator : MA/JU
Sample : PB161652BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK652

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 54101529

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070124\
Data File : BP020752.D
Acq On : 02 Jul 2024 15:51
Operator : MA/JU
Sample : PB161652BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK652

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

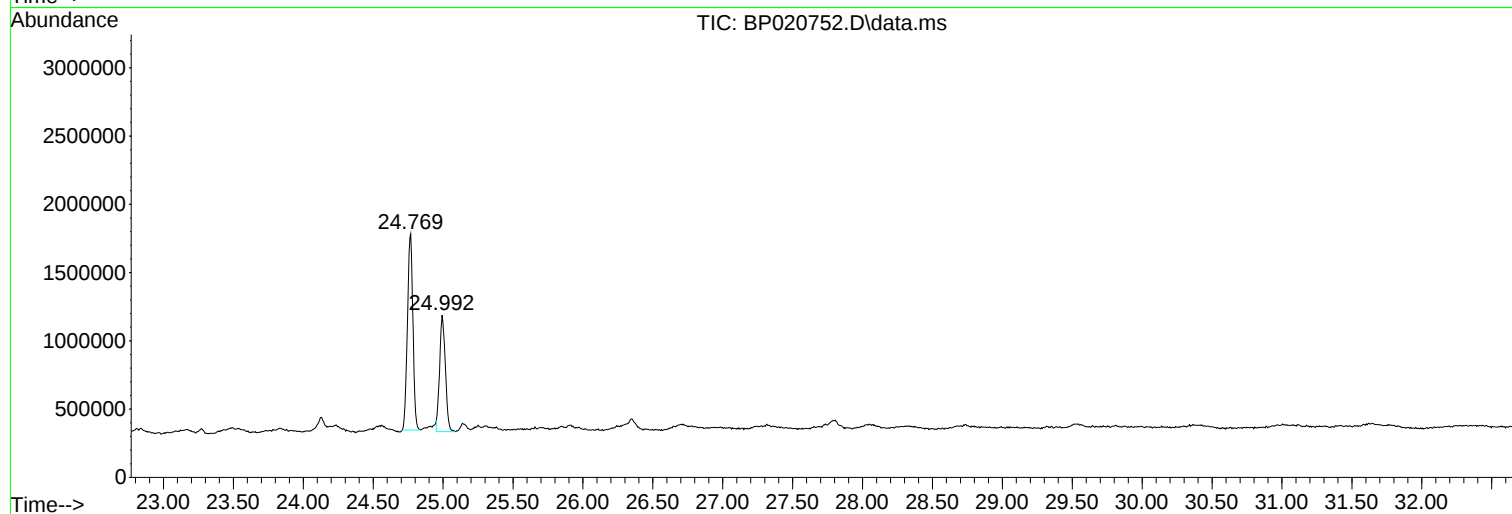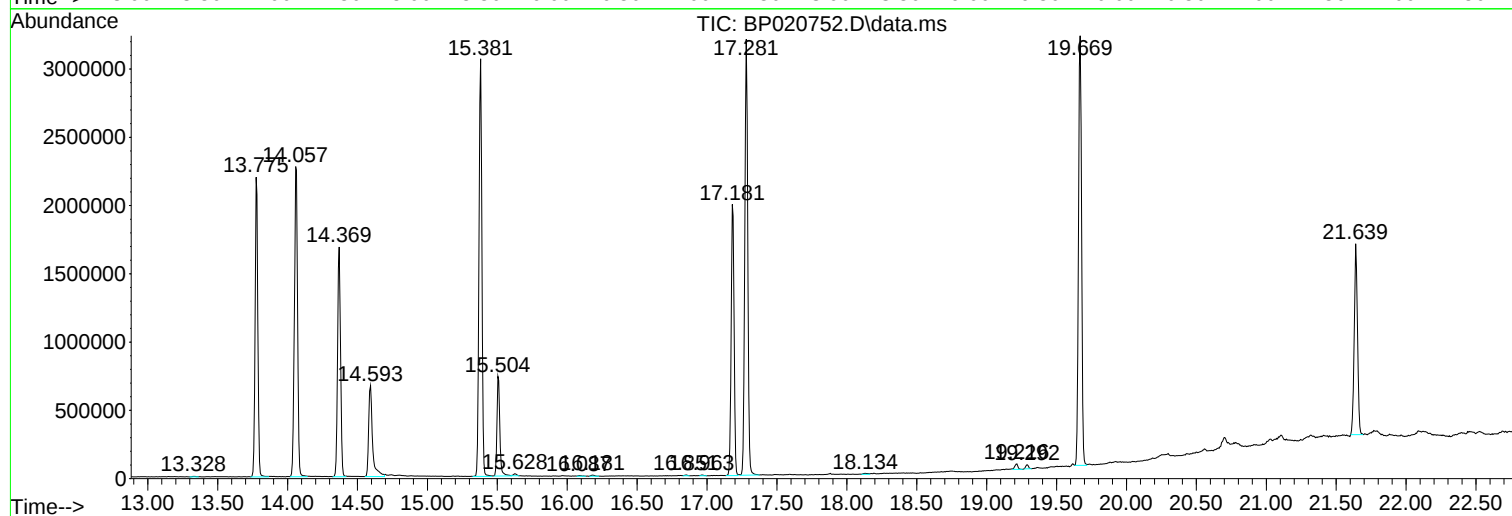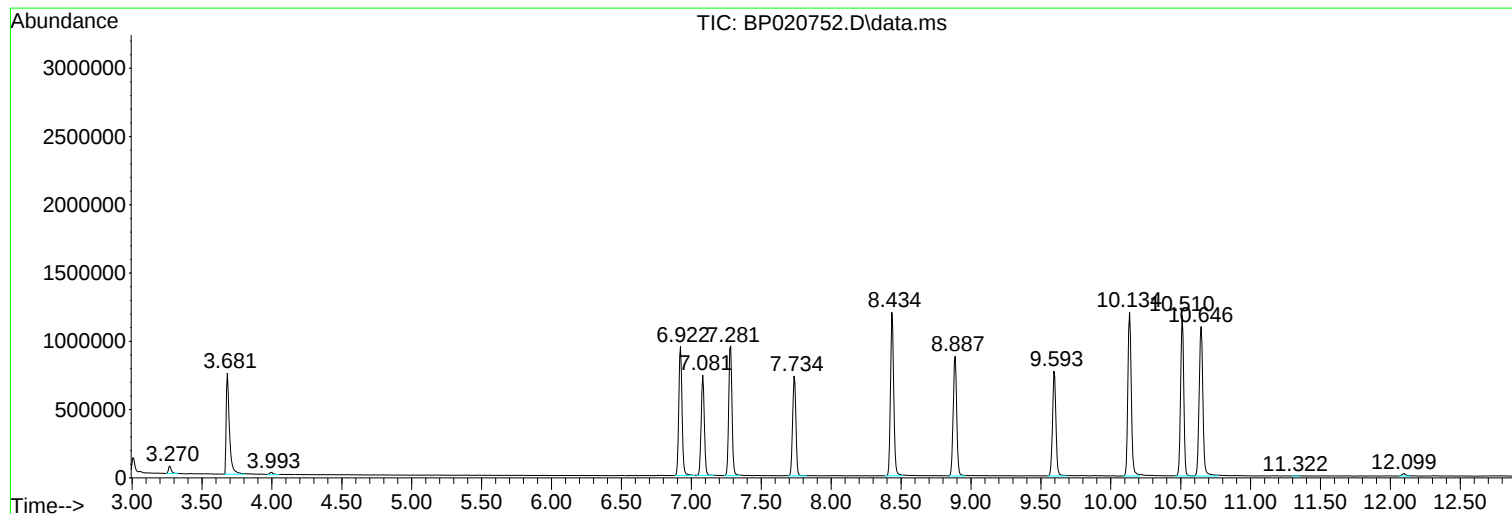

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070124\
Data File : BP020752.D
Acq On : 02 Jul 2024 15:51
Operator : MA/JU
Sample : PB161652BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK652

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070124\
Data File : BP020752.D
Acq On : 02 Jul 2024 15:51
Operator : MA/JU
Sample : PB161652BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK652

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc