
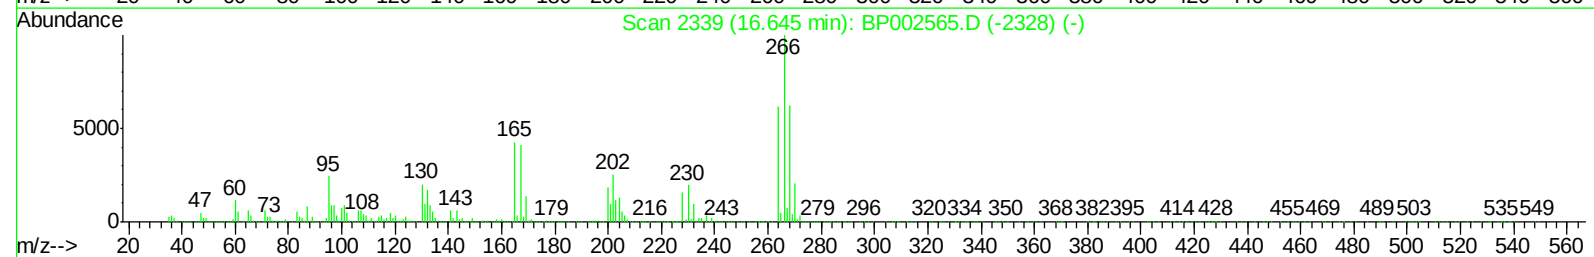
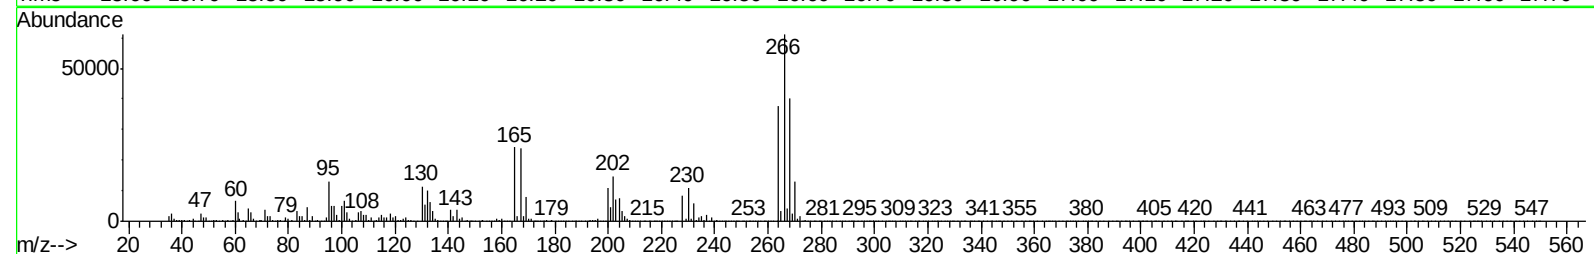


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP070220\
 Data File : BP002619.D
 Acq On : 02 Jul 2020 08:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 03 03:33:21 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP062920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 29 16:51:57 2020
 Response via : Initial Calibration

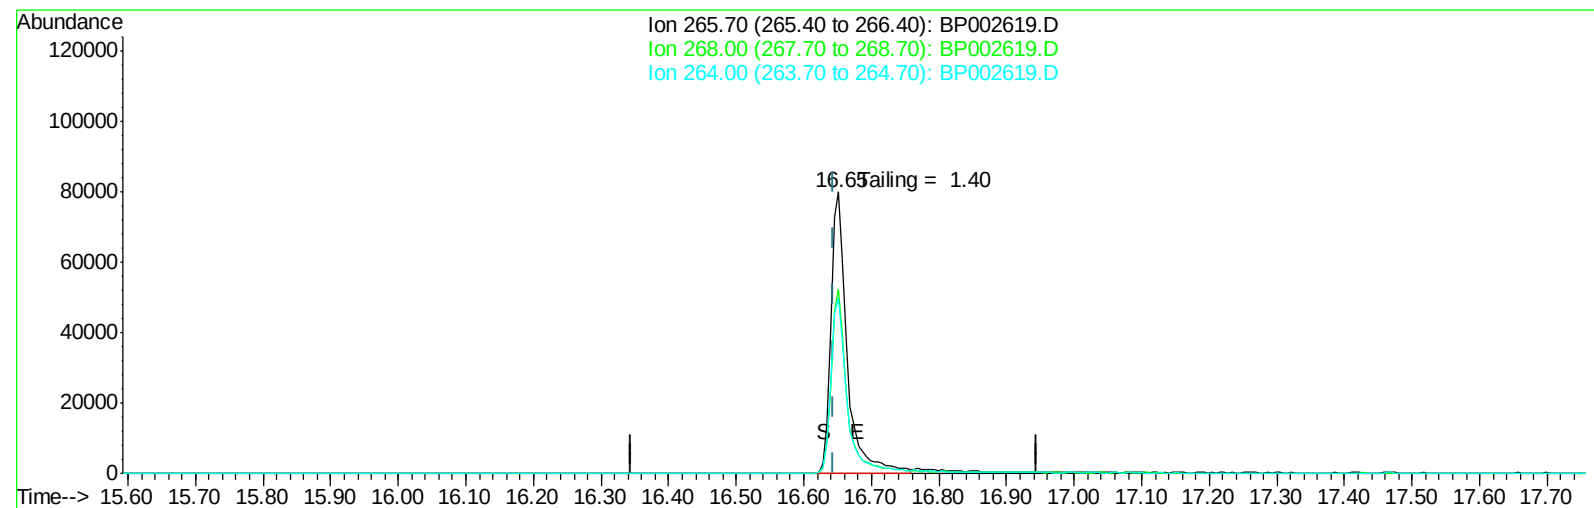

TIC: BP002619.D

(70) Pentachlorophenol (C)




16.651min (+0.006) 156879.58ng

response 136210

Ion	Exp%	Act%
265.70	100	100
268.00	62.10	65.50
264.00	61.60	62.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP070220\
Data File : BP002619.D
Acq On : 02 Jul 2020 08:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 03 03:33:21 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP062920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 29 16:51:57 2020
Response via : Initial Calibration

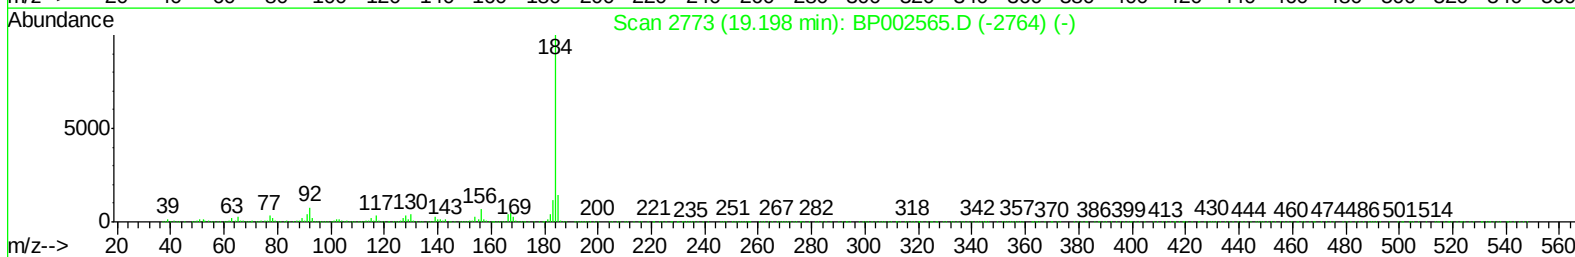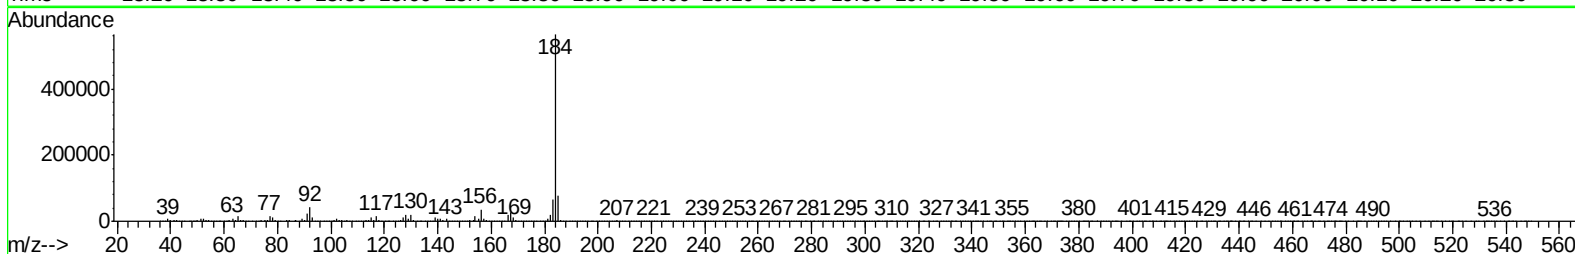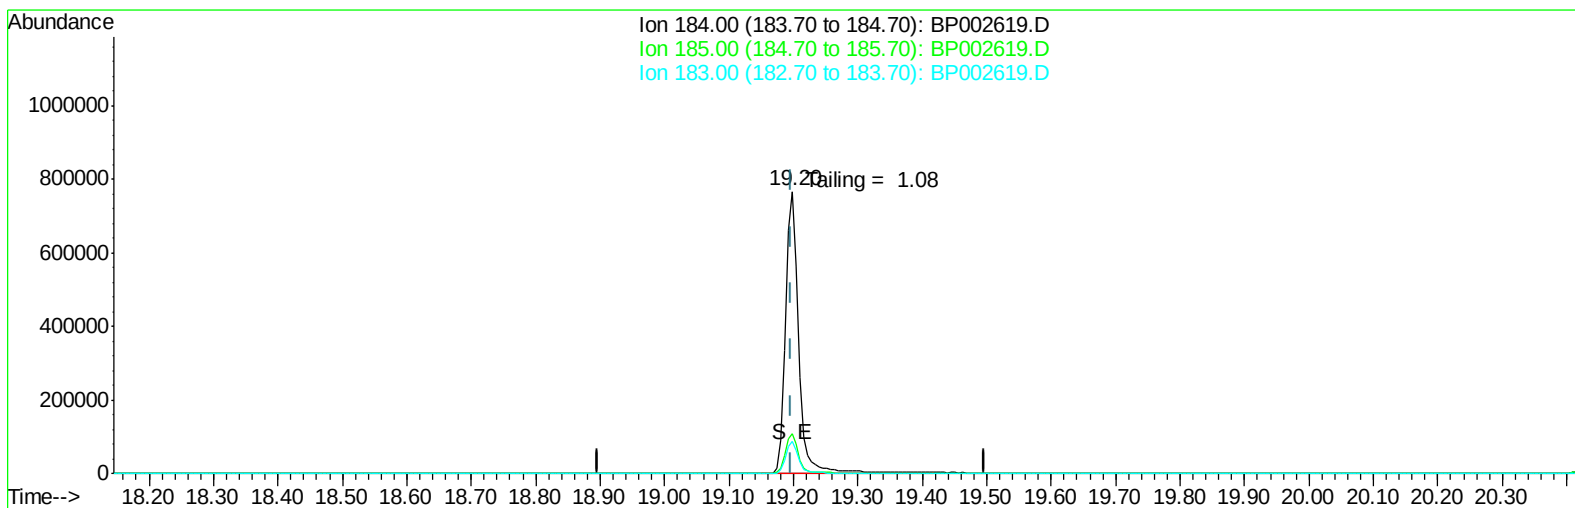

TIC: BP002619.D

(77) Benzidine

19.198min (+0.000) -20.00ng

response 1085244

Ion	Exp%	Act%
184.00	100	100
185.00	14.30	14.00
183.00	11.50	11.53
0.00	0.00	0.00