

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP070220\
 Data File : BP002635.D
 Acq On : 02 Jul 2020 17:39
 Operator : CG/JU
 Sample : L3172-09
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 TP1-TS

Quant Time: Jul 03 04:21:46 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP062920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 29 16:51:57 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	205388	20.00	ng	0.00
21) Naphthalene-d8	10.34	136	835033	20.00	ng	0.00
39) Acenaphthene-d10	14.22	164	539594	20.00	ng	0.00
64) Phenanthrene-d10	16.98	188	1220533	20.00	ng	0.00
76) Chrysene-d12	21.09	240	1315111	20.00	ng	0.00
86) Perylene-d12	23.28	264	1302181	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.19	112	848316	69.93	ng	0.00
7) Phenol-d6	6.76	99	1278176	75.49	ng	0.00
23) Nitrobenzene-d5	8.71	82	869908	53.68	ng	-0.01
42) 2,4,6-Tribromophenol	15.72	330	625501	95.31	ng	0.00
45) 2-Fluorobiphenyl	12.83	172	2248212	61.32	ng	0.00
79) Terphenyl-d14	19.57	244	3755204	61.63	ng	0.00
Target Compounds						
50) Dimethylphthalate	13.68	163	253642	5.985	ng	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP070220\
Data File : BP002635.D
Acq On : 02 Jul 2020 17:39
Operator : CG/JU
Sample : L3172-09
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP1-TS

Quant Time: Jul 03 04:21:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP062920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 29 16:51:57 2020
Response via : Initial Calibration

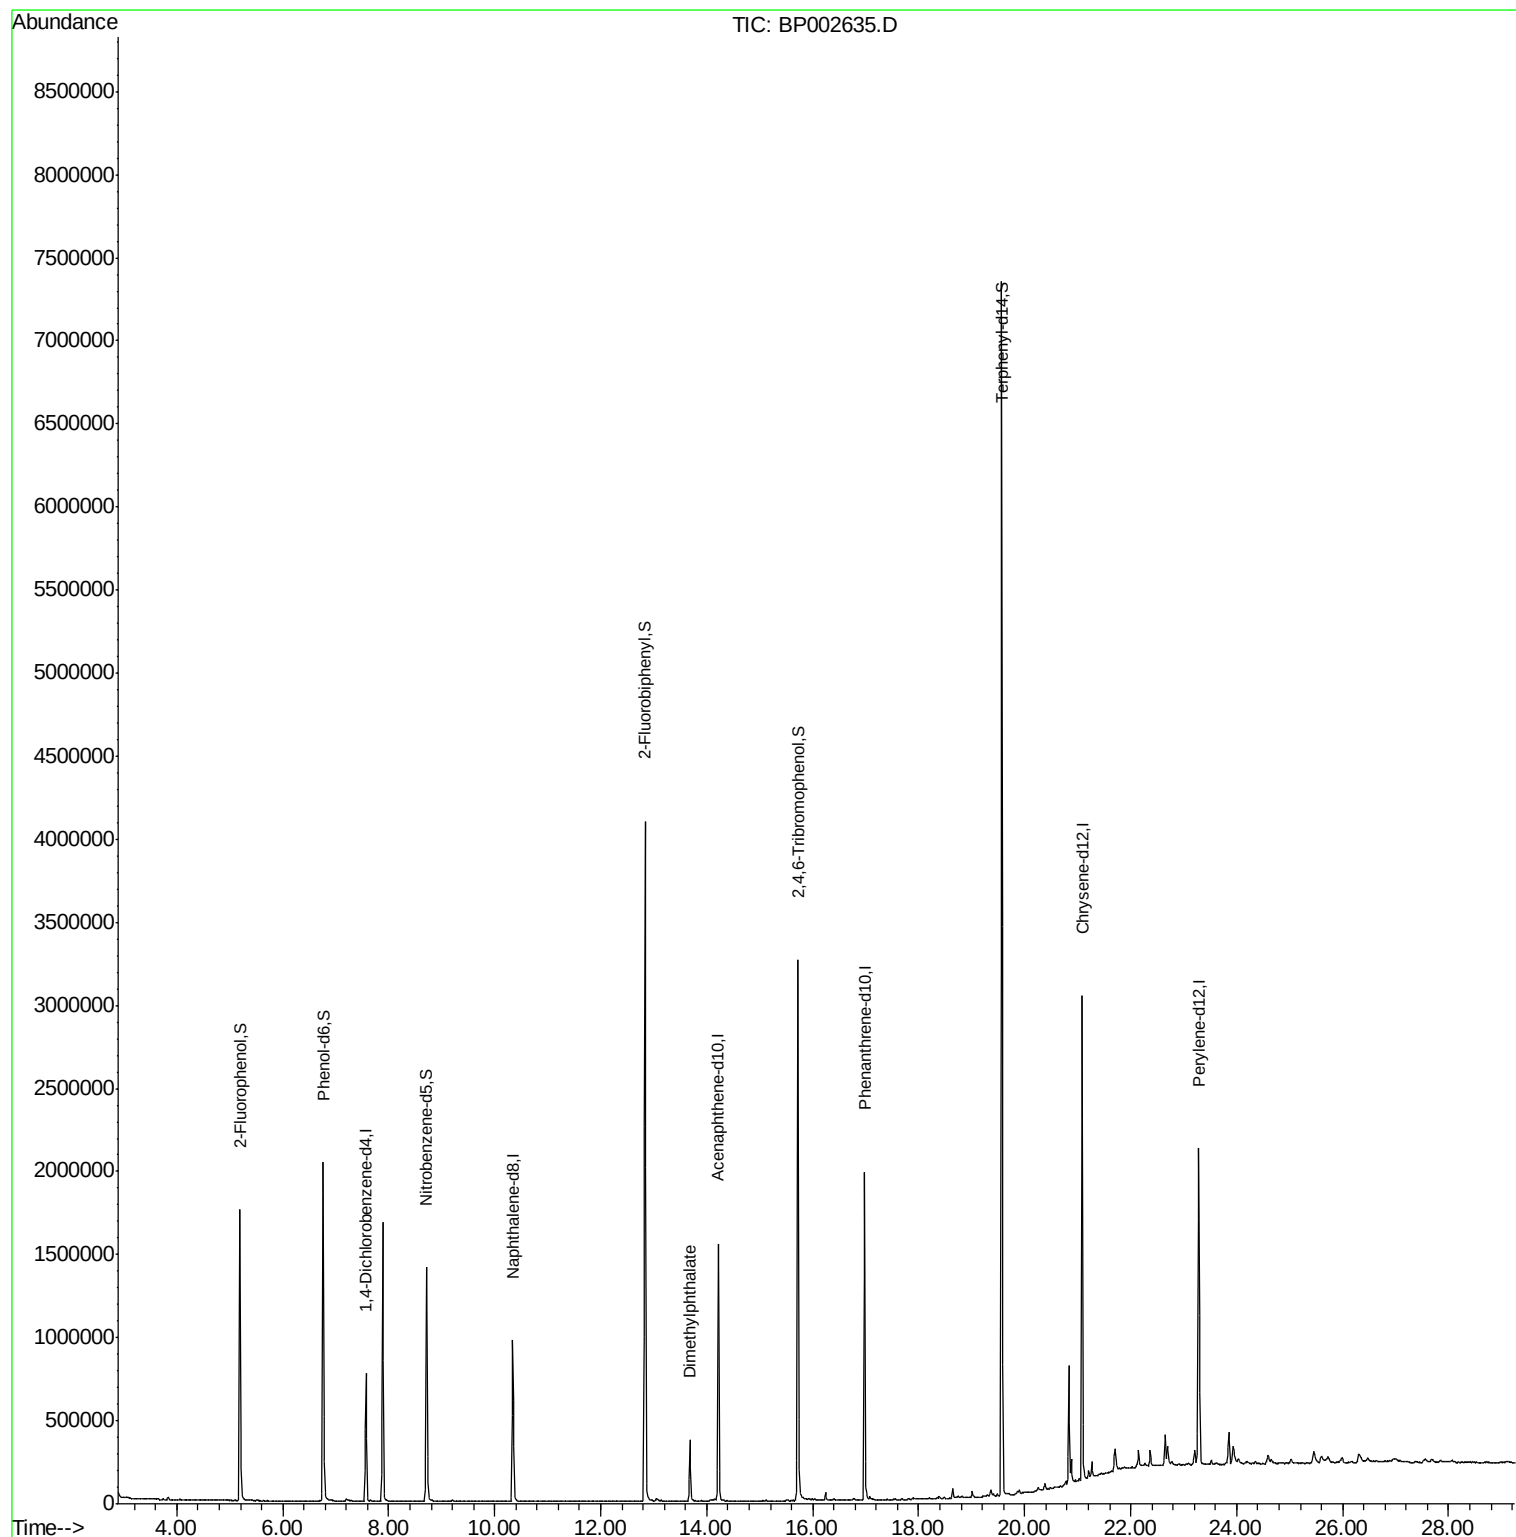







#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.57 min Scan# 796
Delta R.T. -0.01 min
Lab File: BP002635.D
Acq: 02 Jul 2020 17:39

Instrument :
BNA_P
ClientSampleId :
TP1-TS




Tot Ion	Ratio	Lower	Upper
152	100		
150	159.4	124.2	186.2
115	58.6	47.1	70.7

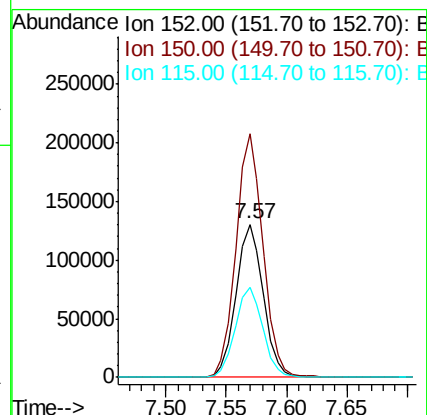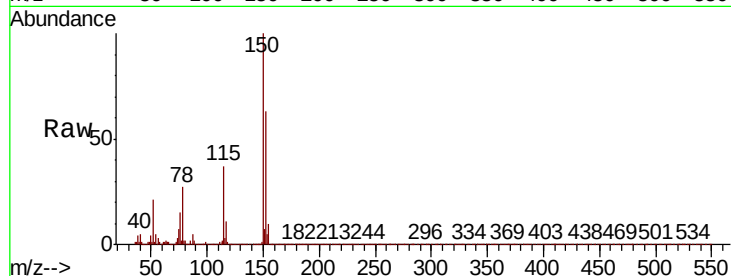


#5

2-Fluorophenol
Concen: 69.931 ng
RT: 5.19 min Scan# 392
Delta R.T. 0.00 min
Lab File: BP002635.D
Acq: 02 Jul 2020 17:39

Tgt Ion	Ratio	Lower	Upper
112	100		
64	57.6	47.0	70.6
63	29.7	26.1	39.1

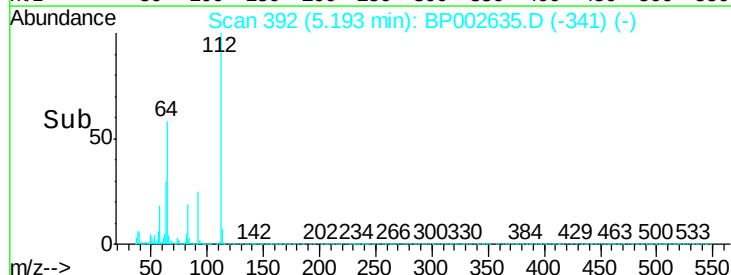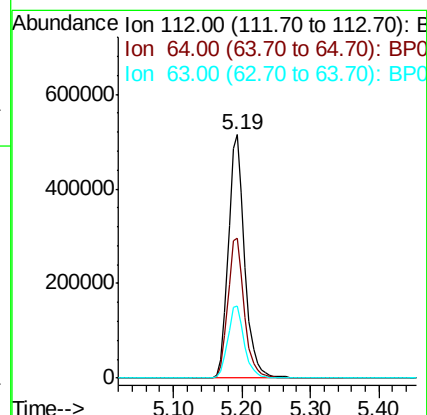

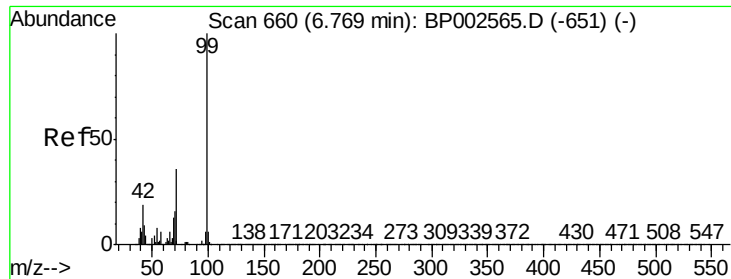

#7

Phenol-d6

Concen: 75.491 ng

RT: 6.76 min Scan# 659

Delta R.T. -0.01 min

Lab File: BP002635.D

Acq: 02 Jul 2020 17:39

Instrument :


BNA_P

ClientSampleId :

TP1-TS

Tot Ion: 99 Resp: 1278176

Ion	Ratio	Lower	Upper
99	100		
42	16.9	15.5	23.3
71	32.0	28.9	43.3






Abundance

Ion 99.00 (98.70 to 99.70): BP0

Ion 42.00 (41.70 to 42.70): BP0

Ion 71.00 (70.70 to 71.70): BP0

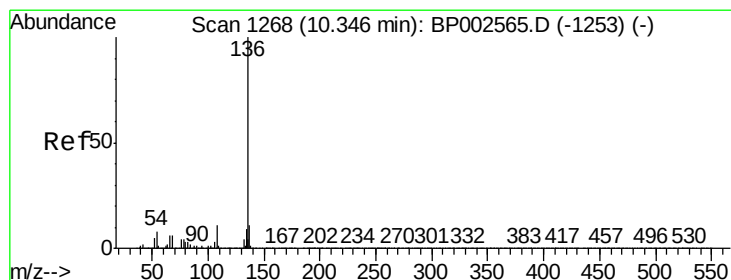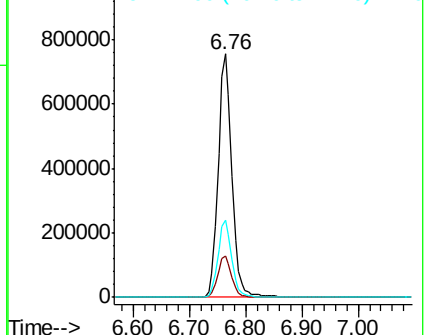

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.34 min Scan# 1267


Delta R.T. -0.01 min

Lab File: BP002635.D

Acq: 02 Jul 2020 17:39

Tgt Ion: 136 Resp: 835033

Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.8	13.2
54	8.5	6.4	9.6
68	7.3	5.1	7.7

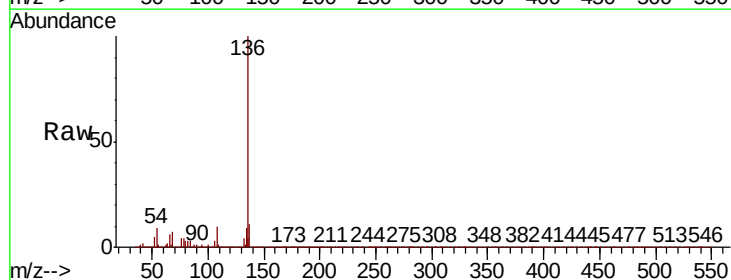



Abundance


Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BP0

Ion 68.00 (67.70 to 68.70): BP0




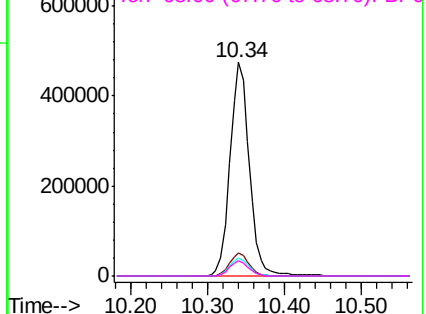


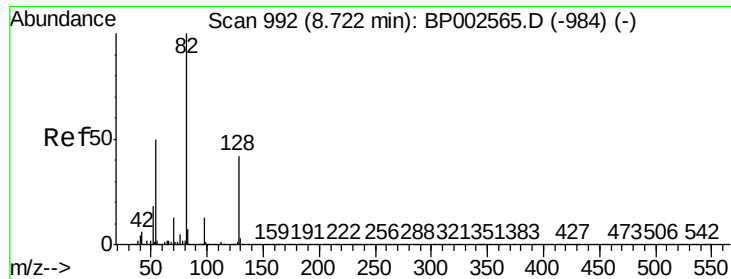

#23
Nitrobenzene-d5
Concen: 53.677 ng
RT: 8.71 min Scan# 990
Delta R.T. -0.01 min
Lab File: BP002635.D
Acq: 02 Jul 2020 17:39




Instrument :
BNA_P
ClientSampleId :
TP1-TS


Tot Ion	82	Resp	869908
Ion Ratio	Lower	Upper	
82	100		
128	40.8	33.4	50.2
54	48.8	40.1	60.1

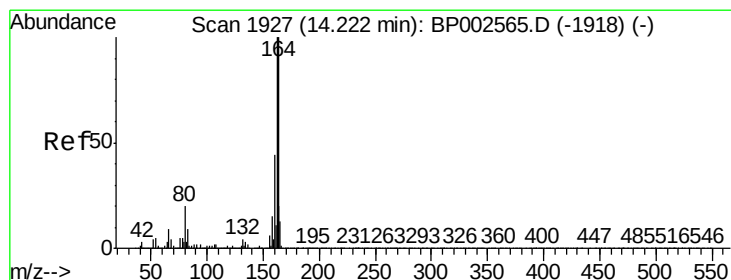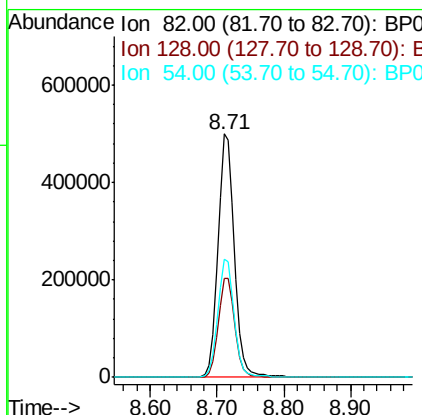

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.22 min Scan# 1927
Delta R.T. 0.00 min
Lab File: BP002635.D
Acq: 02 Jul 2020 17:39

Tgt Ion	164	Resp	539594
Ion Ratio	Lower	Upper	
164	100		
162	98.9	80.3	120.5
160	44.4	35.0	52.6


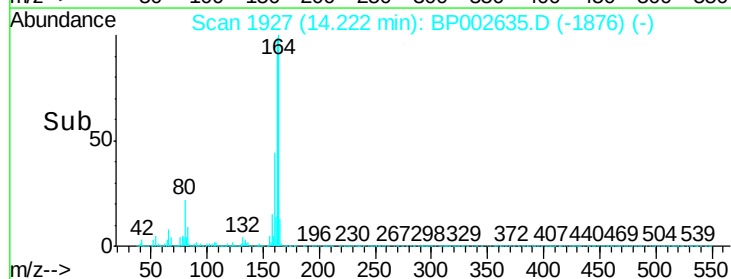
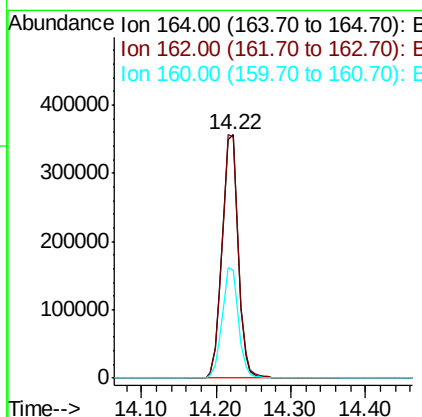
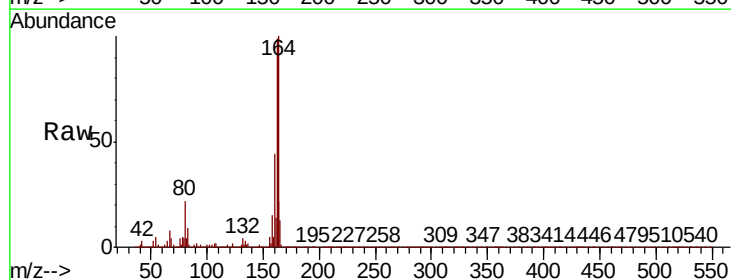


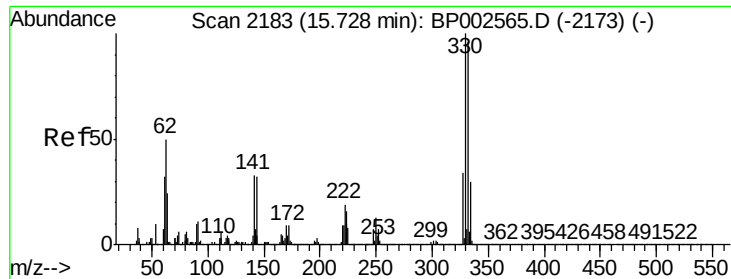

#42
 2,4,6-Tribromophenol
 Concen: 95.307 ng
 RT: 15.72 min Scan# 2182
 Delta R.T. -0.01 min
 Lab File: BP002635.D
 Acq: 02 Jul 2020 17:39




Instrument :
 BNA_P
 ClientSampleId :
 TP1-TS


Tot Ion:330 Resp: 625501
 Ion Ratio Lower Upper
 330 100
 332 96.7 77.7 116.5
 141 35.5 29.0 43.6

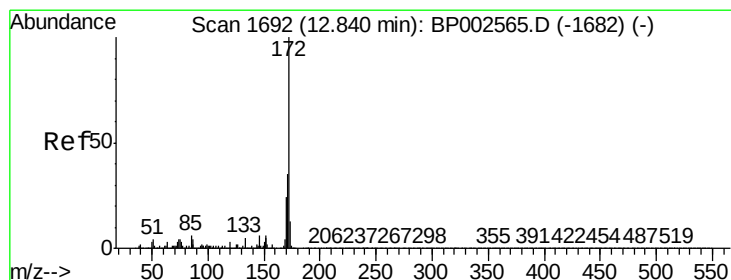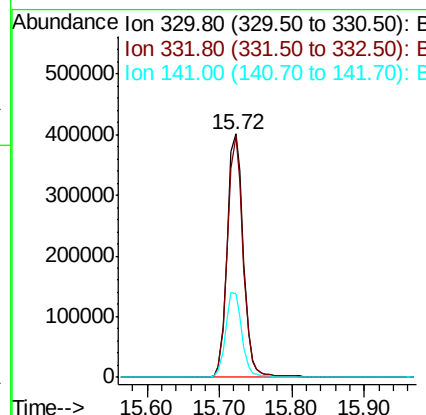

#45
 2-Fluorobiphenyl
 Concen: 61.324 ng
 RT: 12.83 min Scan# 1691
 Delta R.T. -0.01 min
 Lab File: BP002635.D
 Acq: 02 Jul 2020 17:39

Tgt Ion:172 Resp: 2248212
 Ion Ratio Lower Upper
 172 100
 171 35.3 28.0 42.0
 170 24.2 19.0 28.4

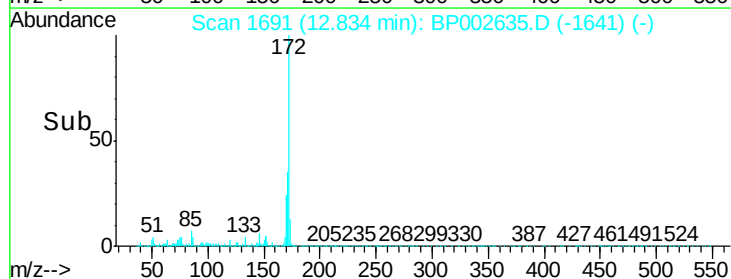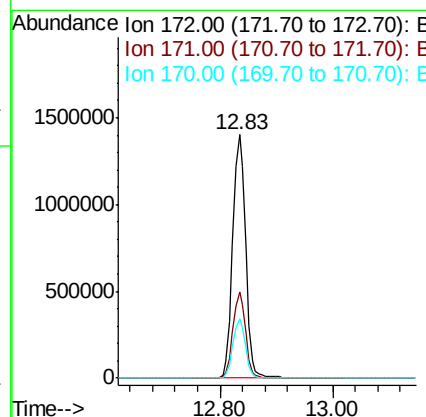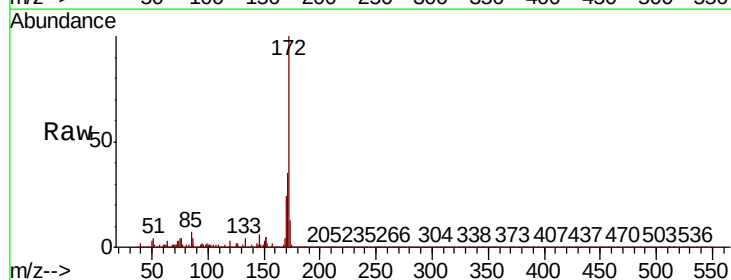

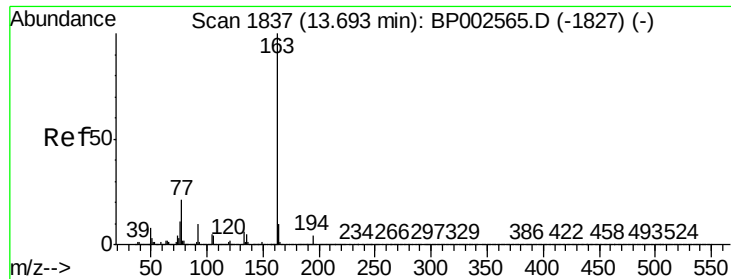

#50

Dimethylphthalate

Concen: 5.985 ng

RT: 13.68 min Scan# 1835

Delta R.T. -0.01 min

Lab File: BP002635.D

Acq: 02 Jul 2020 17:39

Instrument :

BNA_P

ClientSampleId :

TP1-TS


Tot Ion:163 Resp: 253642

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.0




164 10.4 8.2 12.4



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

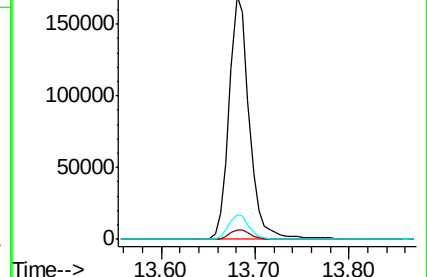

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 16.98 min Scan# 2396

Delta R.T. 0.00 min

Lab File: BP002635.D

Acq: 02 Jul 2020 17:39


Tgt Ion:188 Resp: 1220533

Ion Ratio Lower Upper

188 100

94 9.6 7.8 11.6



80 10.7 8.2 12.4




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BP0

Ion 80.00 (79.70 to 80.70): BP0

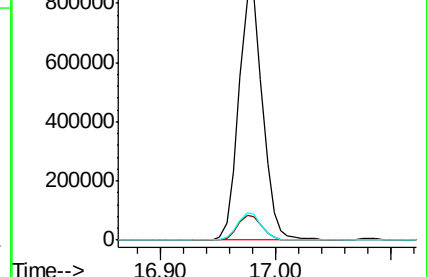







#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.09 min Scan# 3094
Delta R.T. -0.01 min
Lab File: BP002635.D
Acq: 02 Jul 2020 17:39

Instrument :
BNA_P
ClientSampleId :
TP1-TS

Tot Ion:240 Resp: 1315111
Ion Ratio Lower Upper
240 100
120 12.0 8.6 13.0
236 26.5 20.8 31.2




Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E


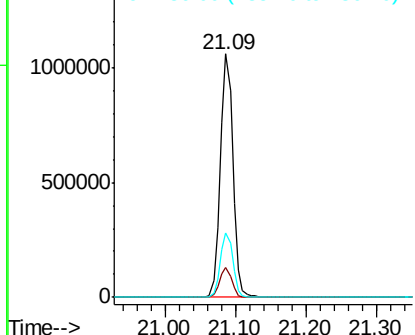



#79
Terphenyl-d14
Concen: 61.634 ng
RT: 19.57 min Scan# 2836
Delta R.T. -0.01 min
Lab File: BP002635.D
Acq: 02 Jul 2020 17:39

Tgt Ion:244 Resp: 3755204
Ion Ratio Lower Upper
244 100
212 7.6 6.5 9.7
122 10.5 7.9 11.9



Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

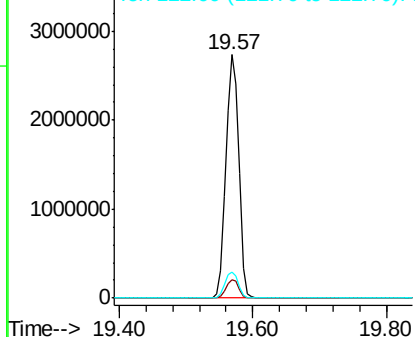

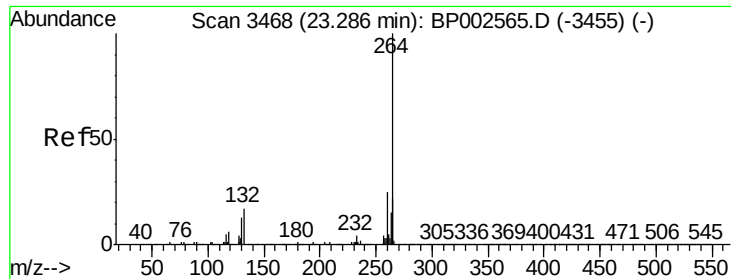


#86
Pervlene-d12
Concen: 20.000 ng
RT: 23.28 min Scan# 3467
Delta R.T. -0.01 min
Lab File: BP002635.D
Acq: 02 Jul 2020 17:39

Instrument :
BNA_P
ClientSampleId :
TP1-TS

Tot Ion:264 Resp: 1302181

Ion	Ratio	Lower	Upper
264	100		
260	24.1	19.7	29.5
265	20.9	17.6	26.4



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

