


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070220\
 Data File : BP002619.D
 Acq On : 02 Jul 2020 08:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 29 16:51:57 2020

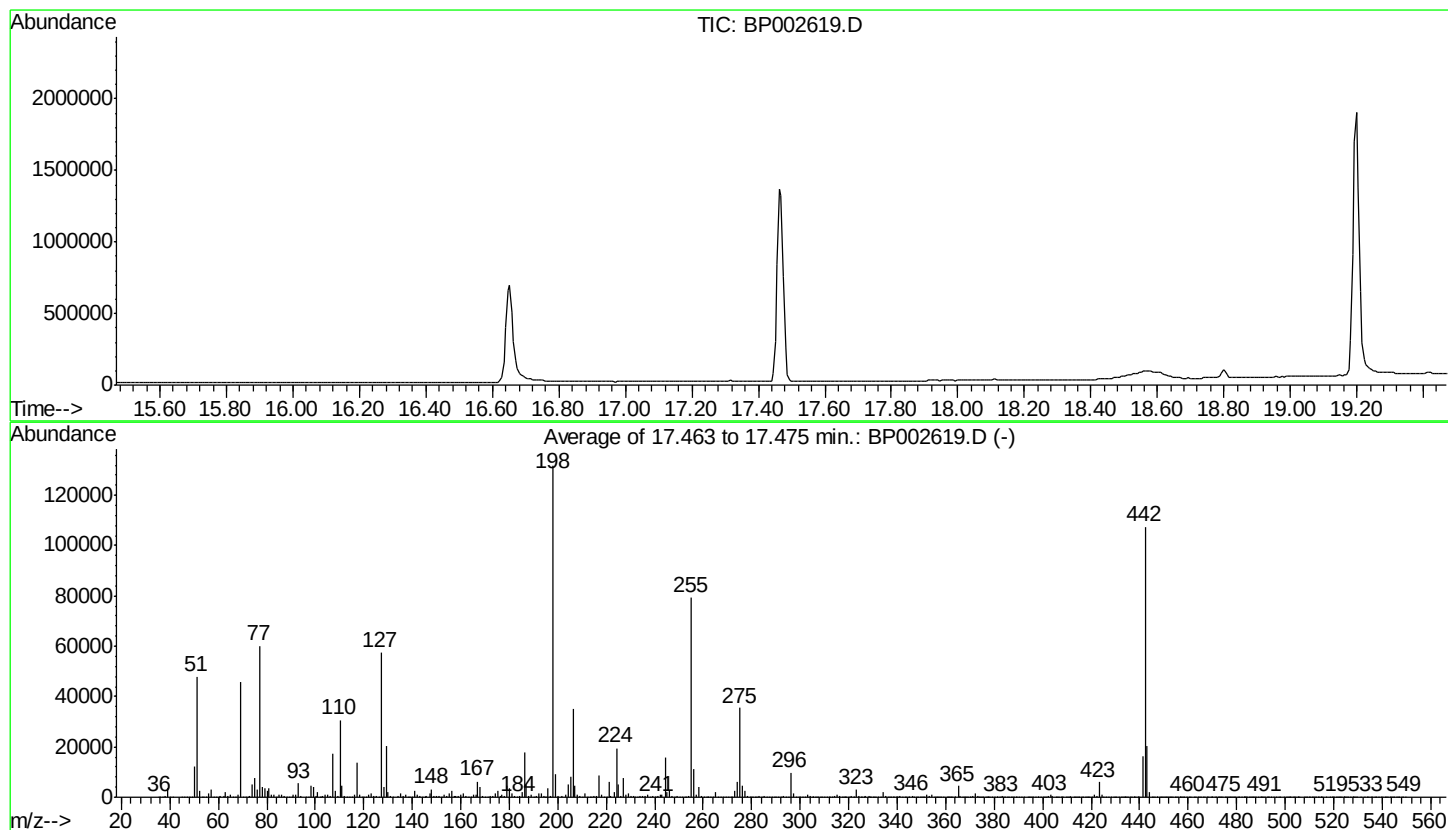

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	47847	PASS
68	69	0.00	2	1.8	803	PASS
69	198	0.00	100	34.8	45839	PASS
70	69	0.00	2	0.4	185	PASS
127	198	10	80	43.5	57351	PASS
197	198	0.00	2	0.5	615	PASS
198	198	100	100	100.0	131760	PASS
199	198	5	9	6.8	8976	PASS
275	198	10	60	27.0	35578	PASS
365	198	1	100	3.4	4454	PASS
441	198	0.01	100	12.4	16307	PASS
442	198	50	100	81.5	107368	PASS
443	442	15	24	18.8	20180	PASS