


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP070225\  
Data File : BP025061.D  
Acq On : 02 Jul 2025 09:29  
Operator : RC/JU  
Sample : DFTPP626  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP626

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP063025.MA.M  
Title : SVOA CALIBRATION  
Last Update : Tue Jul 01 11:17:33 2025

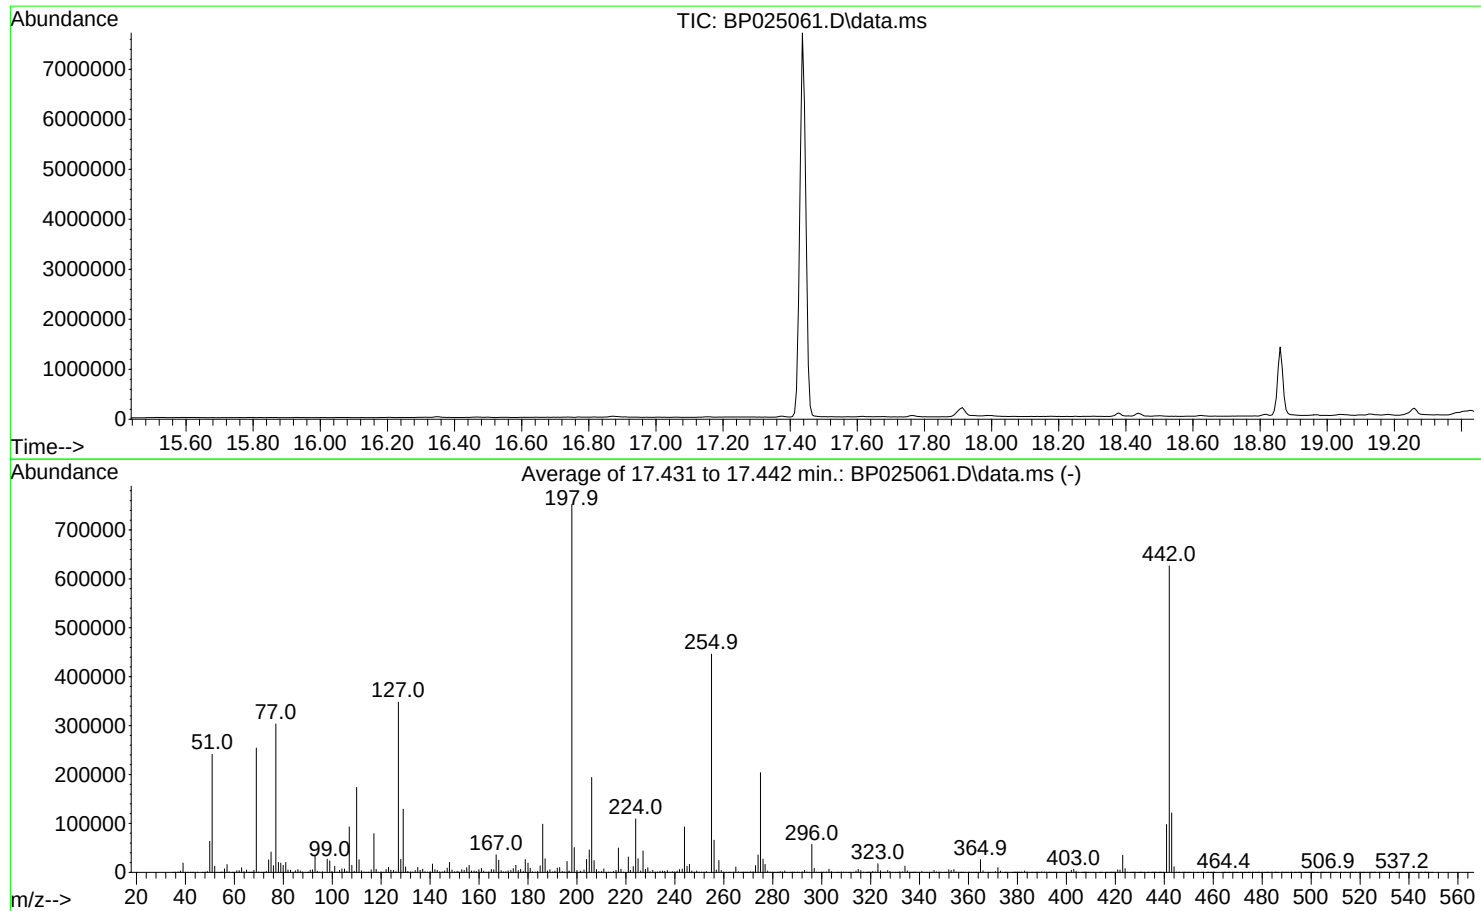

AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2458

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 32.1         | 241355     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.6          | 4149       | PASS                |
| 69             | 198             | 0.00            | 100             | 33.8         | 254101     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.4          | 1135       | PASS                |
| 127            | 198             | 10              | 80              | 46.2         | 347654     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.3          | 2591       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 752054     | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 50638      | PASS                |
| 275            | 198             | 10              | 60              | 27.1         | 203706     | PASS                |
| 365            | 198             | 1               | 100             | 3.5          | 26086      | PASS                |
| 441            | 198             | 0.01            | 100             | 13.0         | 97922      | PASS                |
| 442            | 198             | 50              | 100             | 83.3         | 626382     | PASS                |
| 443            | 442             | 15              | 24              | 19.4         | 121800     | PASS                |