

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070524\
 Data File : BP020793.D
 Acq On : 05 Jul 2024 17:59
 Operator : MA/JU
 Sample : P2987-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0TA3

Quant Time: Jul 05 18:33:21 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 03 15:01:56 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.728	152	271093	20.000	ng/u1	0.00
20) Naphthalene-d8	10.499	136	1140720	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.357	164	745481	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.169	188	1568468	20.000	ng/u1	0.00
79) Chrysene-d12	21.622	240	1472745	20.000	ng/u1	0.00
88) Perylene-d12	24.963	264	1676249	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	26662	4.223	ng/uL	0.00
4) Pyridine-d5	3.681	84	129759	7.052	ng/u1	0.00
7) Phenol-d5	6.916	99	600057	26.987	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.069	67	367053	26.040	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.269	132	501123	27.577	ng/u1	0.00
15) 4-Methylphenol-d8	8.434	113	496770	27.509	ng/u1	0.00
21) Nitrobenzene-d5	8.881	128	251573	29.871	ng/u1	0.00
24) 2-Nitrophenol-d4	9.587	143	287935	34.164	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.128	165	494422	28.480	ng/u1	0.00
31) 4-Chloroaniline-d4	10.634	131	426354	17.524	ng/u1	0.00
46) Dimethylphthalate-d6	13.769	166	1529226	29.503	ng/u1	0.01
49) Acenaphthylene-d8	14.051	160	1735873	28.066	ng/u1	0.01
54) 4-Nitrophenol-d4	14.592	143	230165	29.063	ng/u1	0.01
60) Fluorene-d10	15.369	176	1289730	29.570	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.498	200	197951	25.044	ng/u1	0.00
73) Anthracene-d10	17.269	188	1970701	27.996	ng/u1	0.00
81) Pyrene-d10	19.651	212	2346955	26.526	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.739	264	2361538	28.962	ng/u1	0.00


Target Compounds					Qvalue	
30) Naphthalene	10.546	128	94810	1.553	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070524\
Data File : BP020793.D
Acq On : 05 Jul 2024 17:59
Operator : MA/JU
Sample : P2987-14
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0TA3

Quant Time: Jul 05 18:33:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 03 15:01:56 2024
Response via : Initial Calibration

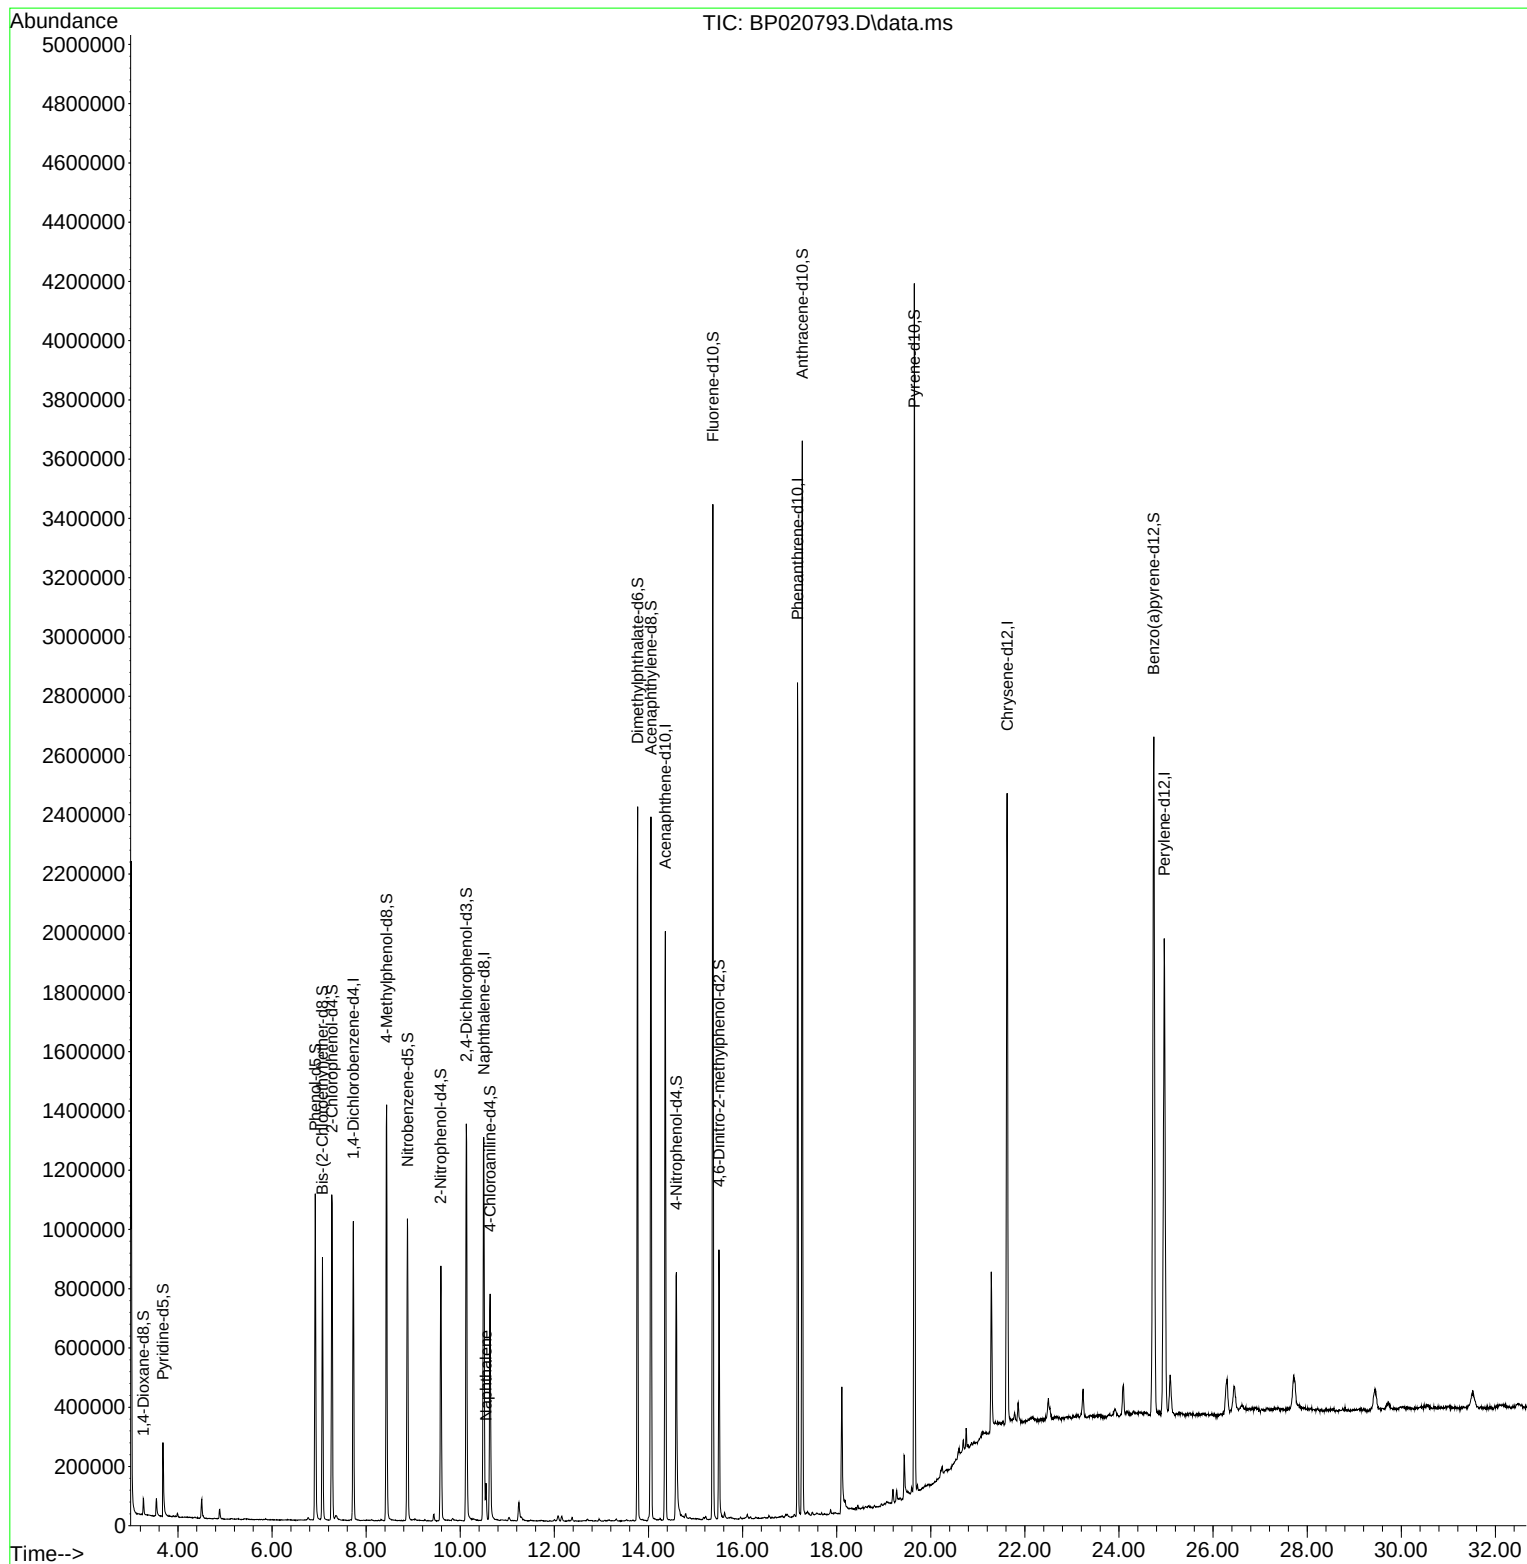

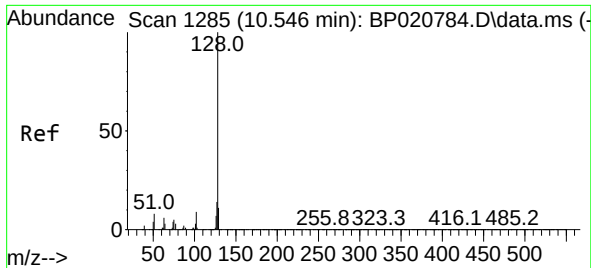

#30
Naphthalene
Concen: 1.553 ng/ul
RT: 10.546 min Scan# 11
Delta R.T. -0.000 min
Lab File: BP020793.D
Acq: 05 Jul 2024 17:59

Instrument :
BNA_P
ClientSampleId :
C0TA3

Tgt Ion:128 Resp: 94810
Ion Ratio Lower Upper
128 100
129 10.2 8.7 13.1
127 13.4 10.6 15.8

