

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070524\
 Data File : BP020795.D
 Acq On : 05 Jul 2024 19:25
 Operator : MA/JU
 Sample : P2987-16
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0TA5

Quant Time: Jul 05 22:41:19 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 03 15:01:56 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.722	152	221880	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.499	136	918940	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.357	164	599897	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.169	188	1266014	20.000	ng/ul	0.00
79) Chrysene-d12	21.622	240	1209403	20.000	ng/ul	0.00
88) Perylene-d12	24.968	264	1408031	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	27341	5.291	ng/uL	0.00
4) Pyridine-d5	3.675	84	286863	19.049	ng/ul	0.00
7) Phenol-d5	6.916	99	629779	34.606	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.069	67	375872	32.580	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.275	132	516453	34.724	ng/ul	0.00
15) 4-Methylphenol-d8	8.434	113	520934	35.245	ng/ul	0.00
21) Nitrobenzene-d5	8.875	128	262245	38.653	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.587	143	296038	43.603	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.128	165	514828	36.812	ng/ul	0.00
31) 4-Chloroaniline-d4	10.634	131	432505	22.067	ng/ul	0.00
46) Dimethylphthalate-d6	13.763	166	1594981	38.240	ng/ul	0.00
49) Acenaphthylene-d8	14.051	160	1808890	36.345	ng/ul	0.01
54) 4-Nitrophenol-d4	14.587	143	252583	39.634	ng/ul	0.00
60) Fluorene-d10	15.369	176	1350785	38.485	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.504	200	214730	33.657	ng/ul	0.00
73) Anthracene-d10	17.275	188	2138288	37.633	ng/ul	0.01
81) Pyrene-d10	19.657	212	2503837	34.462	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.745	264	2602718	38.000	ng/ul	0.00
Target Compounds						
30) Naphthalene	10.540	128	62854	1.278	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070524\
Data File : BP020795.D
Acq On : 05 Jul 2024 19:25
Operator : MA/JU
Sample : P2987-16
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0TA5


Quant Time: Jul 05 22:41:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 03 15:01:56 2024
Response via : Initial Calibration

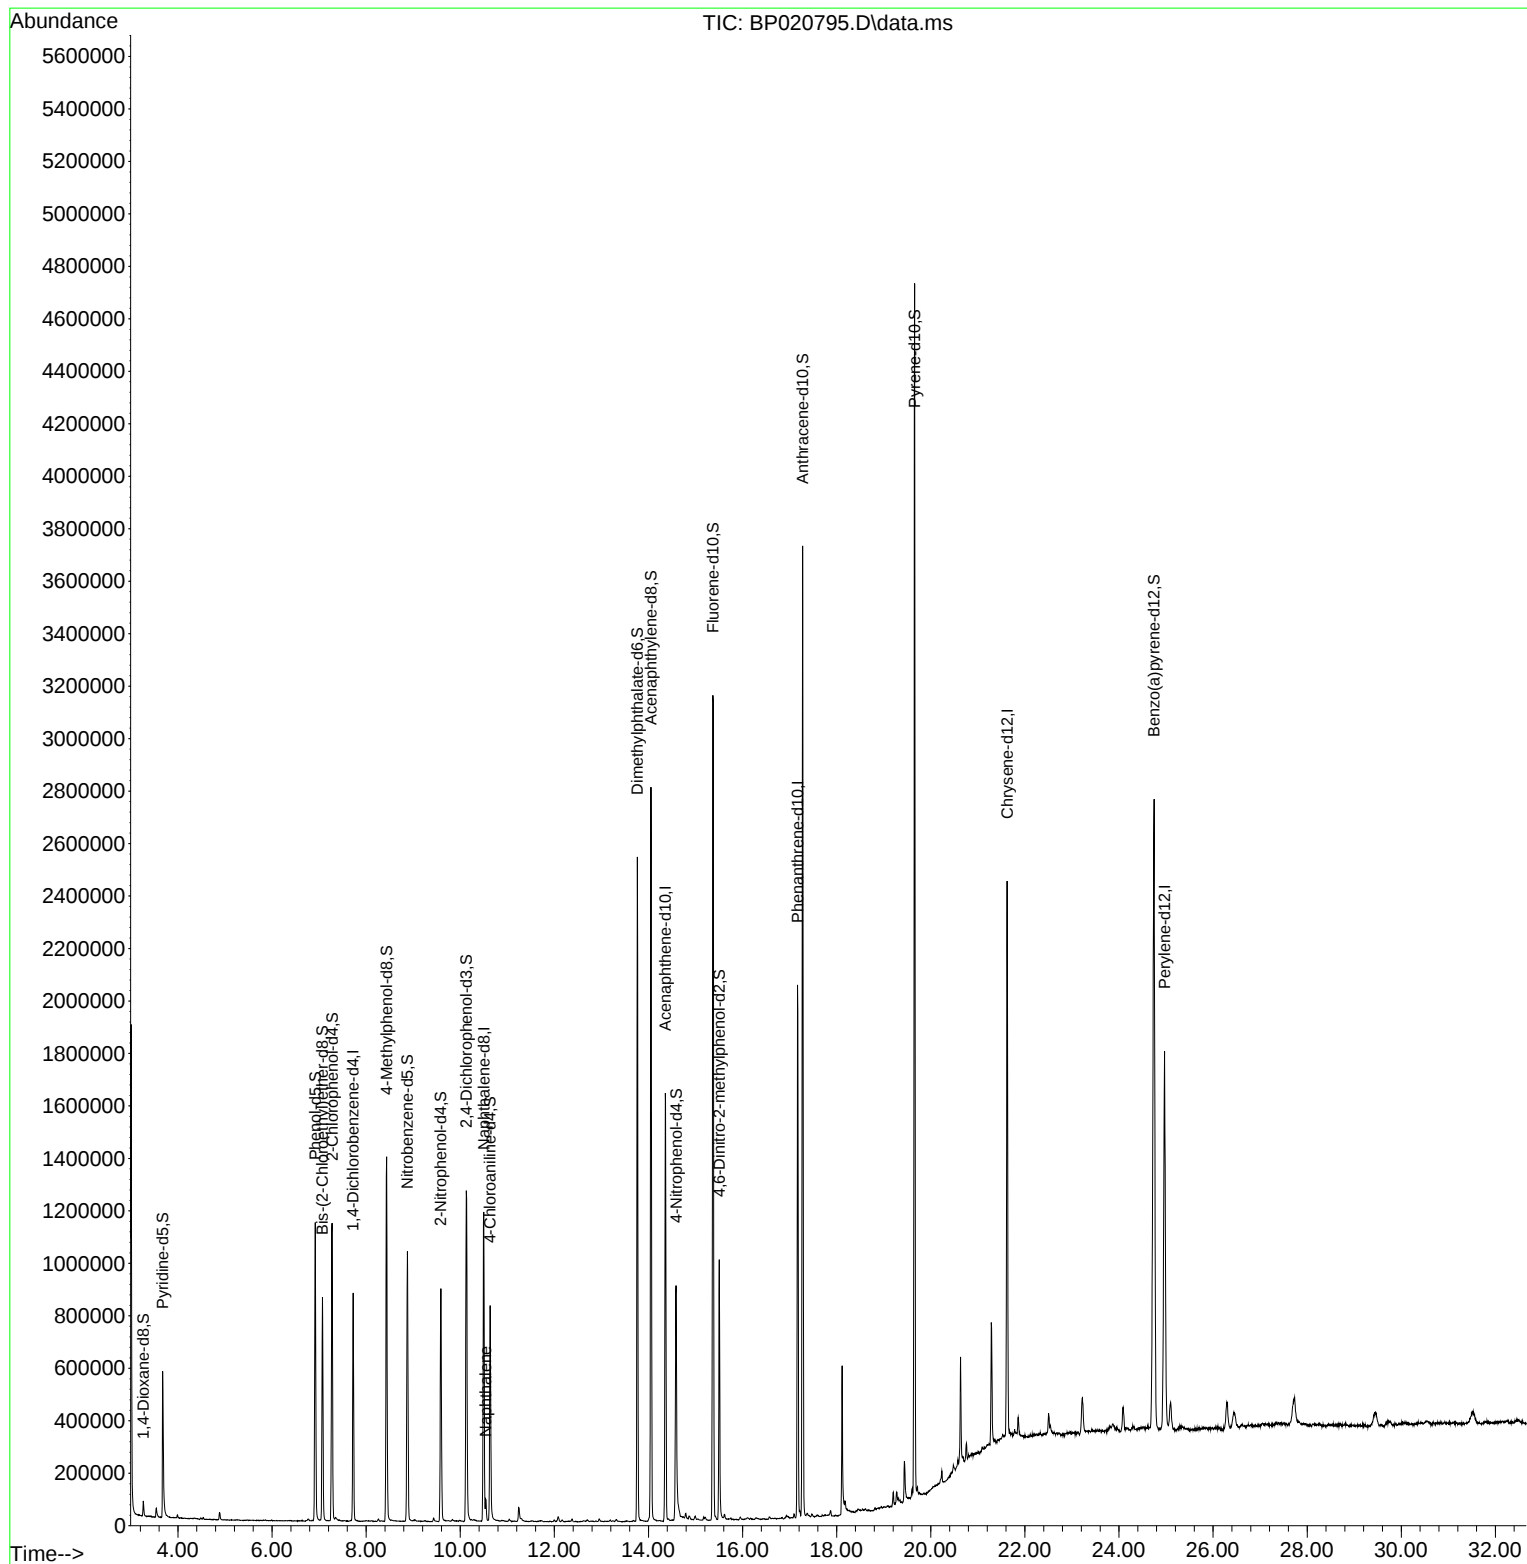

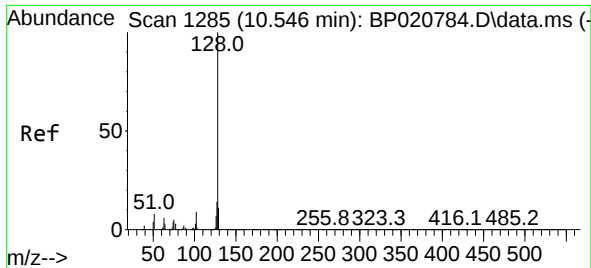

#30
Naphthalene
Concen: 1.278 ng/ul
RT: 10.540 min Scan# 11
Delta R.T. -0.006 min
Lab File: BP020795.D
Acq: 05 Jul 2024 19:25

Instrument :
BNA_P
ClientSampleId :
C0TA5

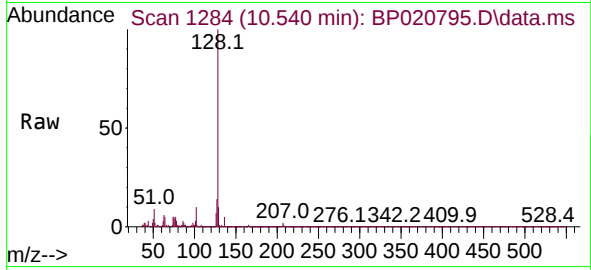

Tgt Ion:128 Resp: 62854
Ion Ratio Lower Upper
128 100
129 10.0 8.7 13.1
127 14.2 10.6 15.8

