


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070620\
 Data File : BP002639.D
 Acq On : 06 Jul 2020 08:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 29 16:51:57 2020

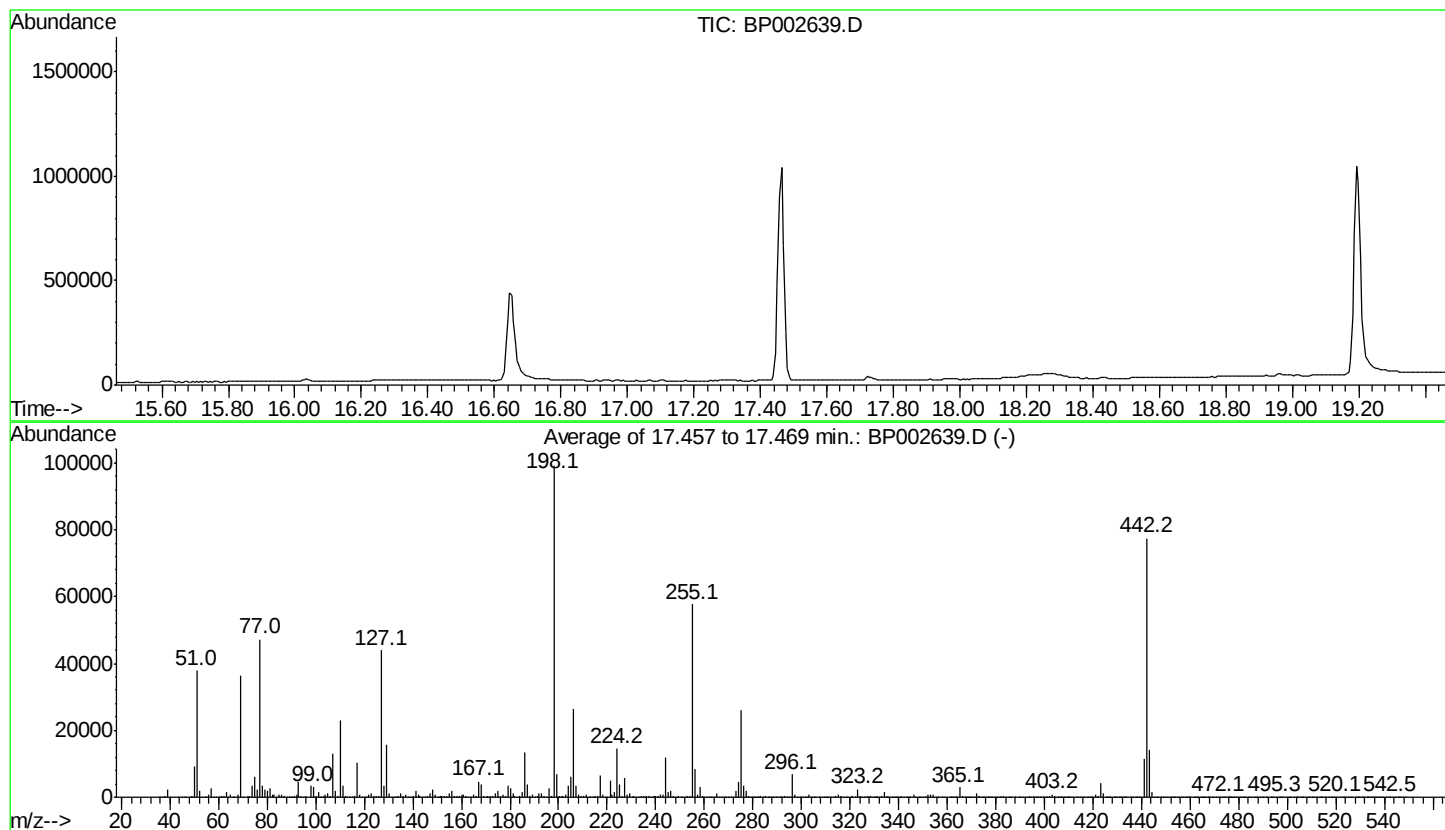

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	37852	PASS
68	69	0.00	2	1.8	655	PASS
69	198	0.00	100	36.8	36537	PASS
70	69	0.00	2	0.3	125	PASS
127	198	10	80	44.3	43992	PASS
197	198	0.00	2	0.3	283	PASS
198	198	100	100	100.0	99197	PASS
199	198	5	9	6.9	6835	PASS
275	198	10	60	26.2	26005	PASS
365	198	1	100	3.0	3007	PASS
441	198	0.01	100	11.4	11333	PASS
442	198	50	100	78.0	77403	PASS
443	442	15	24	18.5	14341	PASS