

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070622\
 Data File : BP010926.D
 Acq On : 06 Jul 2022 12:39
 Operator : CG/JU
 Sample : PB145967BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK967

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010926.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	16	20	27	rVB	149468	182934	2.89%	0.249%
2	3.611	86	89	105	rBV	1477869	2076418	32.75%	2.823%
3	3.929	138	143	151	rVB	39215	57278	0.90%	0.078%
4	6.711	611	616	618	rBV5	5018	7124	0.11%	0.010%
5	6.887	637	646	657	rBV	1652024	2533676	39.96%	3.445%
6	7.052	668	674	682	rVB	1441674	2156322	34.01%	2.932%
7	7.240	698	706	717	rBV	1746789	2675055	42.19%	3.637%
8	7.705	778	785	793	rBV	1574015	2471573	38.98%	3.360%
9	7.922	819	822	825	rBV2	5643	6430	0.10%	0.009%
10	8.152	858	861	868	rBV6	6205	10357	0.16%	0.014%
11	8.422	900	907	916	rBV	1919227	3002809	47.36%	4.082%
12	8.869	974	983	994	rBV	1464077	2309949	36.43%	3.140%
13	9.440	1077	1080	1085	rBV6	4549	7384	0.12%	0.010%
14	9.587	1094	1105	1117	rBV	974284	1576386	24.86%	2.143%
15	9.693	1118	1123	1127	rVB7	7558	14305	0.23%	0.019%
16	10.128	1189	1197	1209	rBV	1630603	2660827	41.96%	3.617%
17	10.322	1228	1230	1235	rVB2	5022	6478	0.10%	0.009%
18	10.505	1252	1261	1269	rBV	2001629	3324714	52.43%	4.520%
19	10.646	1278	1285	1298	rBV	871376	1476089	23.28%	2.007%
20	10.834	1315	1317	1323	rVB5	7024	11329	0.18%	0.015%
21	11.452	1417	1422	1426	rBV5	5434	10152	0.16%	0.014%
22	11.493	1426	1429	1432	rBV4	4501	7268	0.11%	0.010%
23	12.099	1526	1532	1538	rBV3	33433	55829	0.88%	0.076%
24	12.169	1541	1544	1548	rVB5	6257	10815	0.17%	0.015%
25	12.310	1558	1568	1569	rBV9	6357	12669	0.20%	0.017%
26	12.399	1579	1583	1586	rVB5	6561	9902	0.16%	0.013%
27	12.863	1657	1662	1667	rBV8	5577	9967	0.16%	0.014%
28	13.146	1705	1710	1714	rVV3	8186	14999	0.24%	0.020%
29	13.193	1714	1718	1721	rVV3	8556	12839	0.20%	0.017%
30	13.228	1721	1724	1729	rVB6	5886	9335	0.15%	0.013%
31	13.781	1812	1818	1825	rBV	2255125	3052722	48.15%	4.150%
32	14.051	1857	1864	1876	rBV	2722640	3987181	62.88%	5.421%
33	14.363	1909	1917	1924	rBV	2458304	3534049	55.74%	4.805%
34	14.422	1924	1927	1934	rVB6	10386	20475	0.32%	0.028%
35	14.575	1945	1953	1967	rBV	882402	1422060	22.43%	1.933%
36	14.728	1976	1979	1982	rBV4	4534	6536	0.10%	0.009%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070622\
 Data File : BP010926.D
 Acq On : 06 Jul 2022 12:39
 Operator : CG/JU
 Sample : PB145967BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK967

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

37	14.751	1982	1983	1989	rVB2	7617	9974	0.16%	0.014%
38	14.993	2020	2024	2027	rBV6	7065	9043	0.14%	0.012%
39	15.204	2056	2060	2066	rVB5	6913	7900	0.12%	0.011%
40	15.363	2080	2087	2094	rBV	3467833	4860859	76.66%	6.608%
41	15.481	2102	2107	2122	rVB	585481	803302	12.67%	1.092%
42	15.604	2124	2128	2131	rVB	32308	41378	0.65%	0.056%
43	16.151	2217	2221	2227	rVB8	12786	21157	0.33%	0.029%
44	16.322	2246	2250	2254	rVB7	4702	7662	0.12%	0.010%
45	16.422	2263	2267	2274	rVB10	5946	9312	0.15%	0.013%
46	17.128	2380	2387	2397	rBV	2642770	3656108	57.66%	4.970%
47	17.228	2397	2404	2424	rVB	3448725	4913014	77.48%	6.679%
48	17.763	2492	2495	2497	rBV4	6915	9773	0.15%	0.013%
49	19.051	2711	2714	2719	rBV2	37219	46945	0.74%	0.064%
50	19.122	2723	2726	2730	rVV	32056	36616	0.58%	0.050%
51	19.475	2781	2786	2795	rBV	4236282	5401615	85.19%	7.343%
52	21.239	3081	3086	3095	rBV2	3347703	4211970	66.43%	5.726%
53	23.451	3455	3462	3472	rBV2	3309821	6340644	100.00%	8.620%
54	23.604	3482	3488	3500	rVB2	2329514	4425238	69.79%	6.016%




Sum of corrected areas: 73556745

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070622\
Data File : BP010926.D
Acq On : 06 Jul 2022 12:39
Operator : CG/JU
Sample : PB145967BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK967

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

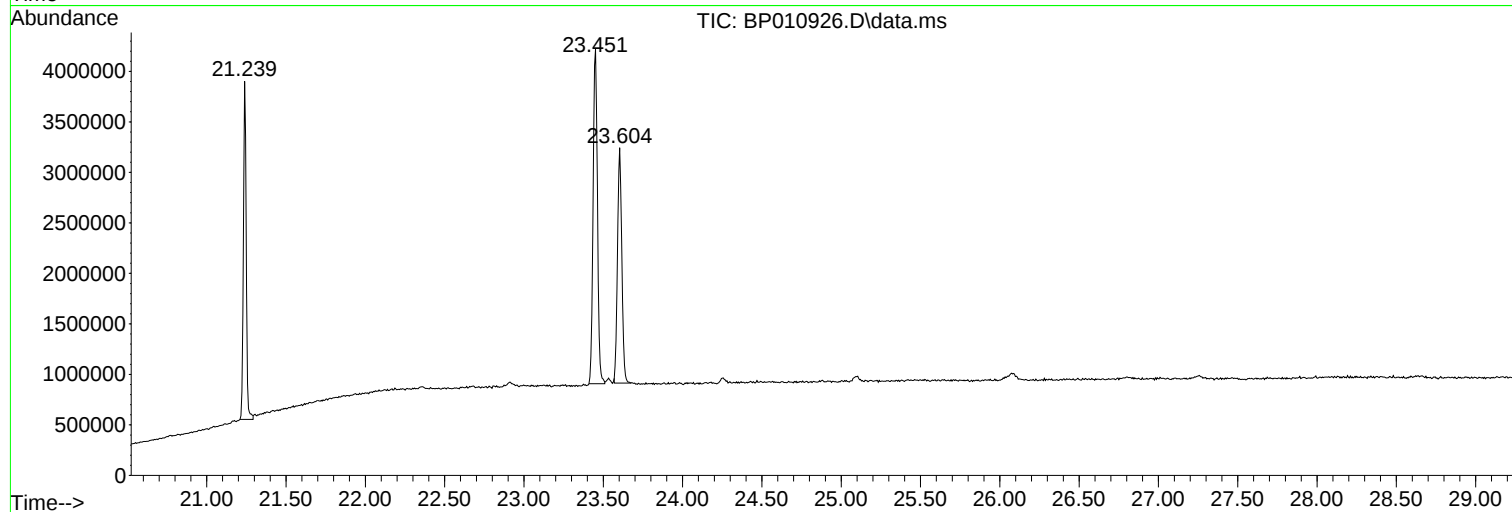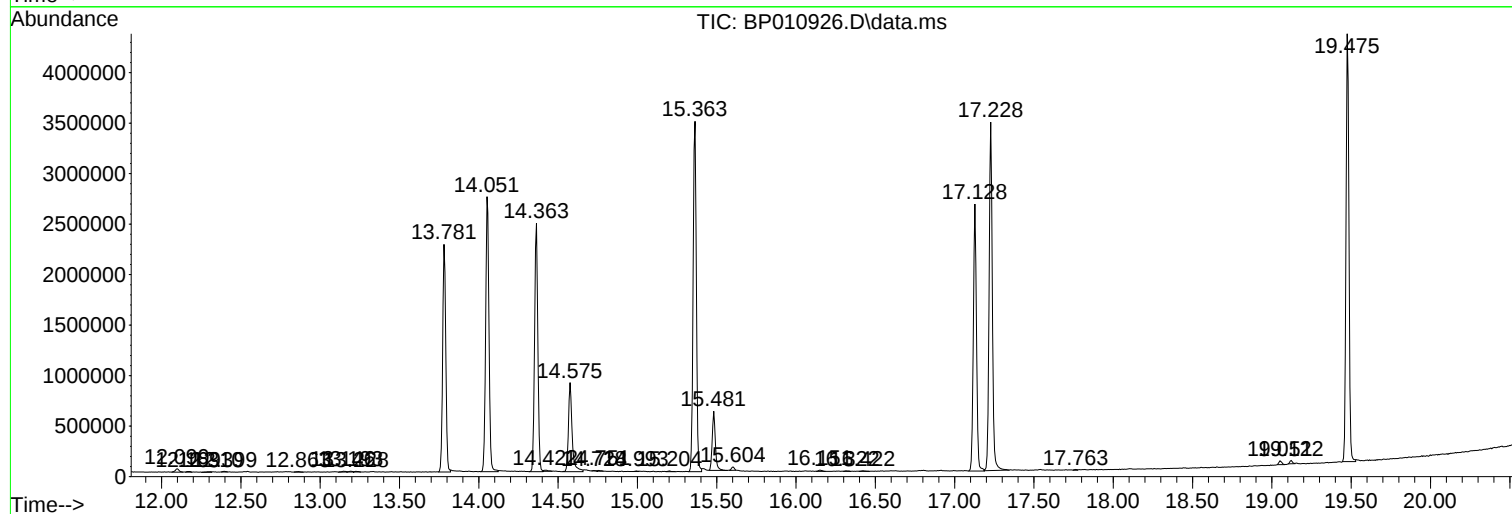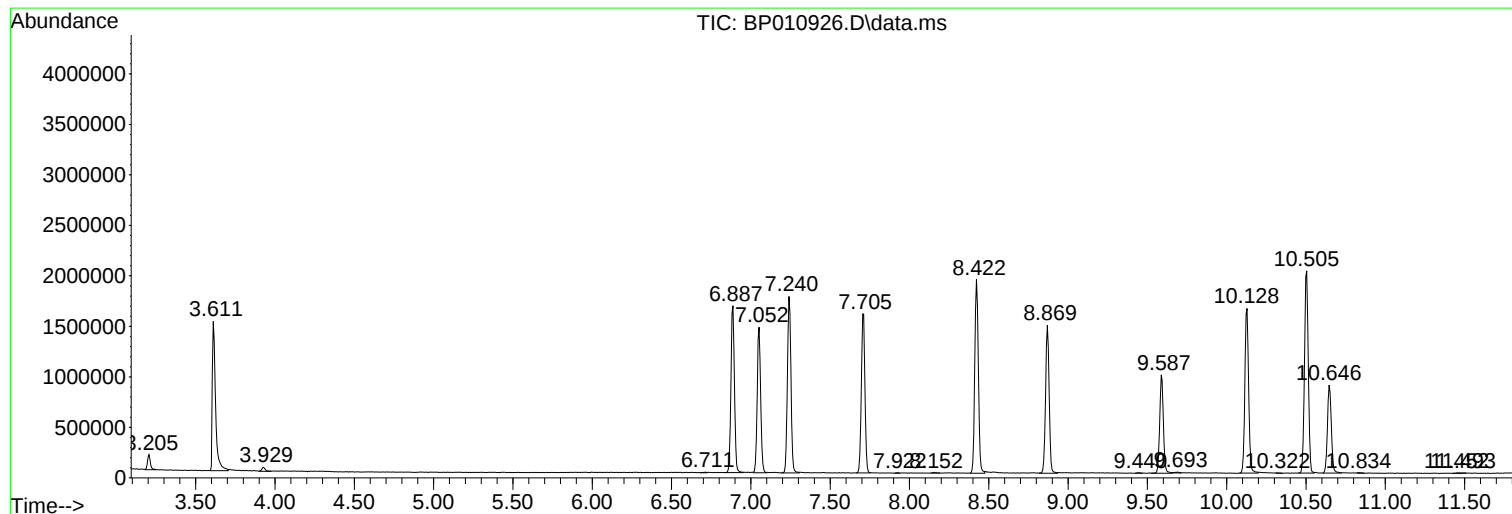

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070622\
Data File : BP010926.D
Acq On : 06 Jul 2022 12:39
Operator : CG/JU
Sample : PB145967BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK967

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070622\
Data File : BP010926.D
Acq On : 06 Jul 2022 12:39
Operator : CG/JU
Sample : PB145967BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK967

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------