

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070622\
 Data File : BP010928.D
 Acq On : 06 Jul 2022 13:48
 Operator : CG/JU
 Sample : N3574-10
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010928.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.652	93	96	104	rBV5	13201	31561	0.71%	0.132%
2	3.922	138	142	146	rBV	34426	44622	1.01%	0.187%
3	6.658	603	607	610	rBV6	2812	5231	0.12%	0.022%
4	7.040	669	672	677	rVB6	2854	4722	0.11%	0.020%
5	7.240	700	706	708	rBV6	3833	6588	0.15%	0.028%
6	7.705	776	785	795	rBV	1772890	2704759	61.25%	11.335%
7	8.869	979	983	986	rBV6	2767	4657	0.11%	0.020%
8	8.899	986	988	994	rVB7	3284	6068	0.14%	0.025%
9	10.128	1190	1197	1199	rBV8	4397	9306	0.21%	0.039%
10	10.498	1252	1260	1269	rBV	2319344	3741235	84.73%	15.679%
11	12.169	1538	1544	1550	rVB	5899	10663	0.24%	0.045%
12	12.393	1575	1582	1589	rVB10	5678	11592	0.26%	0.049%
13	12.775	1645	1647	1651	rBV5	4241	6916	0.16%	0.029%
14	12.851	1656	1660	1663	rBV6	3653	5146	0.12%	0.022%
15	13.081	1696	1699	1703	rBV6	3882	5829	0.13%	0.024%
16	13.145	1706	1710	1715	rVV8	4028	7810	0.18%	0.033%
17	13.187	1715	1717	1720	rVV4	5879	7461	0.17%	0.031%
18	13.228	1722	1724	1731	rVB8	6035	8759	0.20%	0.037%
19	13.792	1815	1820	1823	rVB7	4614	7998	0.18%	0.034%
20	14.045	1859	1863	1866	rBV3	6682	13415	0.30%	0.056%
21	14.069	1866	1867	1875	rVB5	5299	9015	0.20%	0.038%
22	14.357	1909	1916	1925	rBV	2886770	4116021	93.21%	17.250%
23	14.539	1944	1947	1951	rVB6	3349	5033	0.11%	0.021%
24	14.675	1966	1970	1973	rVB6	4496	5656	0.13%	0.024%
25	14.763	1979	1985	1987	rVB7	5164	6425	0.15%	0.027%
26	15.357	2082	2086	2090	rBV7	8157	14107	0.32%	0.059%
27	15.410	2092	2095	2100	rVB6	8456	11354	0.26%	0.048%
28	16.322	2244	2250	2251	rBV6	3752	4438	0.10%	0.019%
29	16.910	2346	2350	2355	rVB5	6605	10438	0.24%	0.044%
30	17.122	2379	2386	2401	rBV	2861047	4277215	96.87%	17.925%
31	21.233	3080	3085	3094	rBV	3640771	4415635	100.00%	18.506%
32	23.592	3480	3486	3496	rVB2	2167721	4341517	98.32%	18.195%




Sum of corrected areas: 23861192

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070622\
Data File : BP010928.D
Acq On : 06 Jul 2022 13:48
Operator : CG/JU
Sample : N3574-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

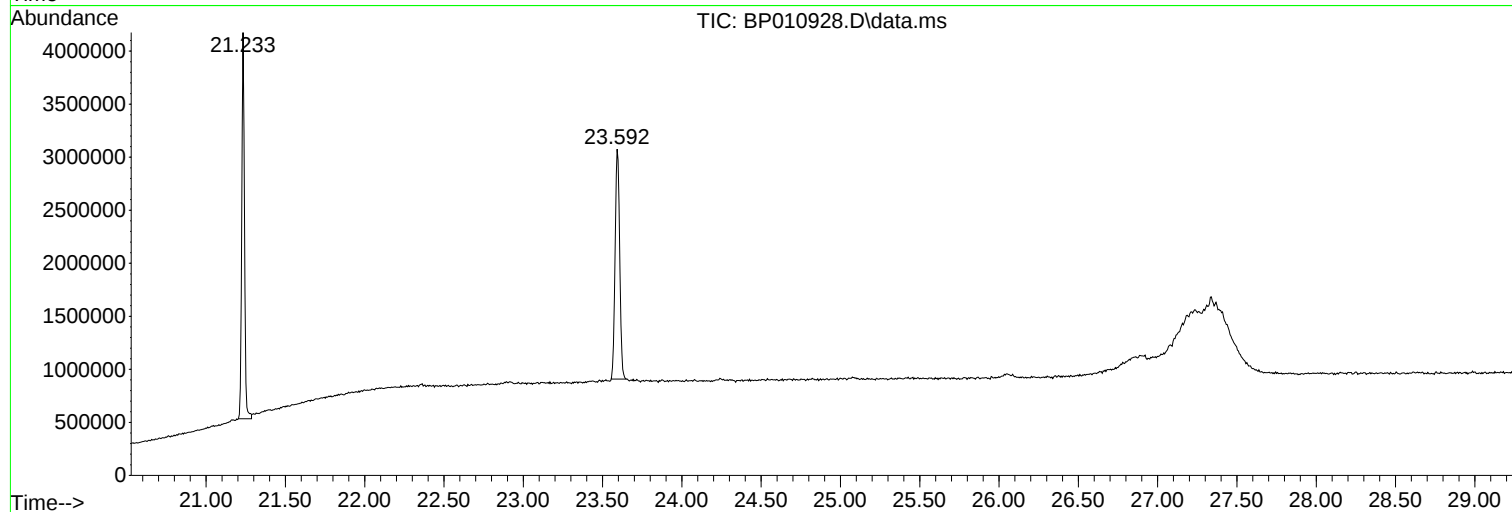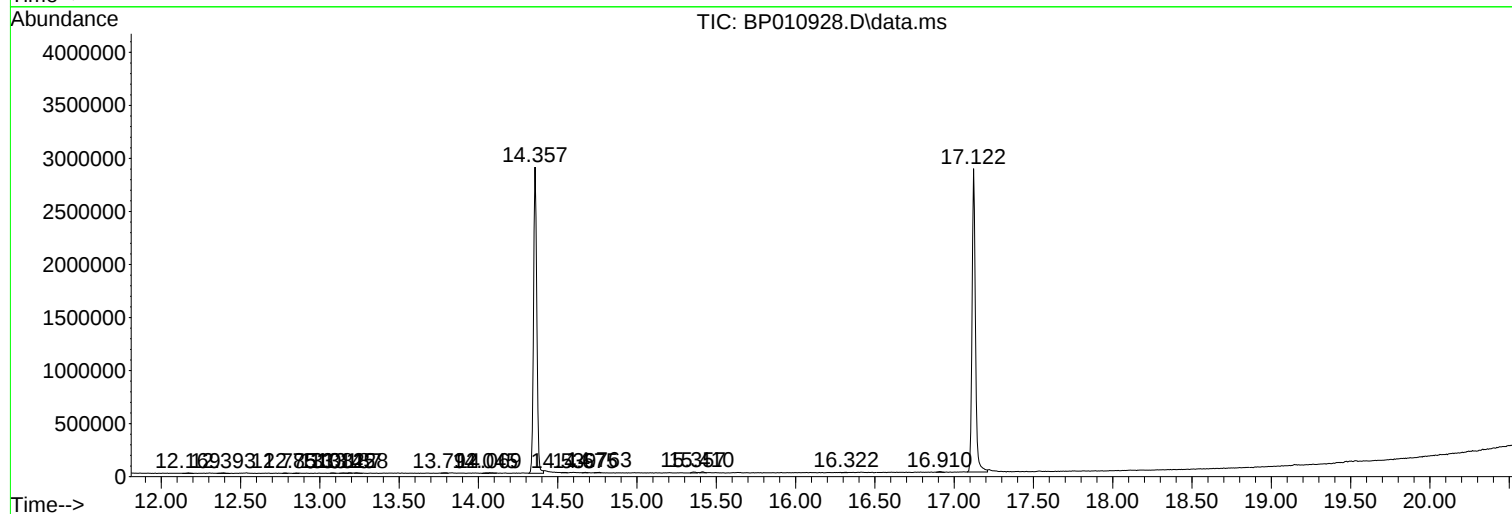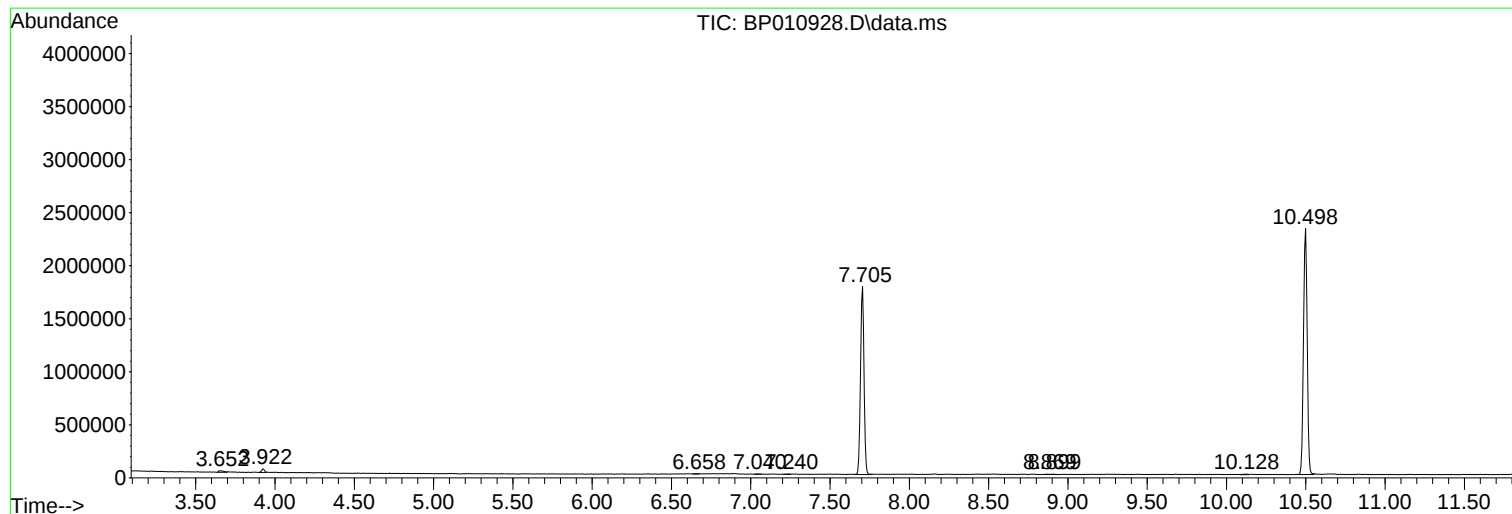

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070622\
Data File : BP010928.D
Acq On : 06 Jul 2022 13:48
Operator : CG/JU
Sample : N3574-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070622\
Data File : BP010928.D
Acq On : 06 Jul 2022 13:48
Operator : CG/JU
Sample : N3574-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc