

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP070720\
 Data File : BP002659.D
 Acq On : 07 Jul 2020 15:49
 Operator : CG/JU
 Sample : L3202-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 RO-COMP

Quant Time: Jul 07 16:44:12 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP062920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 29 16:51:57 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	216165	20.00	ng	0.00
21) Naphthalene-d8	10.34	136	841462	20.00	ng	0.00
39) Acenaphthene-d10	14.22	164	523757	20.00	ng	0.00
64) Phenanthrene-d10	16.97	188	1135843	20.00	ng	0.00
76) Chrysene-d12	21.08	240	1223386	20.00	ng	-0.01
86) Perylene-d12	23.27	264	1307277	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.19	112	1158790	90.76	ng	0.00
7) Phenol-d6	6.76	99	1625612	91.22	ng	0.00
23) Nitrobenzene-d5	8.71	82	1045917	64.04	ng	-0.01
42) 2,4,6-Tribromophenol	15.72	330	709310	111.35	ng	-0.01
45) 2-Fluorobiphenyl	12.83	172	2469836	69.41	ng	0.00
79) Terphenyl-d14	19.57	244	3840663	67.76	ng	0.00
Target Compounds						
50) Dimethylphthalate	13.68	163	220533	5.361	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP070720\
Data File : BP002659.D
Acq On : 07 Jul 2020 15:49
Operator : CG/JU
Sample : L3202-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
RO-COMP

Quant Time: Jul 07 16:44:12 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP062920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 29 16:51:57 2020
Response via : Initial Calibration

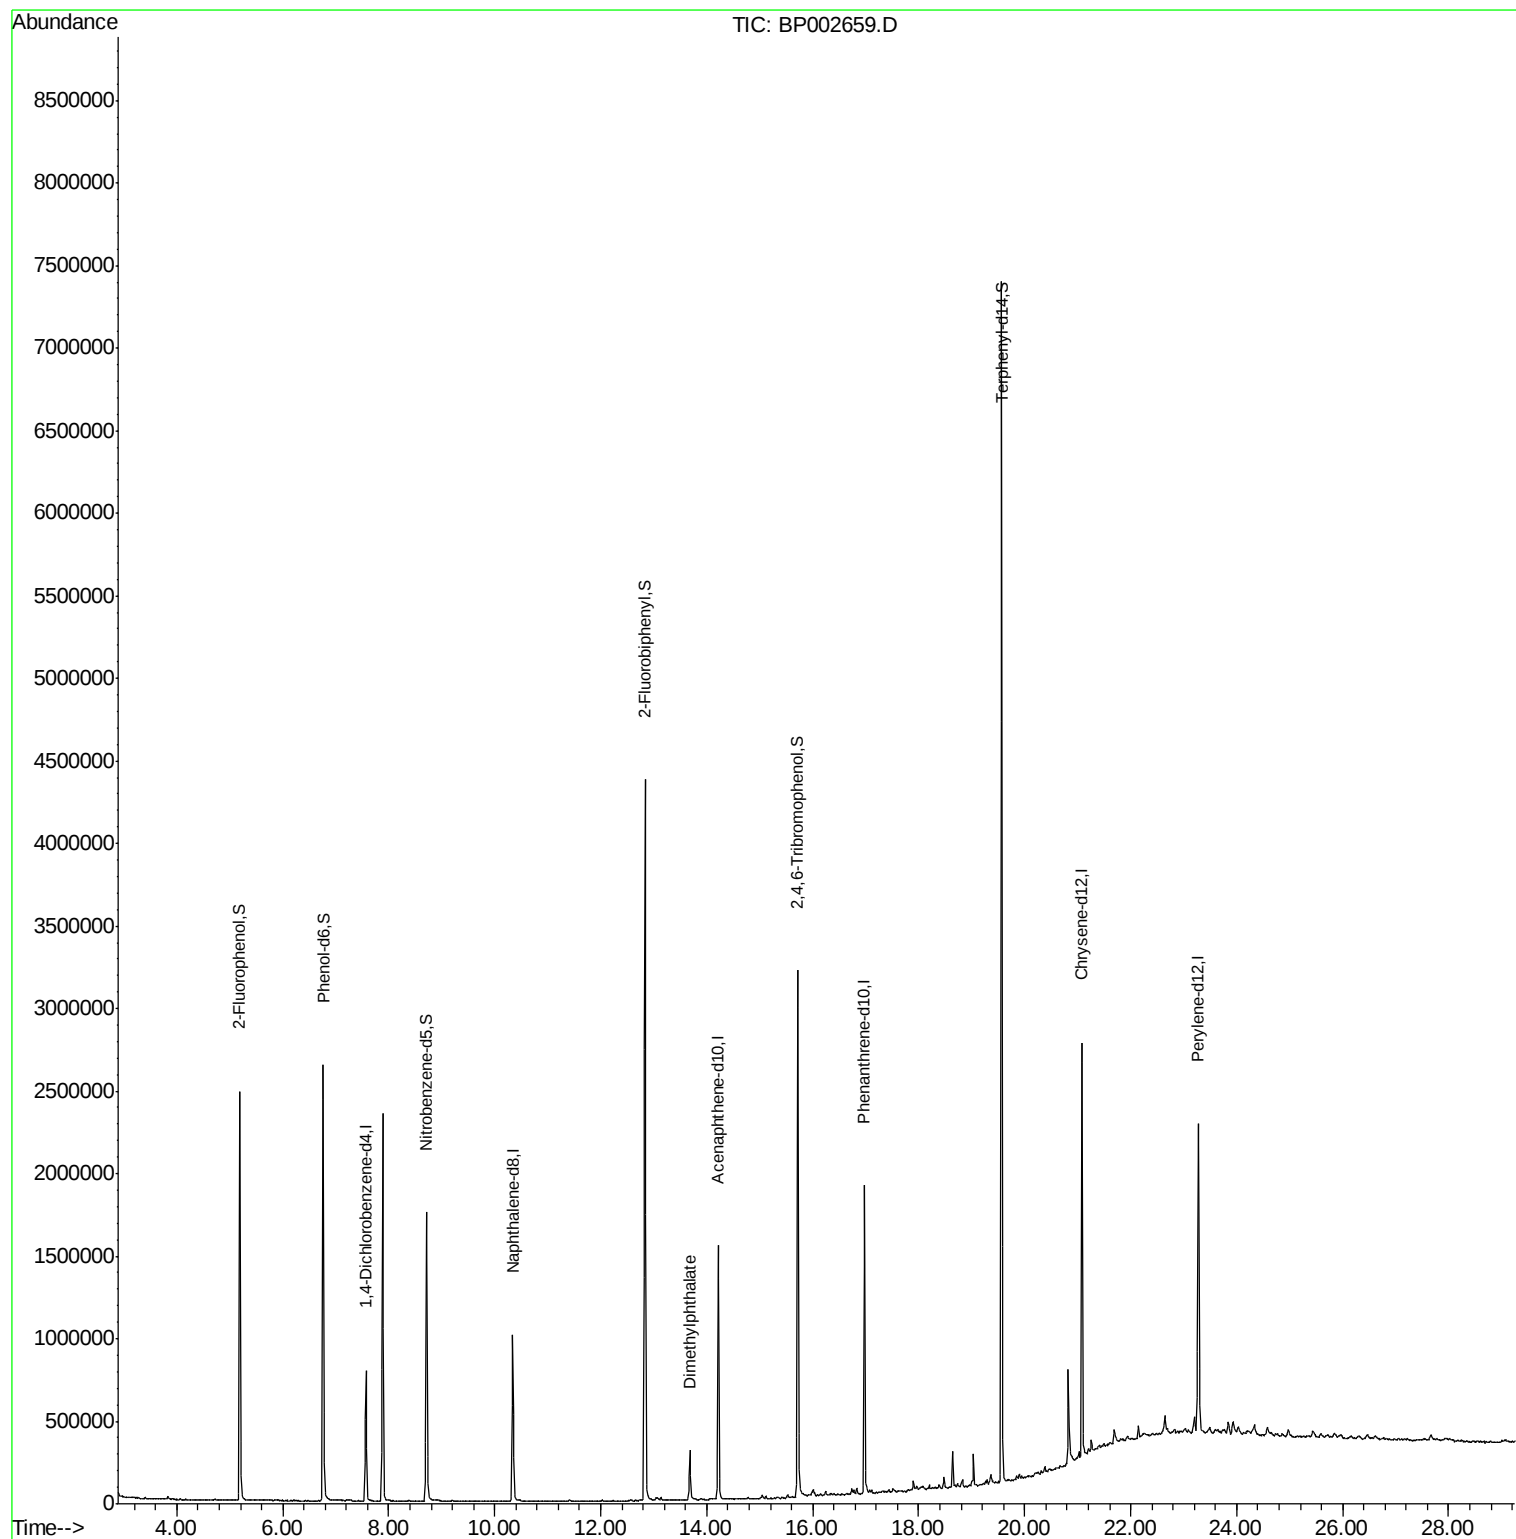

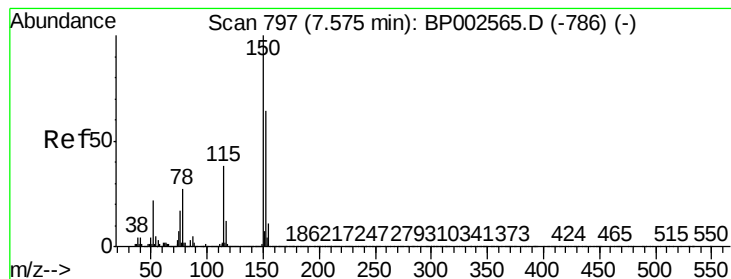


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.57 min Scan# 796
Delta R.T. -0.01 min
Lab File: BP002659.D
Acq: 07 Jul 2020 15:49

Instrument :
BNA_P
ClientSampleId :
RO-COMP

Tot Ion	Ratio	Lower	Upper
152	100		
150	152.3	124.2	186.2
115	54.7	47.1	70.7




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

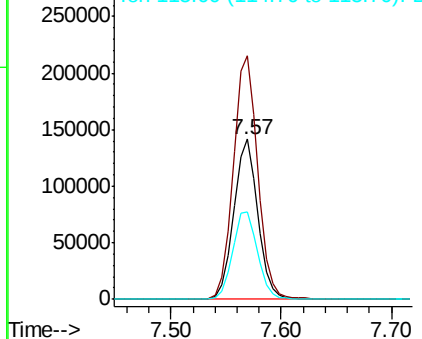



#5


2-Fluorophenol
Concen: 90.762 ng
RT: 5.19 min Scan# 392
Delta R.T. -0.00 min
Lab File: BP002659.D
Acq: 07 Jul 2020 15:49

Tgt Ion	Ratio	Lower	Upper
112	100		
64	55.7	47.0	70.6
63	28.6	26.1	39.1



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BP0
Ion 63.00 (62.70 to 63.70): BP0

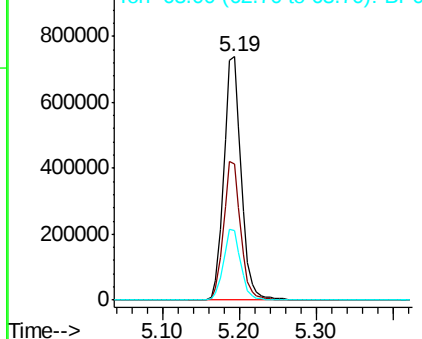

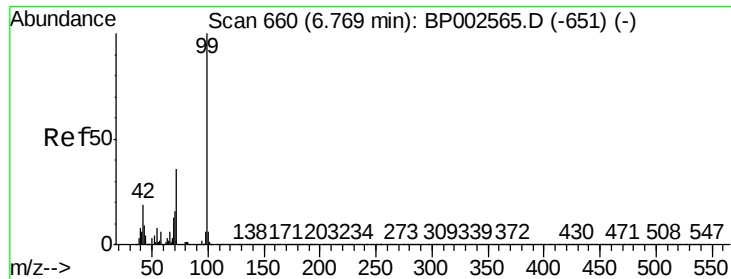

#7

Phenol-d6

Concen: 91.225 ng

RT: 6.76 min Scan# 659

Delta R.T. -0.01 min

Lab File: BP002659.D

Acq: 07 Jul 2020 15:49

Instrument :

BNA_P

ClientSampled :

RO-COMP


Tot Ion: 99 Resp: 1625612

Ion Ratio Lower Upper

99 100

42 16.8 15.5 23.3




71 31.7 28.9 43.3



Abundance Ion 99.00 (98.70 to 99.70): BP0

Ion 42.00 (41.70 to 42.70): BP0

Ion 71.00 (70.70 to 71.70): BP0

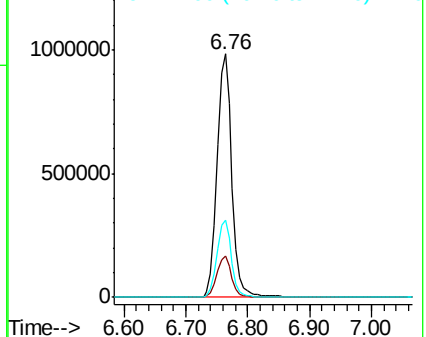

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.34 min Scan# 1267

Delta R.T. -0.01 min

Lab File: BP002659.D

Acq: 07 Jul 2020 15:49

Tgt Ion: 136 Resp: 841462


Ion Ratio Lower Upper

136 100

137 10.9 8.8 13.2

54 8.1 6.4 9.6

68 7.0 5.1 7.7






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BP0

Ion 68.00 (67.70 to 68.70): BP0




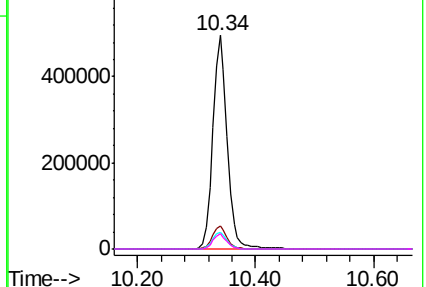


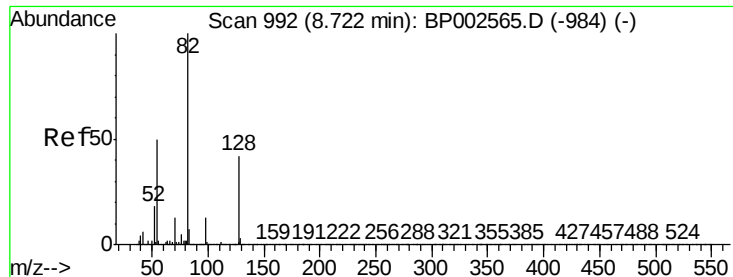

#23
Nitrobenzene-d5
Concen: 64.045 ng
RT: 8.71 min Scan# 990
Delta R.T. -0.01 min
Lab File: BP002659.D
Acq: 07 Jul 2020 15:49




Instrument :
BNA_P
ClientSampleId :
RO-COMP


Tot Ion: 82 Resp: 1045917
Ion Ratio Lower Upper
82 100
128 43.1 33.4 50.2
54 47.7 40.1 60.1

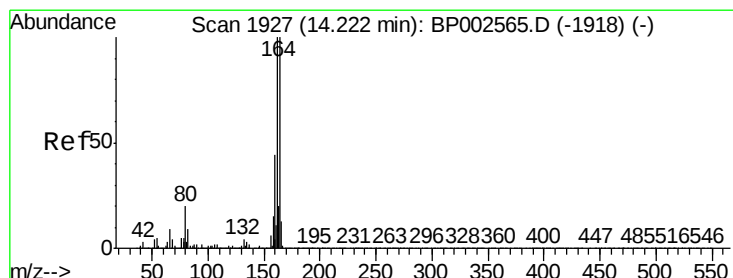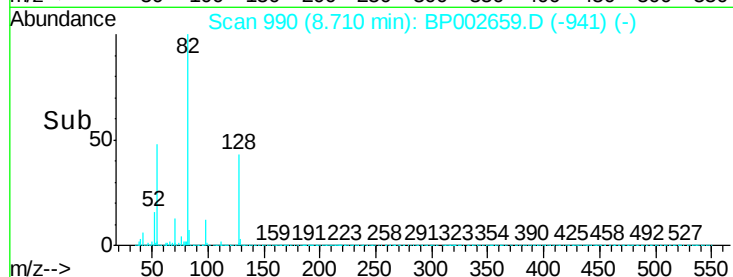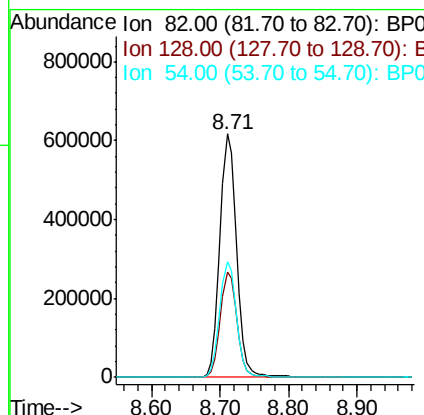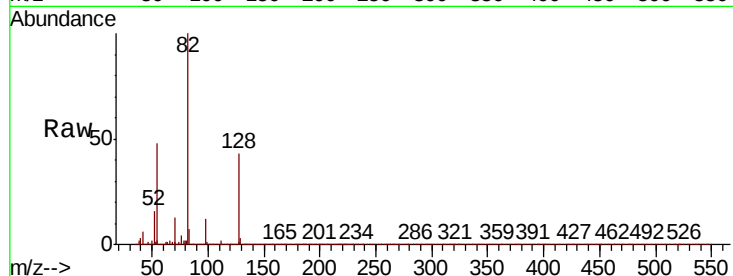

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.22 min Scan# 1926
Delta R.T. -0.01 min
Lab File: BP002659.D
Acq: 07 Jul 2020 15:49

Tgt Ion: 164 Resp: 523757
Ion Ratio Lower Upper
164 100
162 101.1 80.3 120.5
160 45.2 35.0 52.6


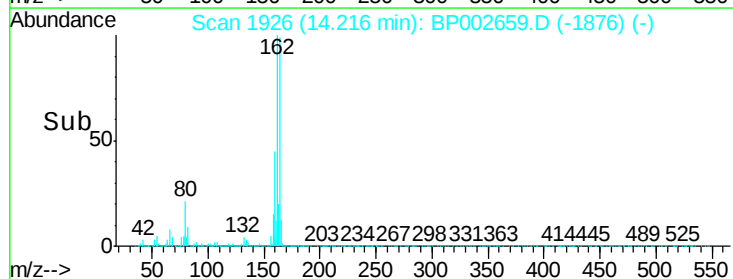
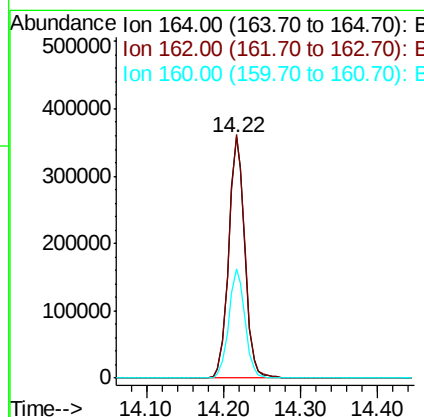
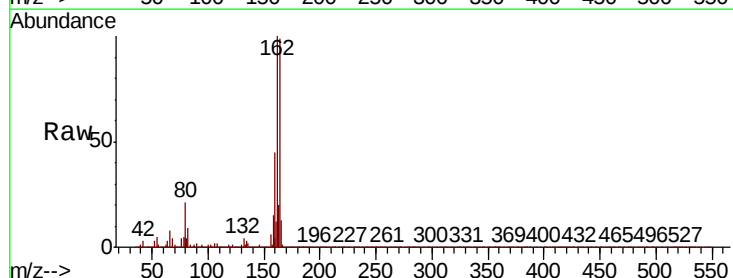


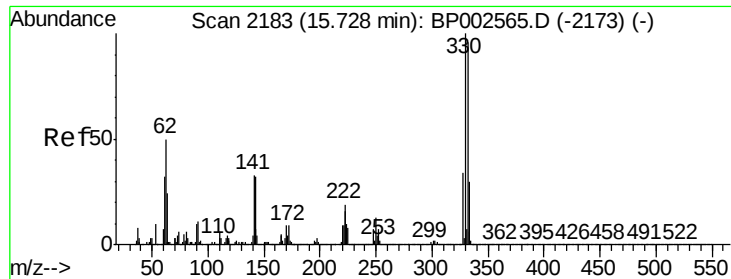

#42
 2,4,6-Tribromophenol
 Concen: 111.345 ng
 RT: 15.72 min Scan# 2181
 Delta R.T. -0.01 min
 Lab File: BP002659.D
 Acq: 07 Jul 2020 15:49




Instrument :
 BNA_P
 ClientSampleId :
 RO-COMP


Tot Ion:330 Resp: 709310
 Ion Ratio Lower Upper
 330 100
 332 97.0 77.7 116.5
 141 27.8 29.0 43.6#

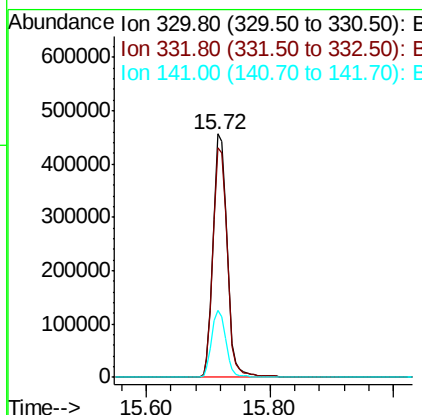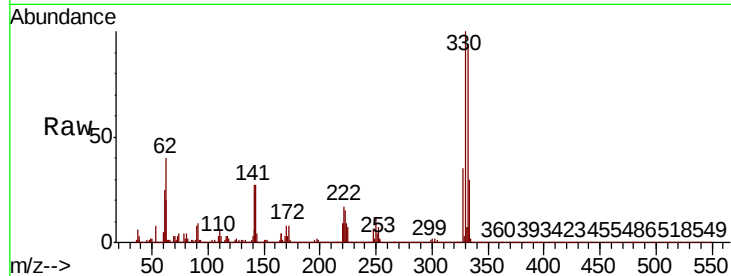

#45
 2-Fluorobiphenyl
 Concen: 69.406 ng
 RT: 12.83 min Scan# 1691
 Delta R.T. -0.01 min
 Lab File: BP002659.D
 Acq: 07 Jul 2020 15:49

Tgt Ion:172 Resp: 2469836
 Ion Ratio Lower Upper
 172 100
 171 35.1 28.0 42.0
 170 24.0 19.0 28.4



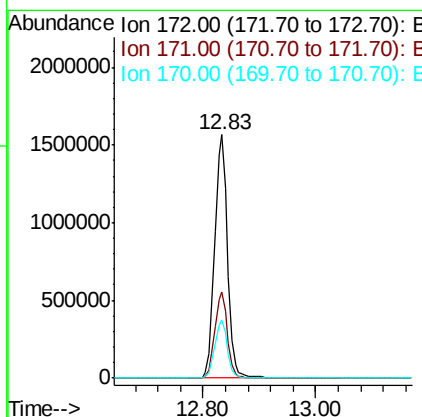



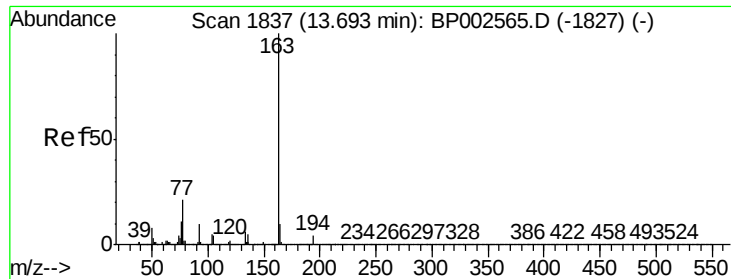

#50
Dimethylphthalate
Concen: 5.361 ng
RT: 13.68 min Scan# 1835
Delta R.T. -0.01 min
Lab File: BP002659.D
Acq: 07 Jul 2020 15:49




Instrument :
BNA_P
ClientSampleId :
RO-COMP


Tot Ion:163 Resp: 220533
Ion Ratio Lower Upper
163 100
194 4.5 3.4 5.0
164 10.4 8.2 12.4

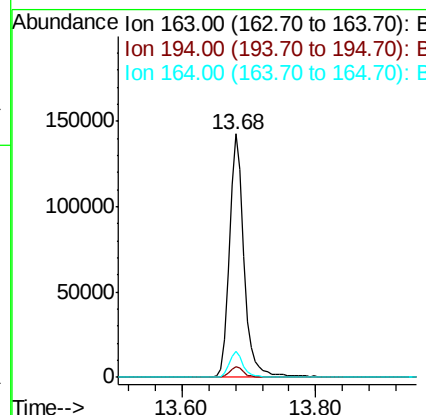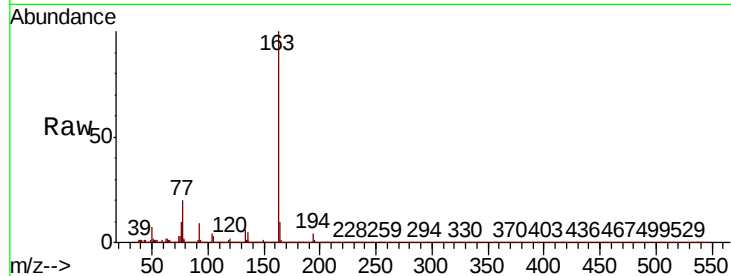

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 16.97 min Scan# 2395
Delta R.T. -0.01 min
Lab File: BP002659.D
Acq: 07 Jul 2020 15:49

Tgt Ion:188 Resp: 1135843
Ion Ratio Lower Upper
188 100
94 9.4 7.8 11.6
80 10.3 8.2 12.4



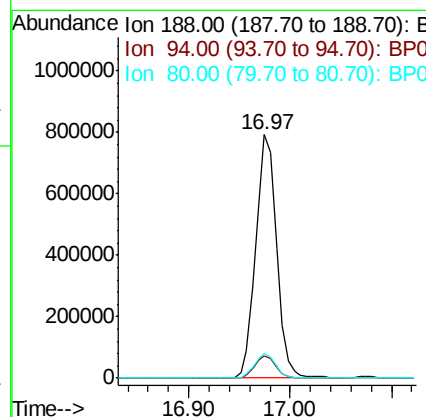





#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.08 min Scan# 3093
Delta R.T. -0.01 min
Lab File: BP002659.D
Acq: 07 Jul 2020 15:49




Instrument :
BNA_P
ClientSampleId :
RO-COMP


Tot Ion:240 Resp: 1223386
Ion Ratio Lower Upper
240 100
120 10.2 8.6 13.0
236 25.4 20.8 31.2

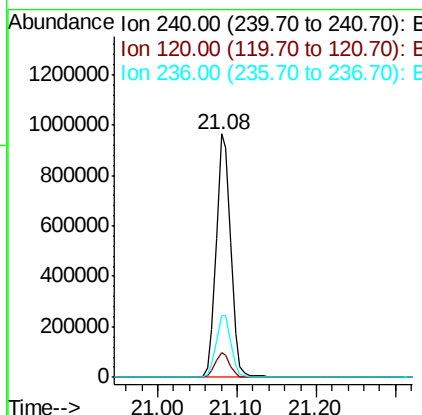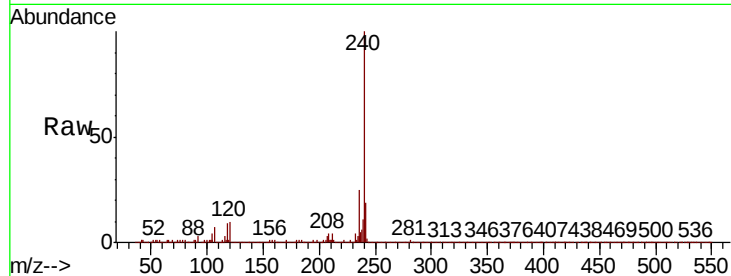

#79
Terphenyl-d14
Concen: 67.763 ng
RT: 19.57 min Scan# 2836
Delta R.T. -0.01 min
Lab File: BP002659.D
Acq: 07 Jul 2020 15:49

Tgt Ion:244 Resp: 3840663
Ion Ratio Lower Upper
244 100
212 7.0 6.5 9.7
122 9.1 7.9 11.9

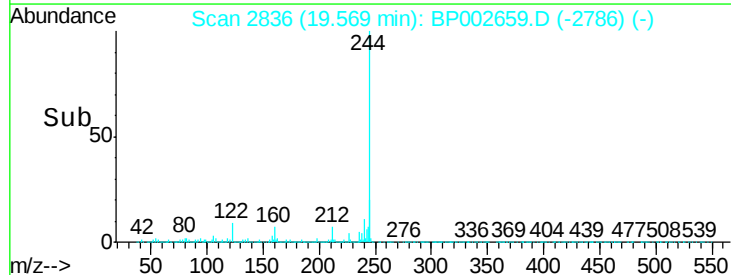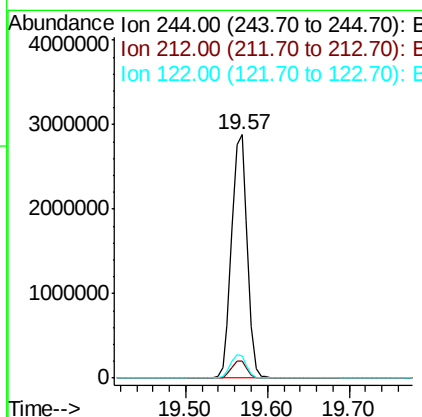



#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 23.27 min Scan# 3466
 Delta R.T. -0.01 min
 Lab File: BP002659.D
 Acq: 07 Jul 2020 15:49

Instrument :
 BNA_P
 ClientSampleId :
 RO-COMP

Tot Ion:264 Resp: 1307277

Ion	Ratio	Lower	Upper
264	100		
260	24.6	19.7	29.5
265	21.6	17.6	26.4

