

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP070720\
Data File : BP002651.D
Acq On : 07 Jul 2020 11:11
Operator : CG/JU
Sample : PB129929BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129929BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.193	386	392	411	rBV	2838170	4213996	40.26%	7.680%
2	6.764	652	659	683	rBV	2608482	4236983	40.48%	7.722%
3	7.569	788	796	808	rBV	898775	1407553	13.45%	2.565%
4	7.887	842	850	870	rBV	3423594	5622112	53.71%	10.247%
5	8.716	982	991	1021	rBV	2424831	4226608	40.38%	7.703%
6	10.340	1259	1267	1287	rBV	979061	1780143	17.01%	3.244%
7	12.834	1683	1691	1715	rBV	5569104	8947310	85.48%	16.307%
8	14.216	1919	1926	1948	rBV	1459270	2262517	21.62%	4.124%
9	15.722	2175	2182	2216	rBV	2372018	4089676	39.07%	7.454%
10	16.981	2389	2396	2410	rBV	1545554	2457443	23.48%	4.479%
11	19.569	2830	2836	2849	rBV	7820032	10467078	100.00%	19.077%
12	21.086	3089	3094	3105	rBV	1951593	2517374	24.05%	4.588%
13	23.280	3460	3467	3483	rBV2	1358272	2639755	25.22%	4.811%




Sum of corrected areas: 54868548

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP070720\
Data File : BP002651.D
Acq On : 07 Jul 2020 11:11
Operator : CG/JU
Sample : PB129929BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129929BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP062920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

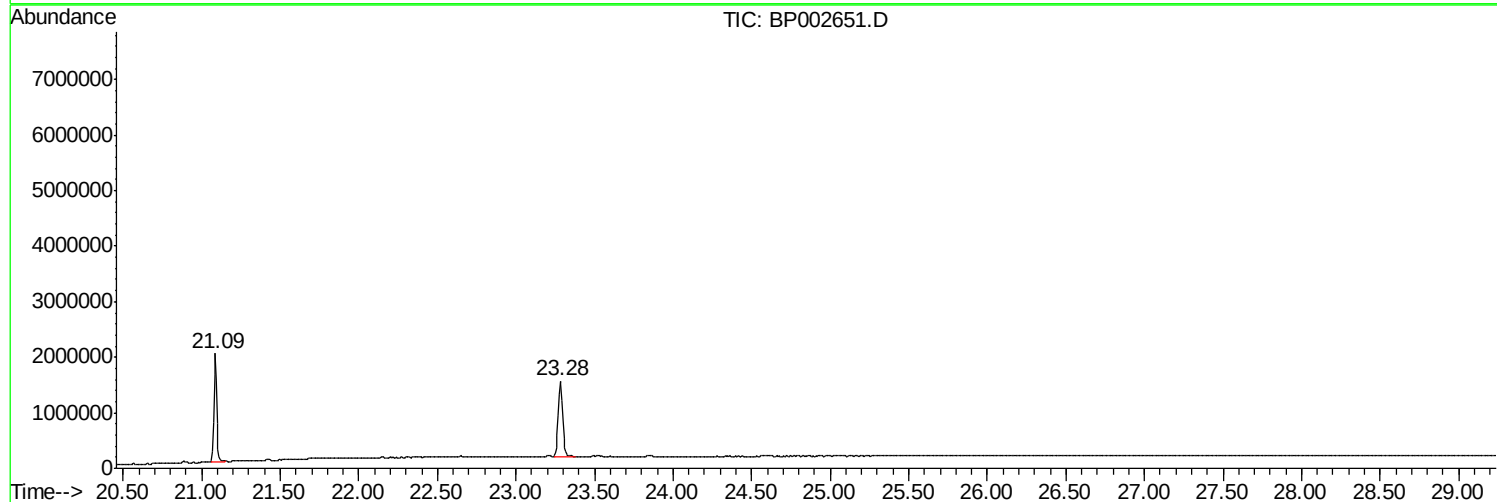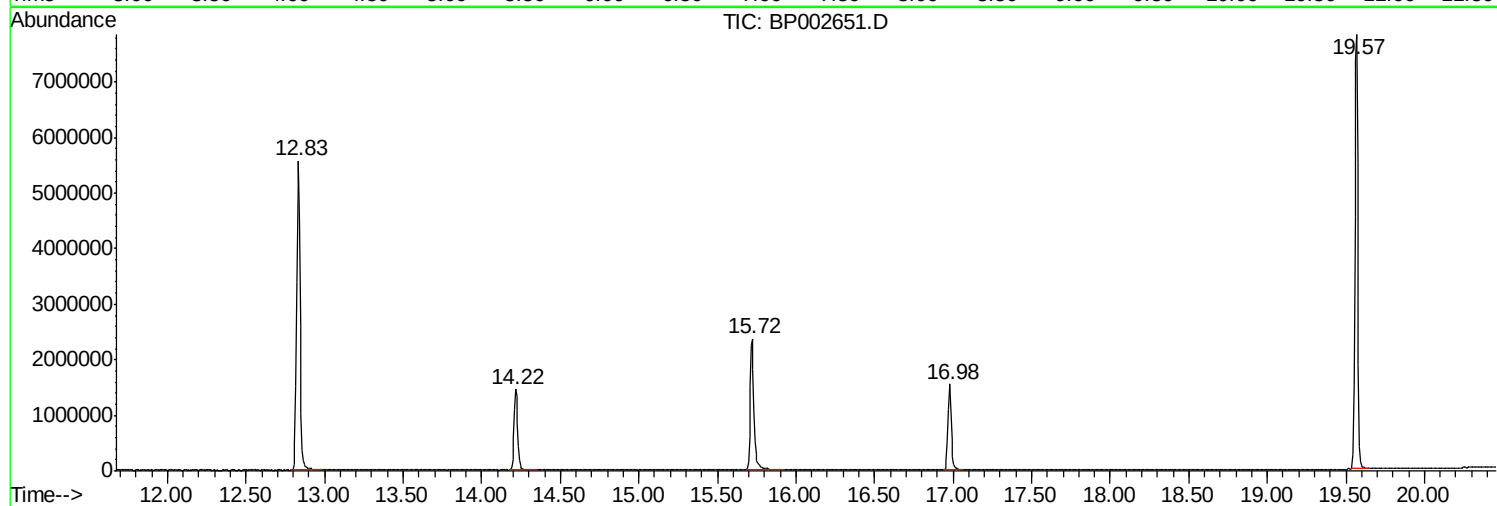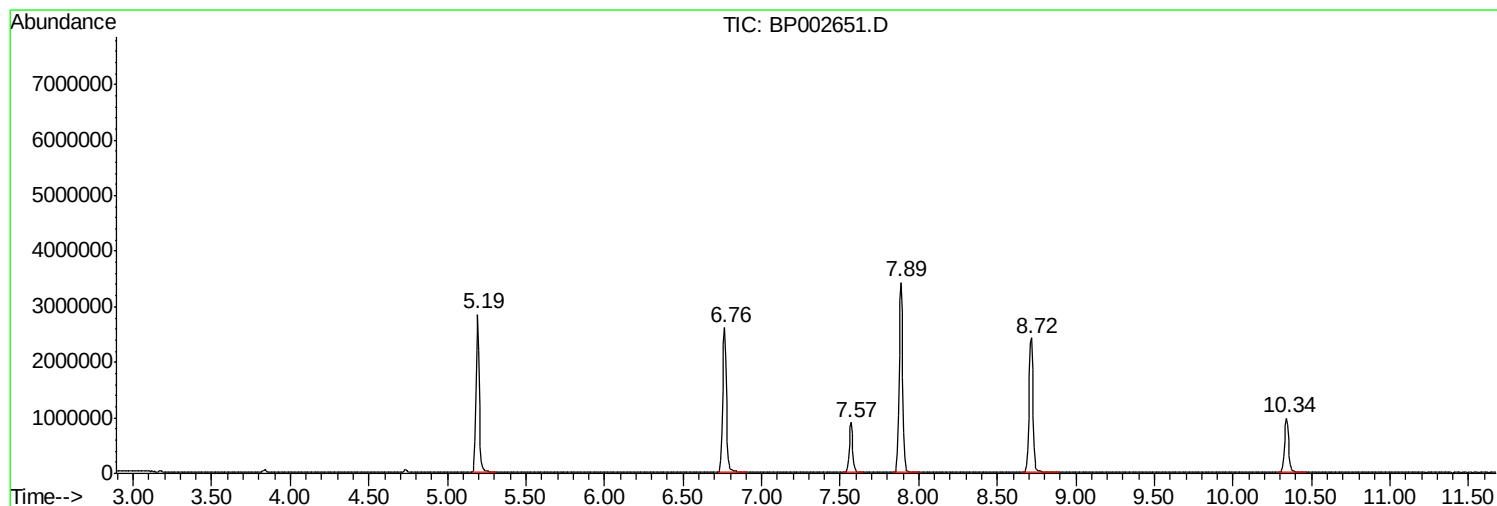

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP070720\
Data File : BP002651.D
Acq On : 07 Jul 2020 11:11
Operator : CG/JU
Sample : PB129929BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129929BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP070720\
Data File : BP002651.D
Acq On : 07 Jul 2020 11:11
Operator : CG/JU
Sample : PB129929BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129929BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc