

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP070720\
Data File : BP002652.D
Acq On : 07 Jul 2020 11:45
Operator : CG/JU
Sample : PB129955BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129955BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.187	385	391	414	rBV	3712584	5712038	52.43%	9.433%
2	6.763	651	659	678	rBV	3490521	5819035	53.41%	9.610%
3	7.569	789	796	807	rBV	822380	1332770	12.23%	2.201%
4	7.887	842	850	864	rBV	3288228	5412791	49.68%	8.939%
5	8.716	982	991	1014	rBV	2318726	4035878	37.04%	6.665%
6	10.340	1260	1267	1286	rBV	986730	1759142	16.15%	2.905%
7	12.834	1683	1691	1715	rBV	5469419	8914821	81.82%	14.723%
8	14.216	1918	1926	1944	rBV2	1446586	2278922	20.92%	3.764%
9	15.722	2175	2182	2215	rBV	3705631	6311728	57.93%	10.424%
10	16.975	2389	2395	2409	rBV	1591106	2526082	23.19%	4.172%
11	19.569	2830	2836	2855	rBV	8178627	10895026	100.00%	17.993%
12	21.086	3089	3094	3105	rBV	1977401	2633102	24.17%	4.349%
13	23.280	3460	3467	3481	rBV2	1515293	2919838	26.80%	4.822%




Sum of corrected areas: 60551173

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP070720\
Data File : BP002652.D
Acq On : 07 Jul 2020 11:45
Operator : CG/JU
Sample : PB129955BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129955BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP062920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

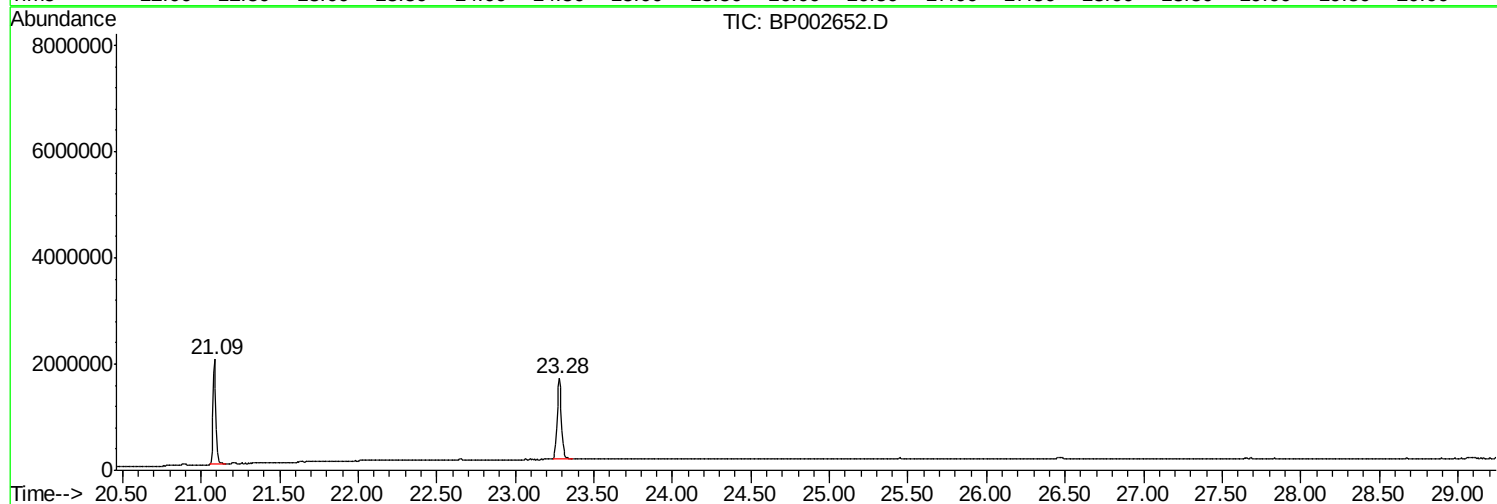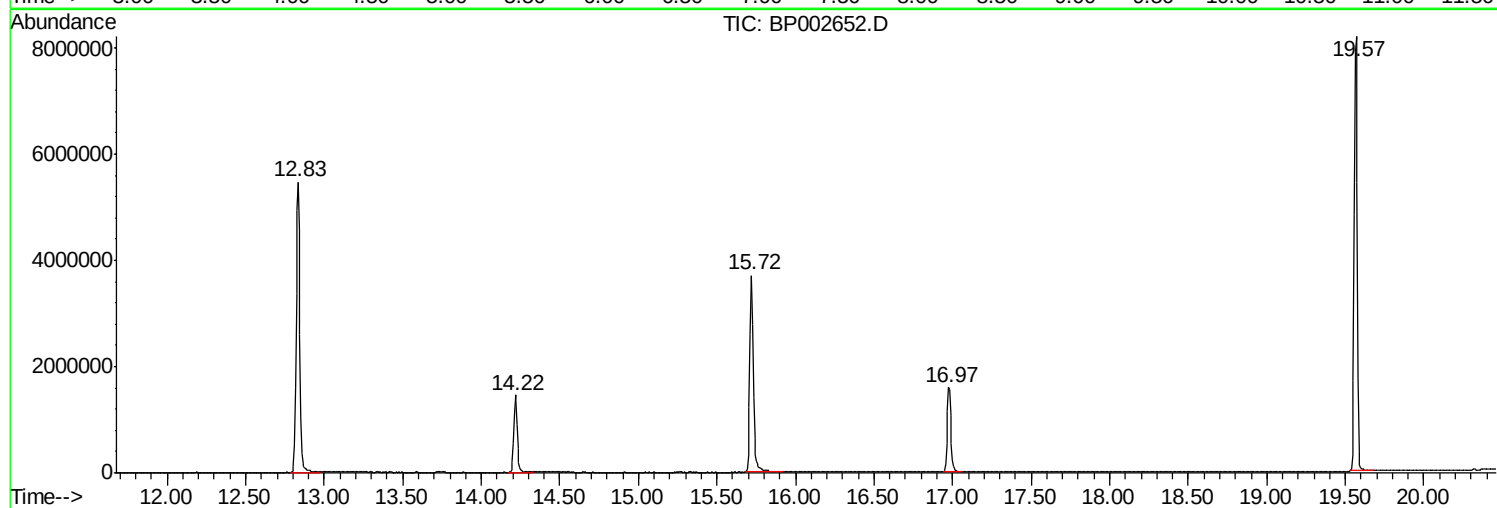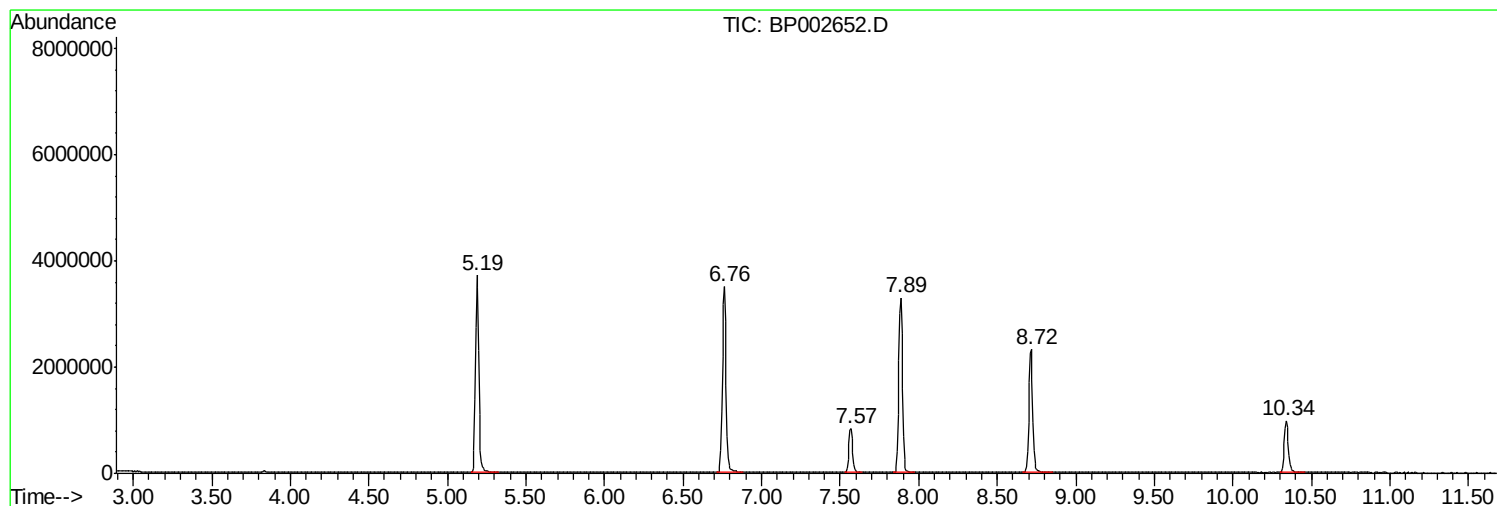

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP070720\
Data File : BP002652.D
Acq On : 07 Jul 2020 11:45
Operator : CG/JU
Sample : PB129955BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129955BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP070720\
Data File : BP002652.D
Acq On : 07 Jul 2020 11:45
Operator : CG/JU
Sample : PB129955BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129955BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc