


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070720\
 Data File : BP002647.D
 Acq On : 07 Jul 2020 08:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 29 16:51:57 2020

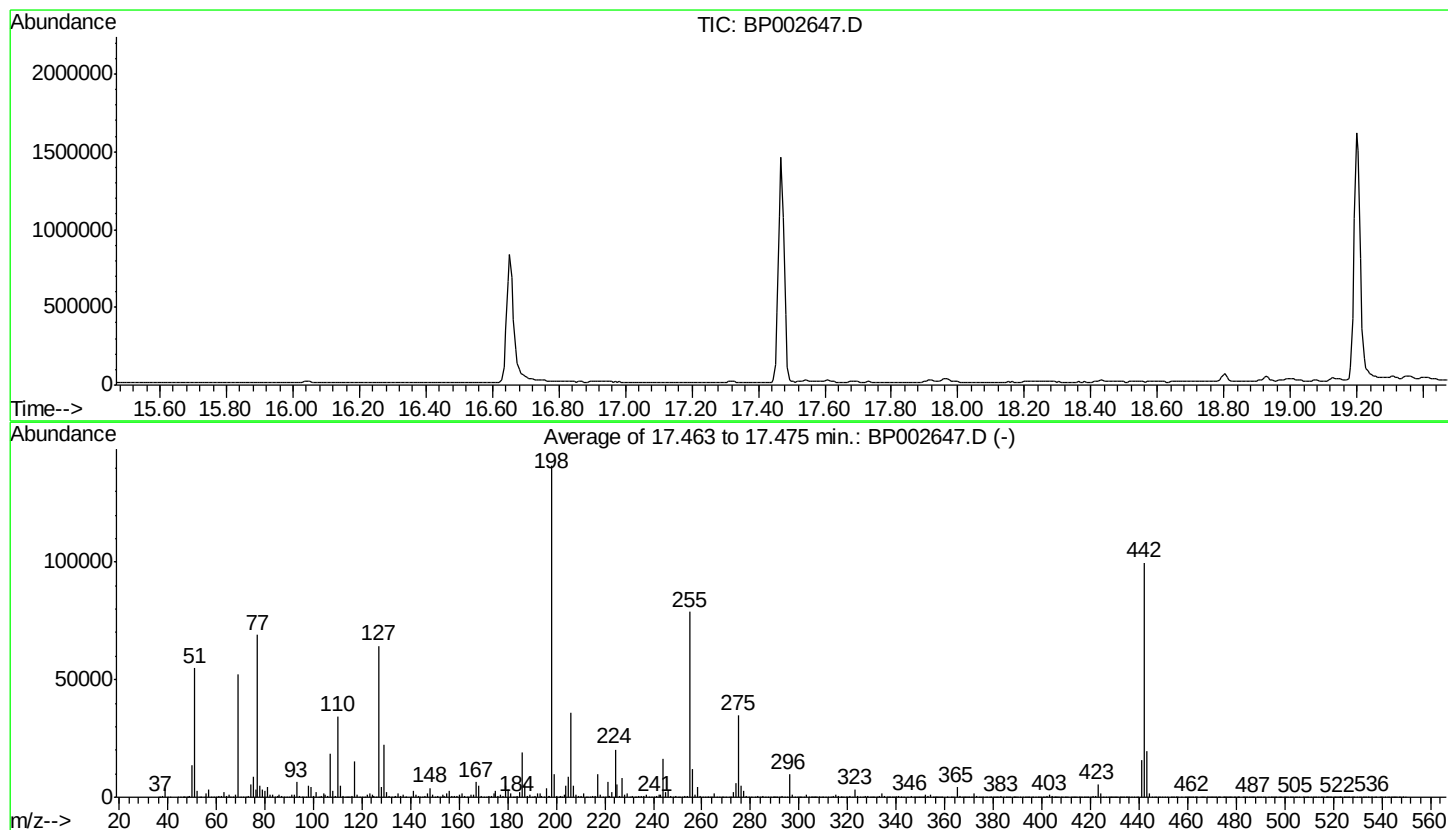

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.0	54983	PASS
68	69	0.00	2	1.8	921	PASS
69	198	0.00	100	37.2	52411	PASS
70	69	0.00	2	0.5	242	PASS
127	198	10	80	45.6	64337	PASS
197	198	0.00	2	0.3	454	PASS
198	198	100	100	100.0	141037	PASS
199	198	5	9	6.9	9762	PASS
275	198	10	60	24.6	34752	PASS
365	198	1	100	3.0	4169	PASS
441	198	0.01	100	11.1	15672	PASS
442	198	50	100	70.7	99743	PASS
443	442	15	24	19.8	19709	PASS