
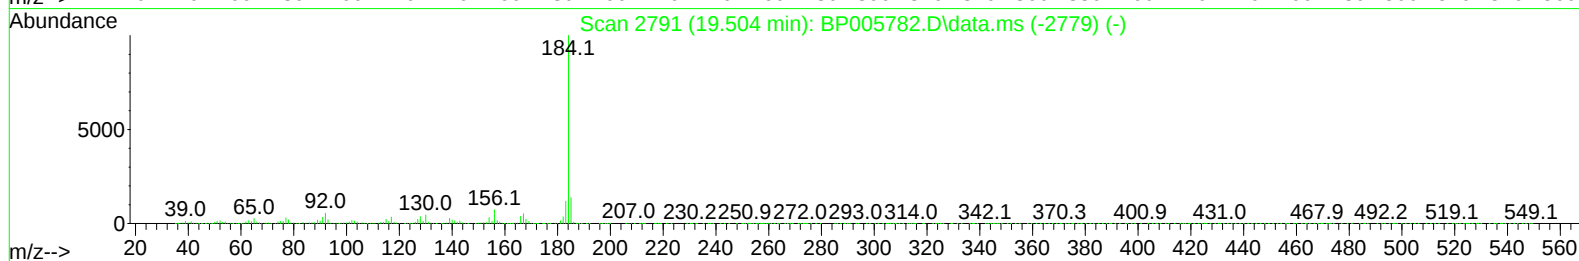
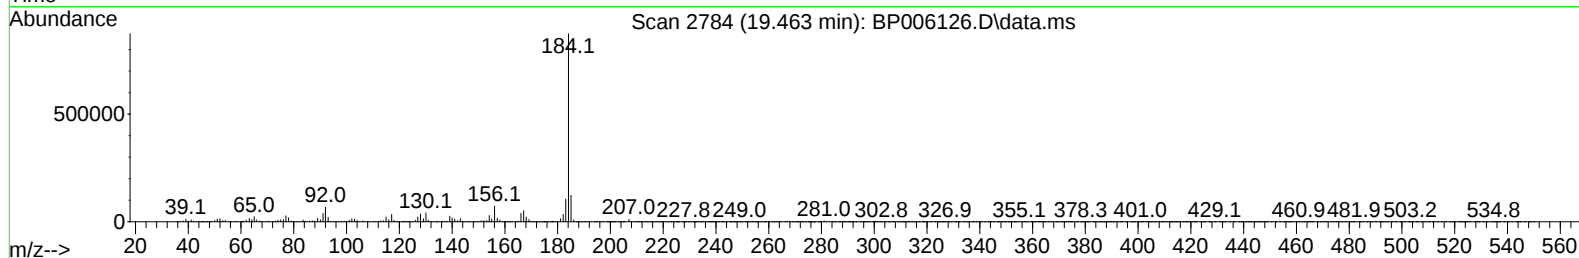


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070721\
Data File : BP006126.D
Acq On : 07 Jul 2021 10:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 07 11:28:29 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 07 11:23:35 2021
Response via : Initial Calibration

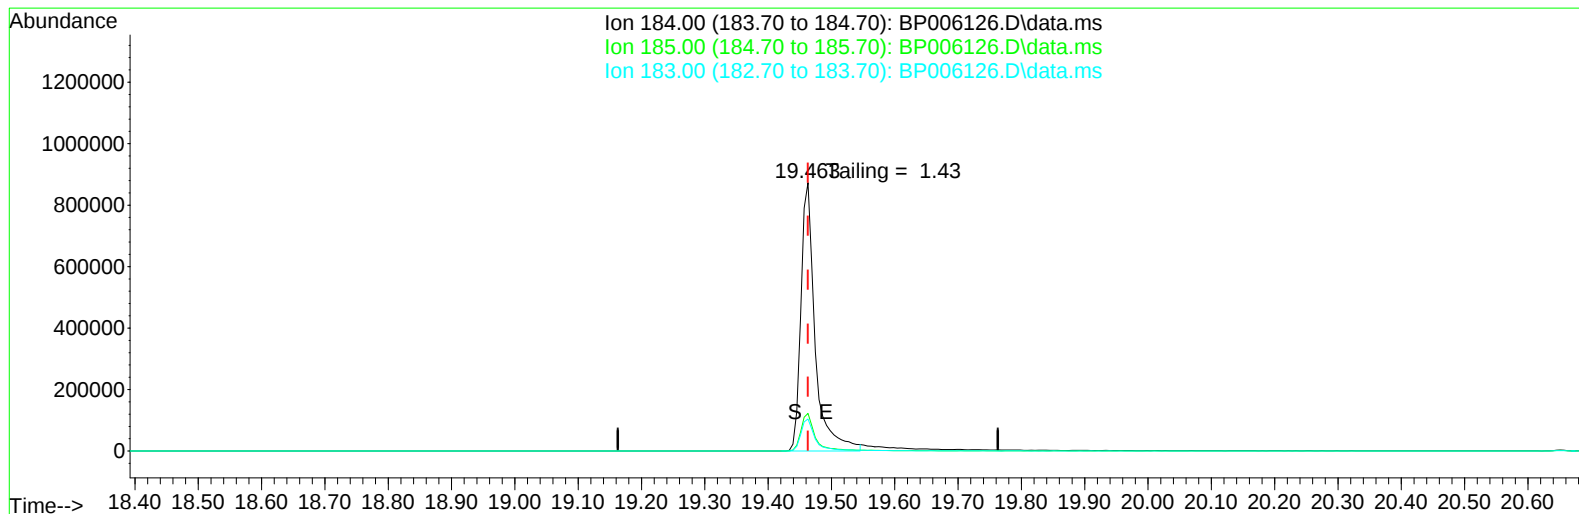




TIC: BP006126.D\data.ms

(77) Benzidine**19.463min (+ 0.000) 496360.91 ng****response 1445959**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.04
183.00	11.90	11.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070721\
 Data File : BP006126.D
 Acq On : 07 Jul 2021 10:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 07 11:28:29 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 07 11:23:35 2021
 Response via : Initial Calibration

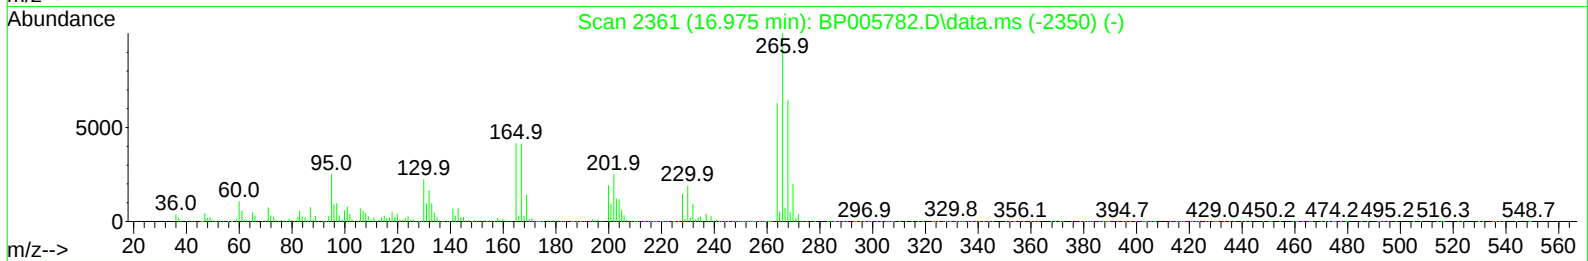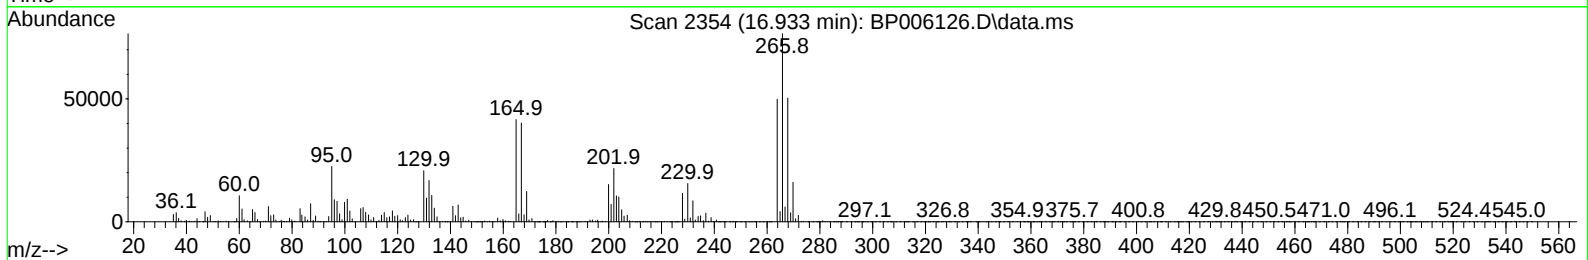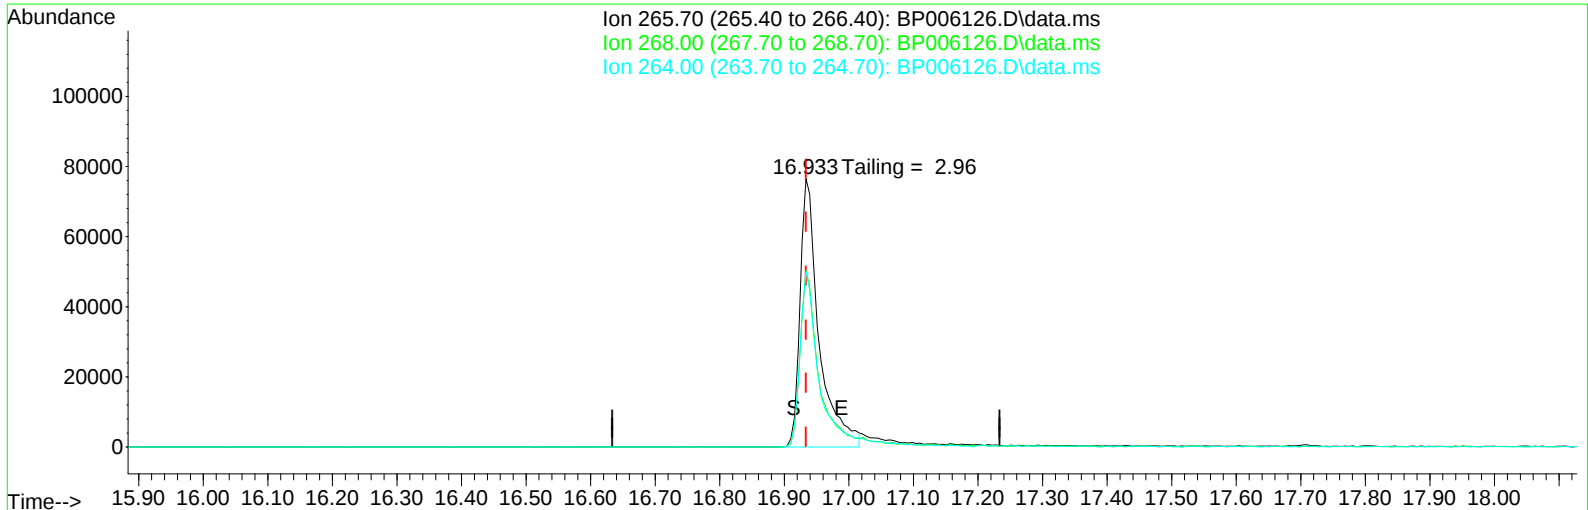

TIC: BP006126.D\data.ms

(70) Pentachlorophenol (C)

16.933min (+ 0.000) 1157649.88 ng

response 168351

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	65.75
264.00	62.90	65.22
0.00	0.00	0.00