
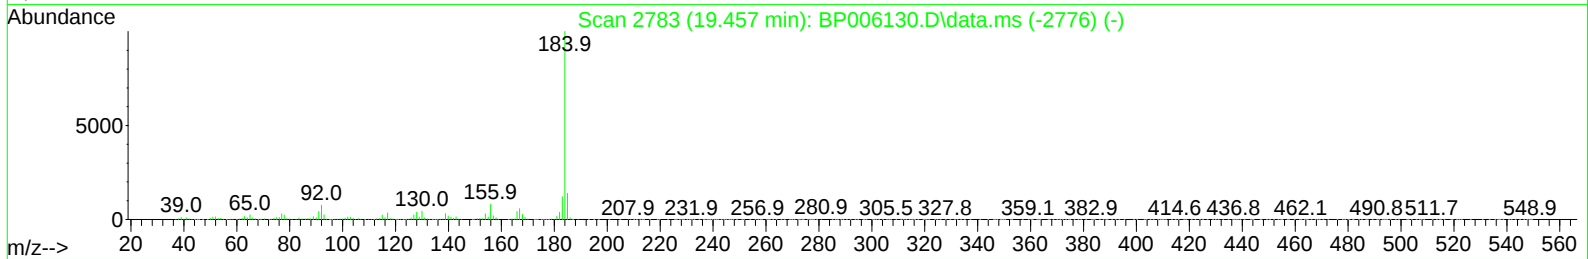
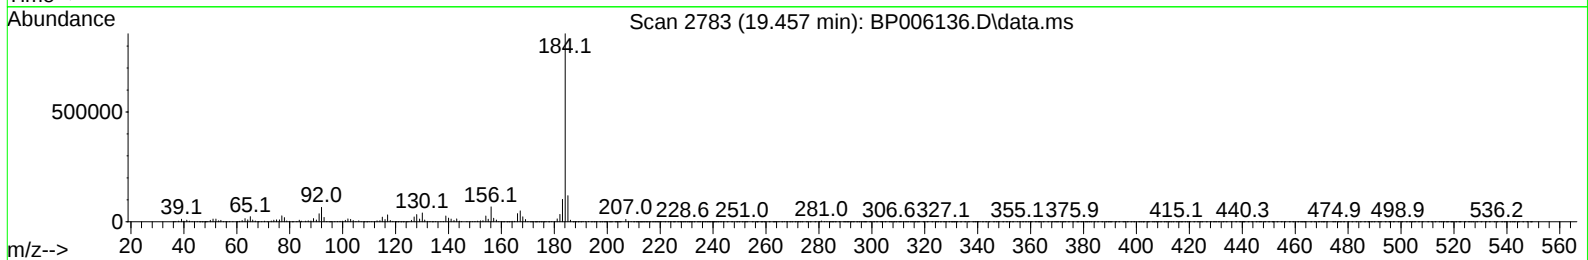


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070821\
 Data File : BP006136.D
 Acq On : 08 Jul 2021 12:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 08 13:47:22 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 07 16:08:13 2021
 Response via : Initial Calibration

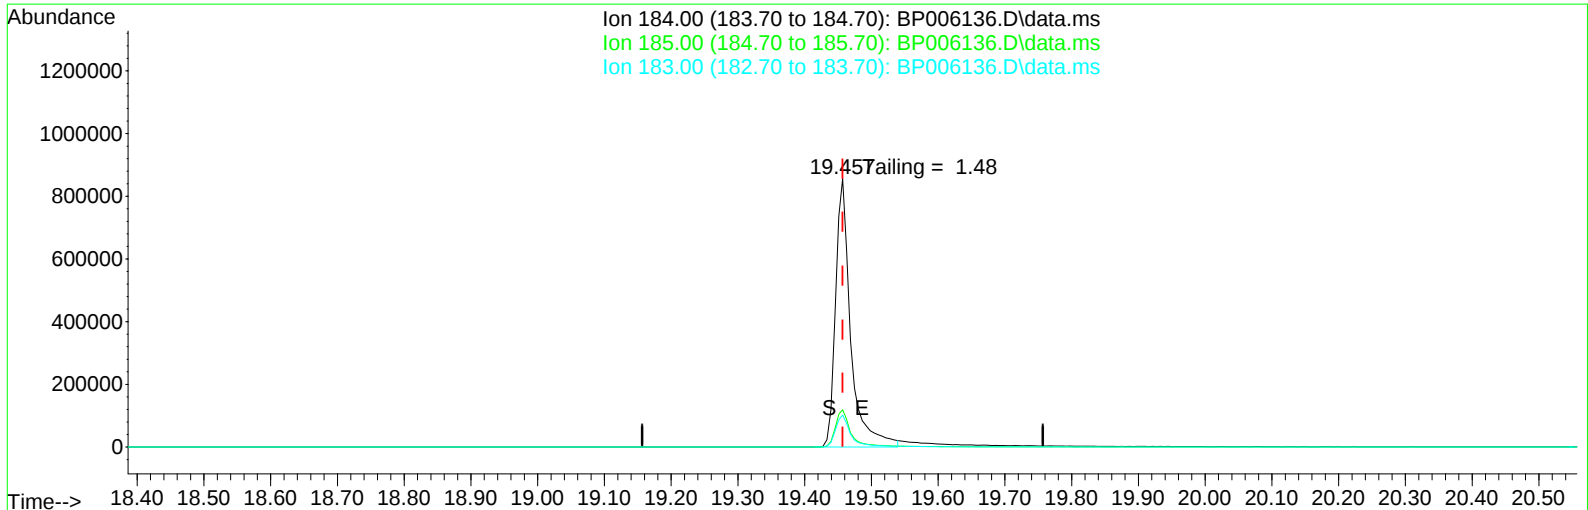

TIC: BP006136.D\data.ms

(77) Benzidine




19.457min (+ 0.000) 365054.23 ng

response 1374747

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.92
183.00	11.90	11.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070821\
Data File : BP006136.D
Acq On : 08 Jul 2021 12:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 08 13:47:22 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 07 16:08:13 2021
Response via : Initial Calibration

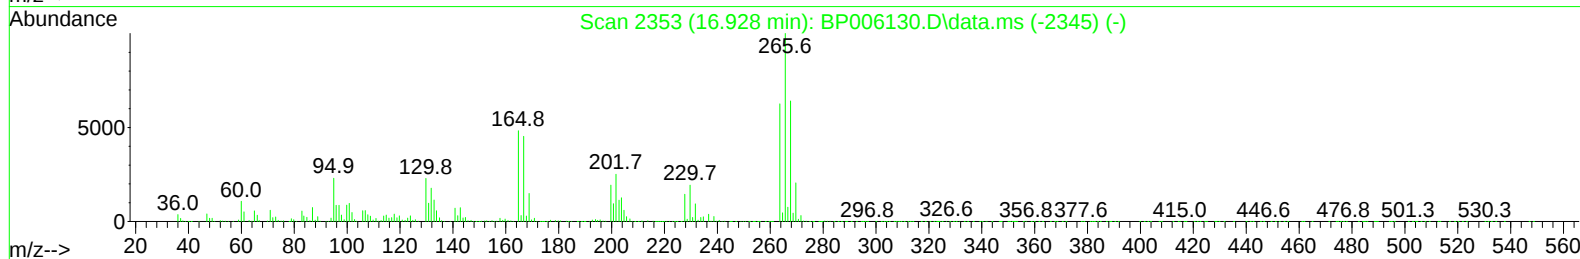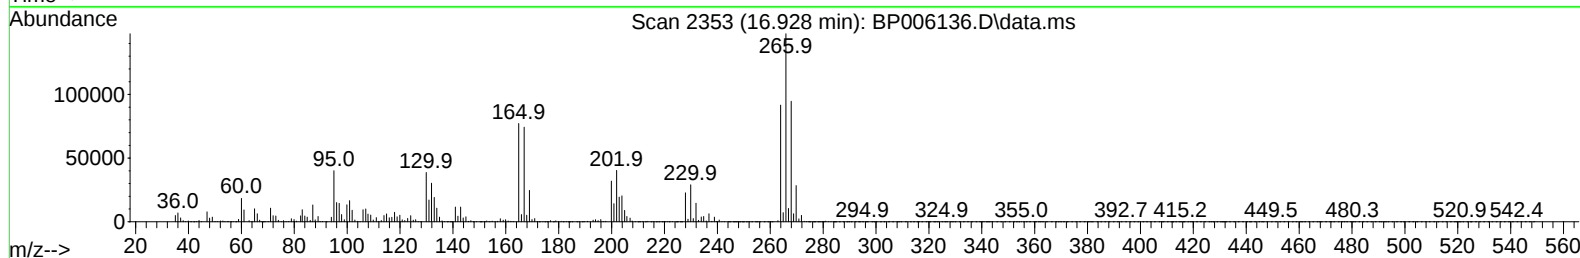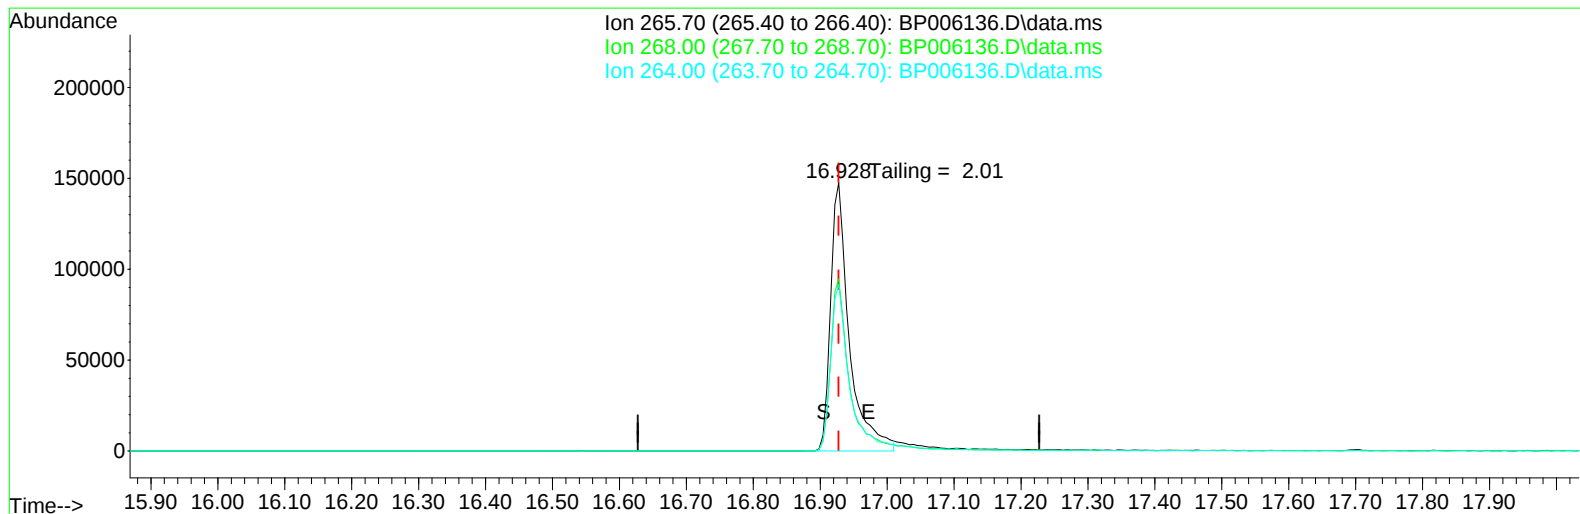

TIC: BP006136.D\data.ms

(70) Pentachlorophenol (C)

16.928min (+ 0.000) 4933800.33 ng

response 293100

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.08
264.00	62.90	62.01
0.00	0.00	0.00