

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070824\
 Data File : BP020834.D
 Acq On : 08 Jul 2024 15:50
 Operator : MA/JU
 Sample : P3084-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E1GE2

Quant Time: Jul 08 16:26:06 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 03 15:01:56 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.728	152	154077	20.000	ng/ul	0.00
20) Naphthalene-d8	10.499	136	620358	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.369	164	407321	20.000	ng/ul	0.02
64) Phenanthrene-d10	17.181	188	895105	20.000	ng/ul	0.02
79) Chrysene-d12	21.616	240	917577	20.000	ng/ul	0.00
88) Perylene-d12	24.963	264	1064210	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	18202	5.073	ng/uL	0.00
4) Pyridine-d5	3.687	84	55184	5.277	ng/ul	0.00
7) Phenol-d5	6.922	99	137764	10.901	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.075	67	305801	38.170	ng/ul	0.00
11) 2-Chlorophenol-d4	7.275	132	381282	36.917	ng/ul	0.00
15) 4-Methylphenol-d8	8.440	113	258133	25.150	ng/ul	0.00
21) Nitrobenzene-d5	8.887	128	208847	45.599	ng/ul	0.00
24) 2-Nitrophenol-d4	9.599	143	236562	51.613	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.128	165	391415	41.458	ng/ul	0.00
31) 4-Chloroaniline-d4	10.652	131	194086	14.669	ng/ul	0.01
46) Dimethylphthalate-d6	13.775	166	1342620	47.408	ng/ul	0.02
49) Acenaphthylene-d8	14.057	160	1438895	42.579	ng/ul	0.02
54) 4-Nitrophenol-d4	14.622	143	48366	11.177	ng/ul	0.04
60) Fluorene-d10	15.381	176	1103150	46.290	ng/ul	0.02
65) 4,6-Dinitro-2-methylph...	15.516	200	230857	51.178	ng/ul	0.02
73) Anthracene-d10	17.281	188	1908085	47.497	ng/ul	0.02
81) Pyrene-d10	19.657	212	2311508	41.933	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.733	264	2525863	48.793	ng/ul	0.00
Target Compounds						
					Qvalue	
6) Benzaldehyde	6.899	77	8483	1.327	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070824\
Data File : BP020834.D
Acq On : 08 Jul 2024 15:50
Operator : MA/JU
Sample : P3084-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E1GE2

Quant Time: Jul 08 16:26:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 03 15:01:56 2024
Response via : Initial Calibration

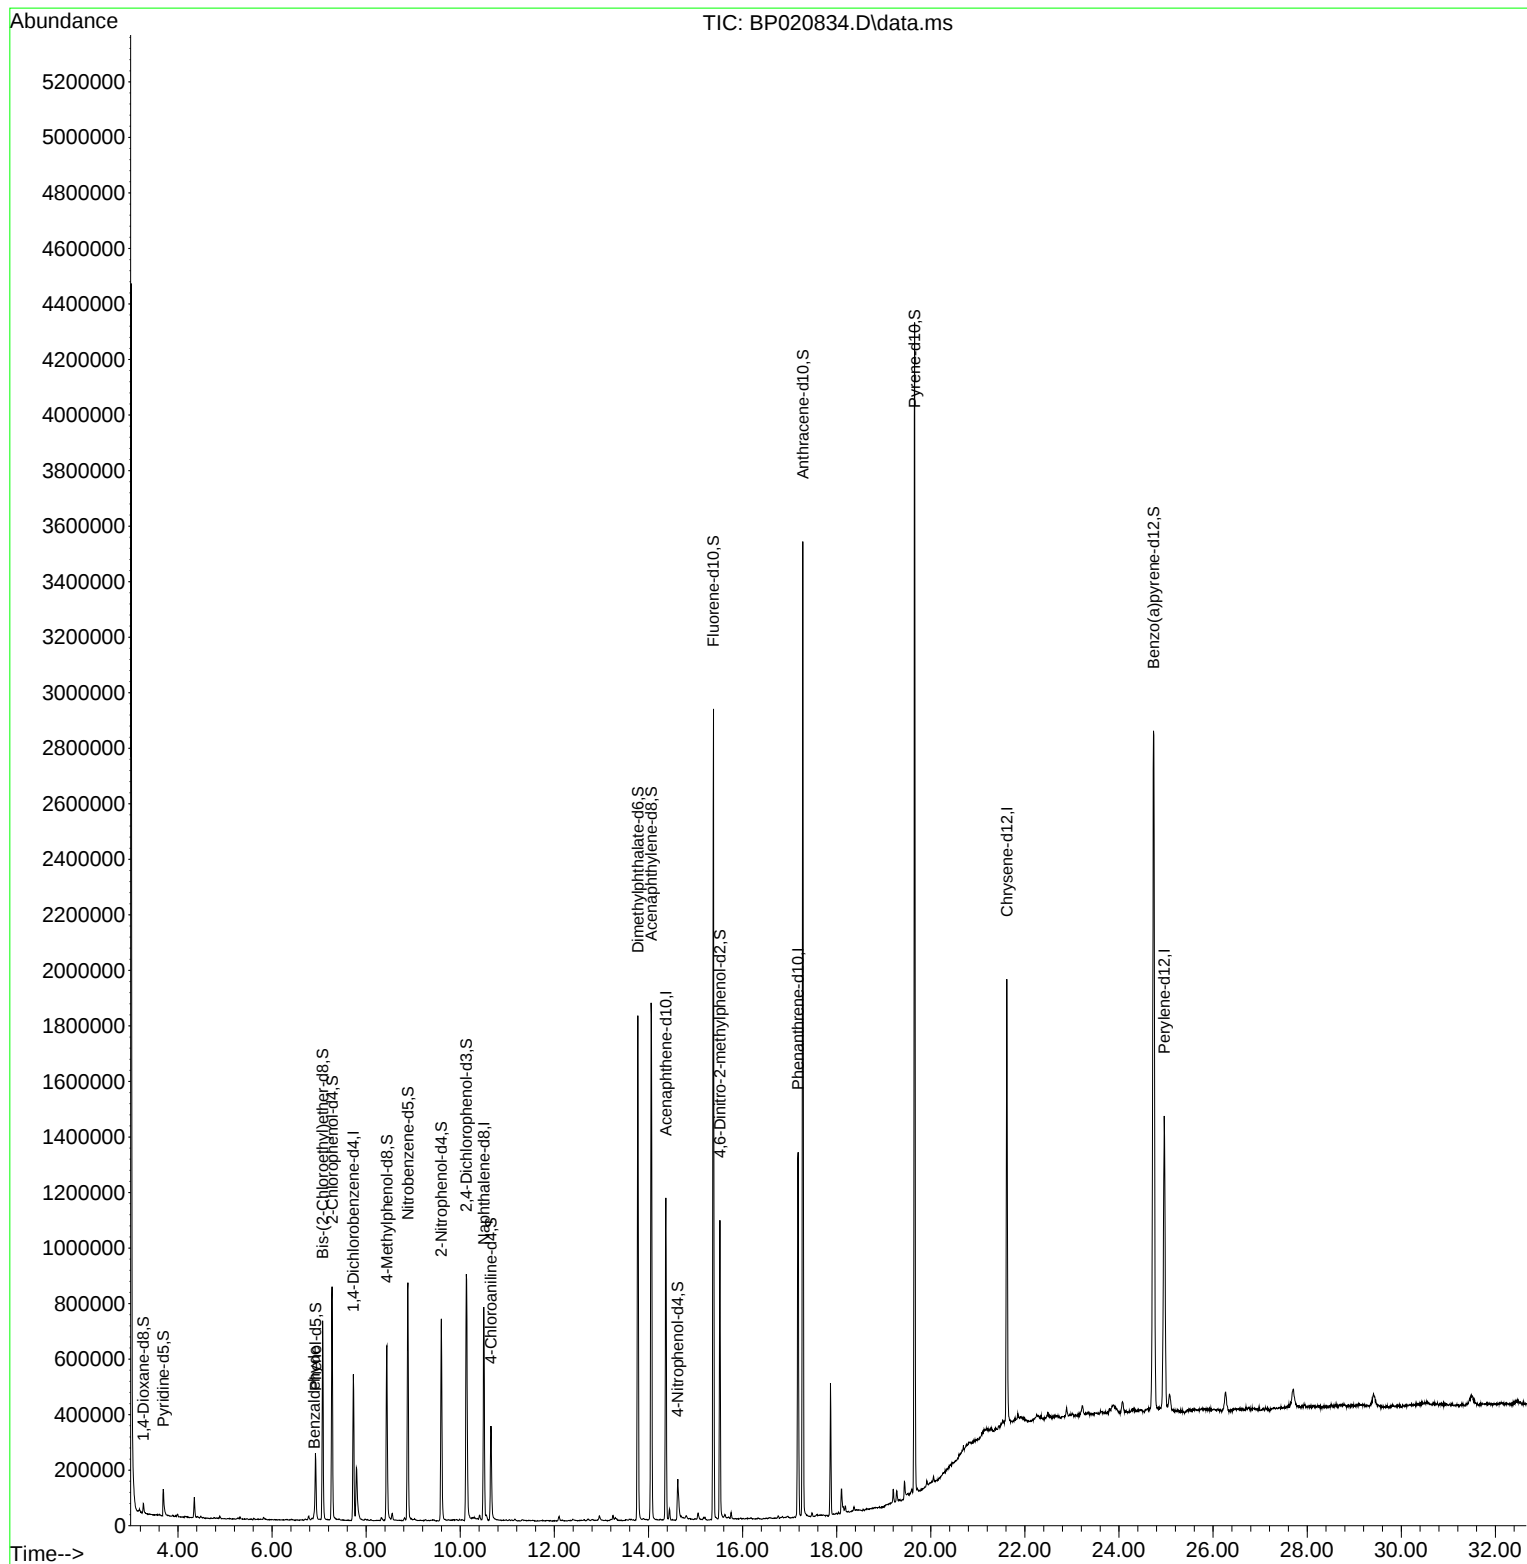

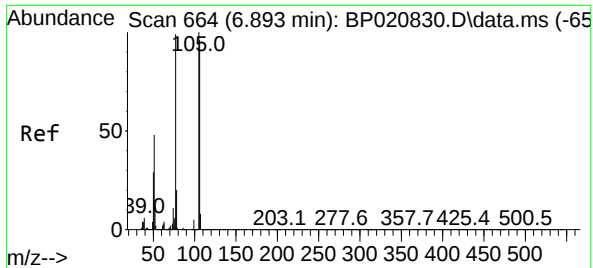

#6
Benzaldehyde
Concen: 1.327 ng/ul
RT: 6.899 min Scan# 60
Delta R.T. 0.006 min
Lab File: BP020834.D
Acq: 08 Jul 2024 15:50

Instrument :
BNA_P
ClientSampleId :
E1GE2

Tgt Ion: 77 Resp: 8483
Ion Ratio Lower Upper
77 100
105 93.7 78.2 117.2
106 90.7 73.2 109.8

