

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070824\
 Data File : BP020835.D
 Acq On : 08 Jul 2024 16:33
 Operator : MA/JU
 Sample : P3084-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E1GE3

Quant Time: Jul 08 17:40:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 03 15:01:56 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.728	152	166969	20.000	ng/ul	0.00
20) Naphthalene-d8	10.499	136	690564	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.363	164	458286	20.000	ng/ul	0.01
64) Phenanthrene-d10	17.186	188	1017199	20.000	ng/ul	0.02
79) Chrysene-d12	21.627	240	1005338	20.000	ng/ul	0.00
88) Perylene-d12	24.974	264	1154147	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	18967	4.878	ng/uL	0.00
4) Pyridine-d5	3.681	84	69594	6.141	ng/ul	0.00
7) Phenol-d5	6.916	99	167762	12.250	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.075	67	353042	40.665	ng/ul	0.00
11) 2-Chlorophenol-d4	7.269	132	435899	38.946	ng/ul	0.00
15) 4-Methylphenol-d8	8.434	113	307020	27.604	ng/ul	0.00
21) Nitrobenzene-d5	8.881	128	239150	46.907	ng/ul	0.00
24) 2-Nitrophenol-d4	9.599	143	276832	54.258	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.128	165	463227	44.076	ng/ul	0.00
31) 4-Chloroaniline-d4	10.646	131	330022	22.407	ng/ul	0.00
46) Dimethylphthalate-d6	13.769	166	1551870	48.703	ng/ul	0.01
49) Acenaphthylene-d8	14.051	160	1653959	43.500	ng/ul	0.01
54) 4-Nitrophenol-d4	14.616	143	57064	11.721	ng/ul	0.04
60) Fluorene-d10	15.381	176	1299443	48.462	ng/ul	0.02
65) 4,6-Dinitro-2-methylph...	15.516	200	258444	50.417	ng/ul	0.02
73) Anthracene-d10	17.286	188	2100573	46.013	ng/ul	0.02
81) Pyrene-d10	19.663	212	2551000	42.237	ng/ul	0.01
92) Benzo(a)pyrene-d12	24.751	264	2683697	47.802	ng/ul	0.01
Target Compounds						
					Qvalue	
6) Benzaldehyde	6.893	77	11846	1.711	ng/ul	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070824\
Data File : BP020835.D
Acq On : 08 Jul 2024 16:33
Operator : MA/JU
Sample : P3084-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E1GE3

Quant Time: Jul 08 17:40:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 03 15:01:56 2024
Response via : Initial Calibration

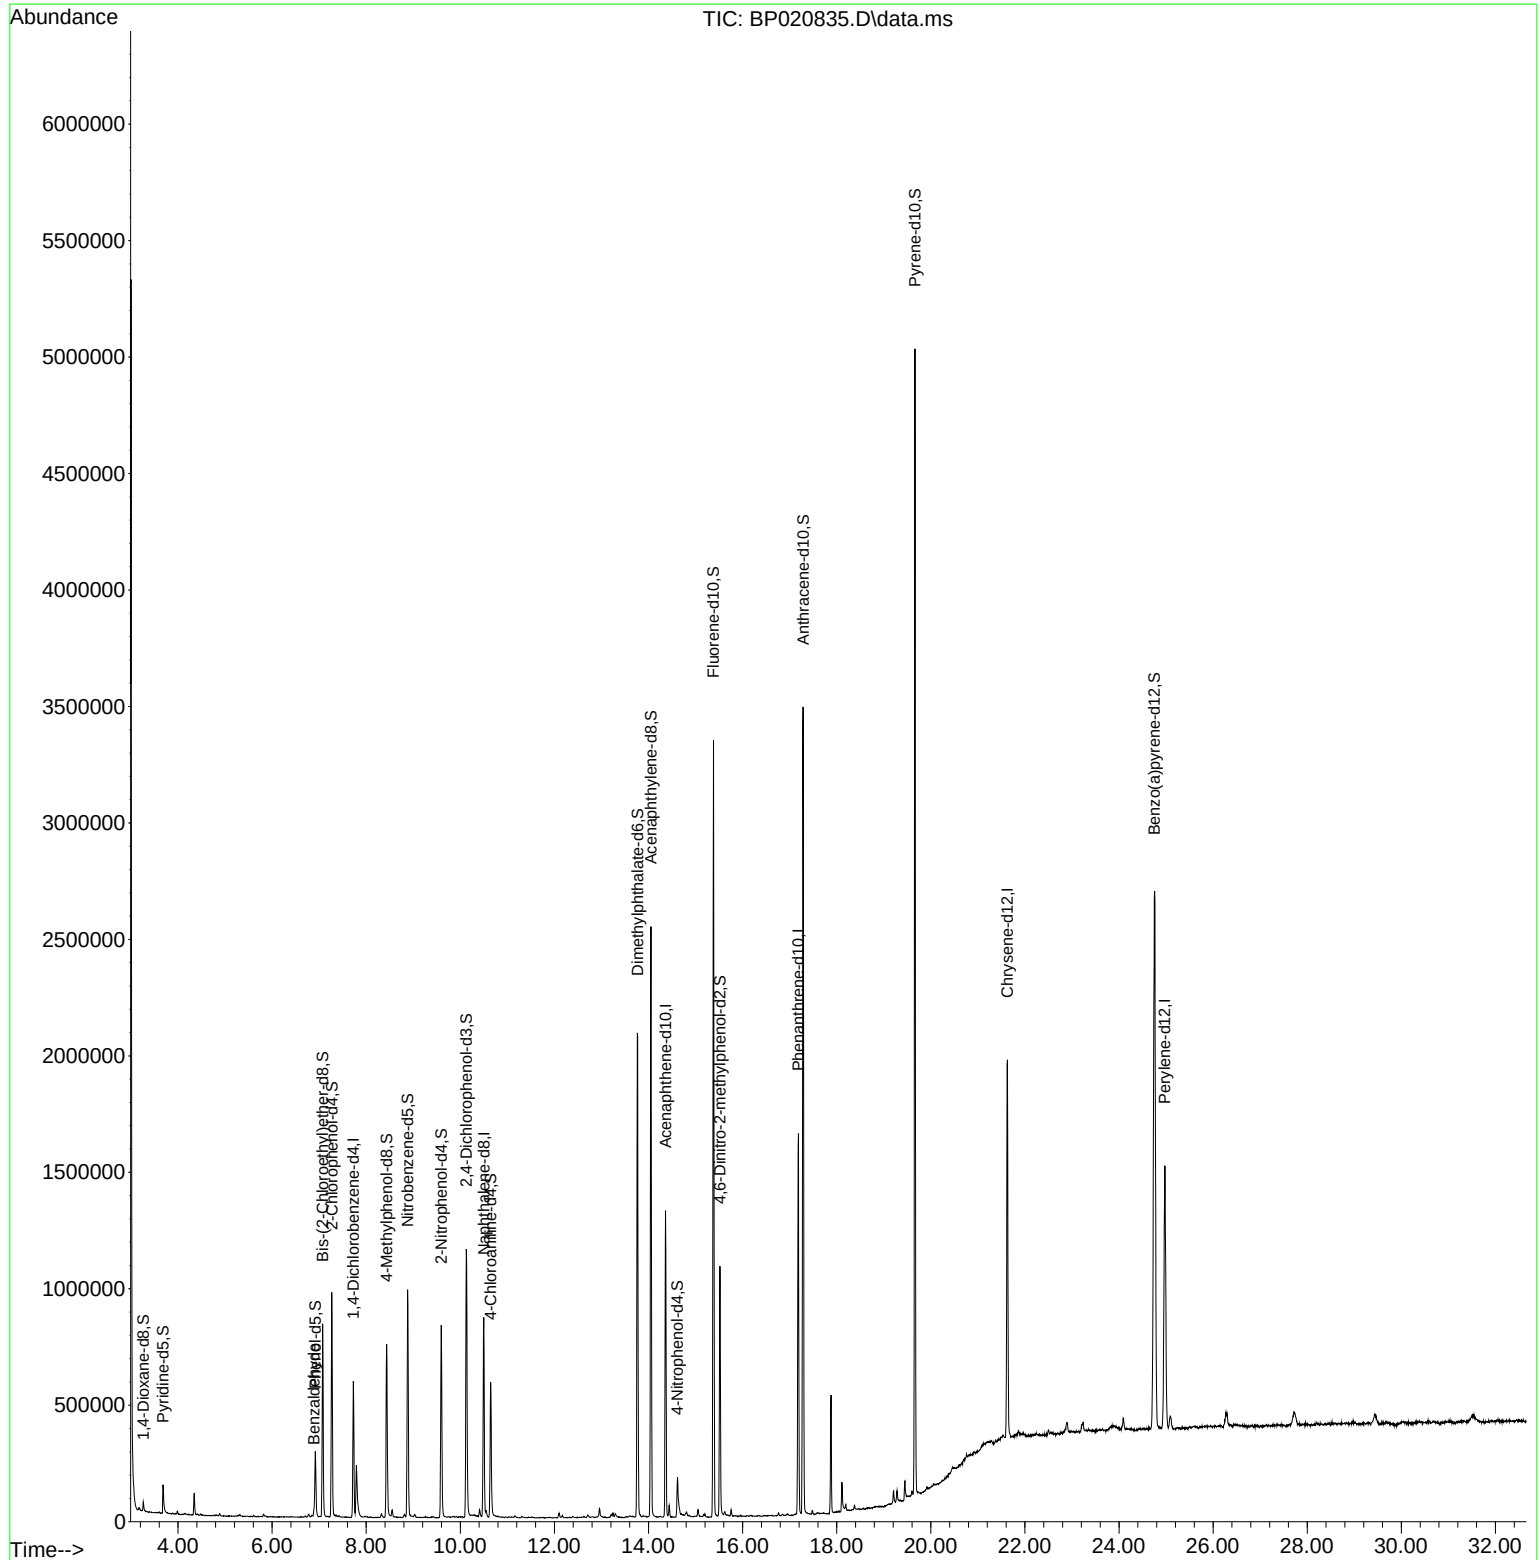

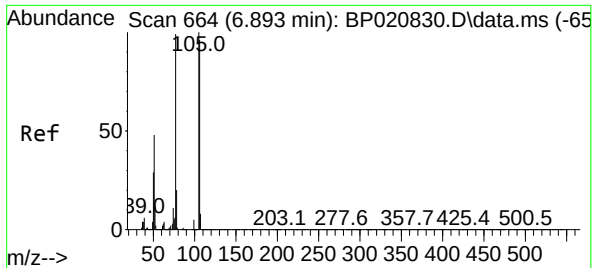

#6
Benzaldehyde
Concen: 1.711 ng/ul
RT: 6.893 min Scan# 61
Delta R.T. -0.000 min
Lab File: BP020835.D
Acq: 08 Jul 2024 16:33

Instrument :
BNA_P
ClientSampleId :
E1GE3

Tgt Ion:	77	Resp:	11846
Ion	Ratio	Lower	Upper
77	100		
105	91.8	78.2	117.2
106	77.2	73.2	109.8

