

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070824\
 Data File : BP020853.D
 Acq On : 09 Jul 2024 06:09
 Operator : MA/JU
 Sample : P3084-06
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E1GC7

Quant Time: Jul 09 06:37:35 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 03 15:01:56 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.728	152	236344	20.000	ng/ul	0.00
20) Naphthalene-d8	10.493	136	995305	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.357	164	669709	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.175	188	1465856	20.000	ng/ul	0.01
79) Chrysene-d12	21.622	240	1389163	20.000	ng/ul	0.00
88) Perylene-d12	24.968	264	1583451	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	25201	4.579	ng/uL	0.00
4) Pyridine-d5	3.681	84	167423	10.437	ng/ul	0.00
7) Phenol-d5	6.922	99	234912	12.118	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.069	67	477381	38.846	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.269	132	595292	37.575	ng/ul	0.00
15) 4-Methylphenol-d8	8.434	113	434114	27.574	ng/ul	0.00
21) Nitrobenzene-d5	8.881	128	326469	44.428	ng/ul	0.00
24) 2-Nitrophenol-d4	9.593	143	384516	52.289	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.128	165	631711	41.704	ng/ul	0.00
31) 4-Chloroaniline-d4	10.646	131	814322	38.361	ng/ul	0.00
46) Dimethylphthalate-d6	13.763	166	2036040	43.725	ng/ul	0.00
49) Acenaphthylene-d8	14.045	160	2263866	40.744	ng/ul	0.00
54) 4-Nitrophenol-d4	14.616	143	83188	11.693	ng/ul	0.04
60) Fluorene-d10	15.375	176	1714947	43.767	ng/ul	0.01
65) 4,6-Dinitro-2-methylph...	15.510	200	319751	43.285	ng/ul	0.01
73) Anthracene-d10	17.275	188	2803224	42.610	ng/ul	0.01
81) Pyrene-d10	19.663	212	3298016	39.518	ng/ul	0.01
92) Benzo(a)pyrene-d12	24.751	264	3391895	44.036	ng/ul	0.01
Target Compounds						
					Qvalue	
6) Benzaldehyde	6.899	77	14844	1.514	ng/ul	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070824\
Data File : BP020853.D
Acq On : 09 Jul 2024 06:09
Operator : MA/JU
Sample : P3084-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E1GC7

Quant Time: Jul 09 06:37:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 03 15:01:56 2024
Response via : Initial Calibration

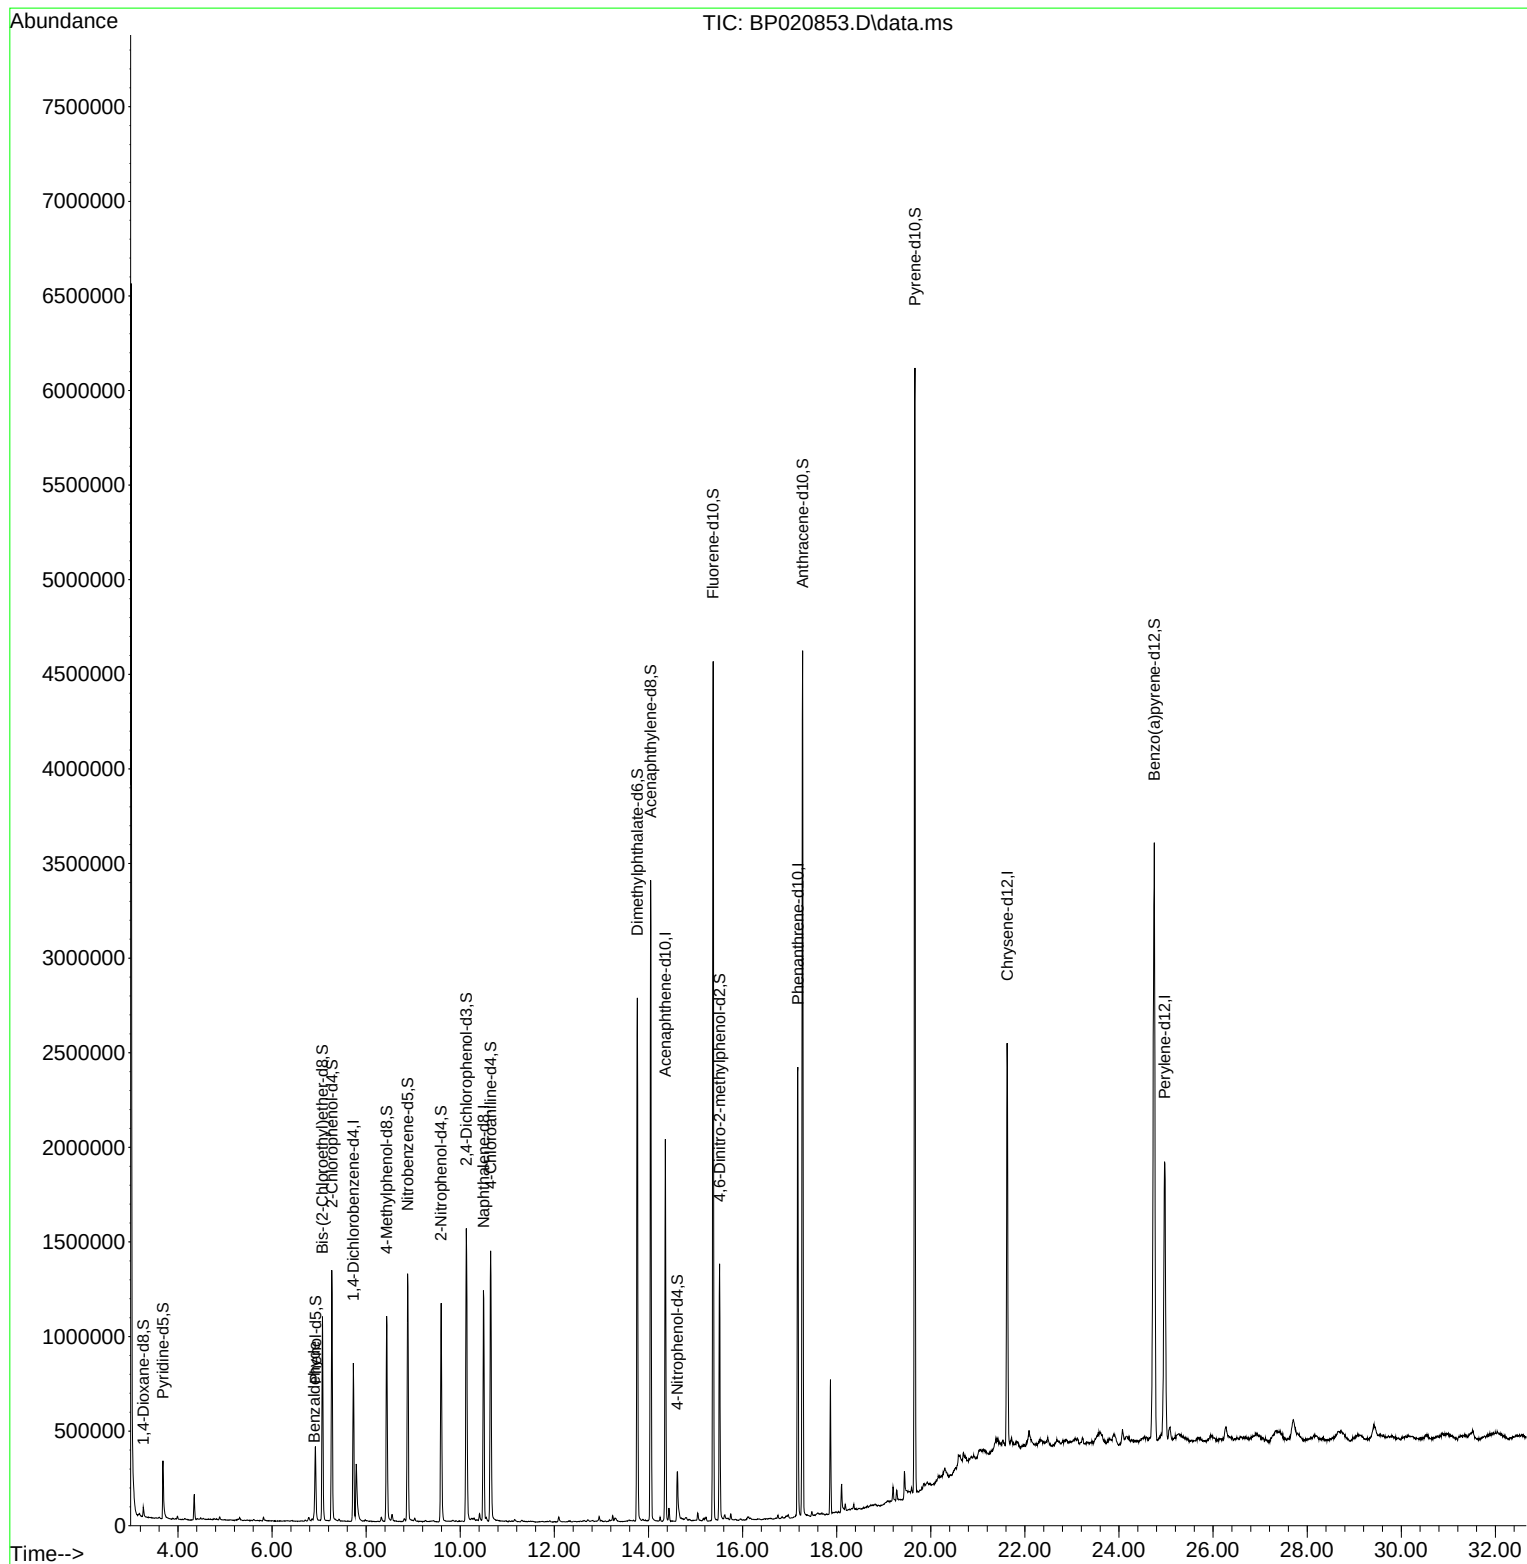

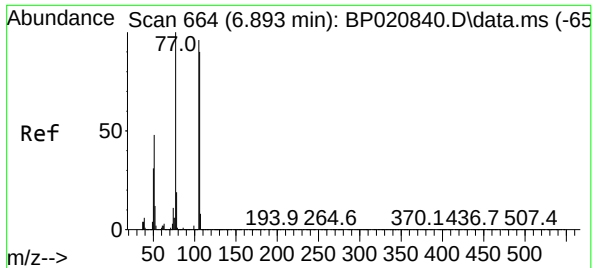

#6
Benzaldehyde
Concen: 1.514 ng/ul
RT: 6.899 min Scan# 60
Delta R.T. 0.006 min
Lab File: BP020853.D
Acq: 09 Jul 2024 06:09

Instrument :
BNA_P
ClientSampleId :
E1GC7

Tgt Ion: 77	Resp: 14844
Ion Ratio	Lower Upper
77 100	
105 80.8	78.2 117.2
106 84.5	73.2 109.8

