

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070824\
 Data File : BP020846.D
 Acq On : 09 Jul 2024 01:10
 Operator : MA/JU
 Sample : P3035-08
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4CX4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020846.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	44	47	54	rVB	30927	40450	0.66%	0.071%
2	3.540	91	94	106	rVB	42425	70683	1.15%	0.123%
3	3.675	115	117	131	rBV	345810	523768	8.51%	0.914%
4	3.987	166	170	176	rVB	20025	28425	0.46%	0.050%
5	4.881	319	322	328	rVB3	6935	10578	0.17%	0.018%
6	6.916	660	668	683	rBV	531300	909535	14.77%	1.587%
7	7.075	688	695	708	rVV	434286	675955	10.98%	1.179%
8	7.269	721	728	739	rBV	551378	916528	14.89%	1.599%
9	7.363	739	744	751	rVB3	7139	17325	0.28%	0.030%
10	7.728	797	806	816	rBV	1269442	2213906	35.96%	3.862%
11	7.798	816	818	825	rVB7	5050	9607	0.16%	0.017%
12	8.440	920	927	941	rBV	665232	1145285	18.60%	1.998%
13	8.881	992	1002	1015	rBV	560965	912069	14.81%	1.591%
14	9.028	1023	1027	1032	rVB8	5048	8046	0.13%	0.014%
15	9.245	1060	1064	1069	rBV7	3560	7016	0.11%	0.012%
16	9.428	1089	1095	1107	rBV	37241	60187	0.98%	0.105%
17	9.592	1114	1123	1138	rBV	441847	798561	12.97%	1.393%
18	10.128	1206	1214	1229	rBV	659383	1217659	19.78%	2.124%
19	10.498	1269	1277	1290	rBV	1810212	3233135	52.51%	5.640%
20	10.645	1294	1302	1316	rBV	608504	1119553	18.18%	1.953%
21	11.051	1362	1371	1375	rBV	8506	19815	0.32%	0.035%
22	11.245	1396	1404	1425	rBV2	42009	126955	2.06%	0.221%
23	12.086	1541	1547	1557	rVV2	11863	23235	0.38%	0.041%
24	13.316	1750	1756	1765	rVB2	4706	12020	0.20%	0.021%
25	13.763	1824	1832	1846	rBV	1044600	1955434	31.76%	3.411%
26	14.045	1868	1880	1897	rBV	1413031	2300358	37.36%	4.013%
27	14.257	1909	1916	1919	rVB9	3042	7143	0.12%	0.012%
28	14.357	1922	1933	1952	rBV	3014930	4468062	72.56%	7.794%
29	14.610	1969	1976	1987	rVB	372370	778590	12.64%	1.358%
30	15.375	2098	2106	2113	rBV	2156736	2914887	47.34%	5.084%
31	15.510	2123	2129	2141	rBV	591003	829809	13.48%	1.447%
32	15.616	2143	2147	2156	rVB9	10668	24319	0.39%	0.042%
33	15.739	2165	2168	2174	rBV7	3730	6191	0.10%	0.011%
34	15.939	2199	2202	2208	rBV8	6447	11280	0.18%	0.020%
35	16.110	2226	2231	2238	rBV9	8919	20168	0.33%	0.035%
36	16.563	2306	2308	2312	rVB4	8246	9683	0.16%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070824\
 Data File : BP020846.D
 Acq On : 09 Jul 2024 01:10
 Operator : MA/JU
 Sample : P3035-08
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4CX4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Title : SVOA CALIBRATION

37	16.916	2366	2368	2371	rBV4	5307	7041	0.11%	0.012%
38	16.945	2371	2373	2385	rVB4	12143	30236	0.49%	0.053%
39	17.092	2394	2398	2403	rVB5	17175	24615	0.40%	0.043%
40	17.174	2404	2412	2417	rBV	3443066	5499887	89.32%	9.594%
41	17.274	2422	2429	2440	rVB2	1964390	3115007	50.59%	5.434%
42	17.592	2479	2483	2490	rBV8	7505	14910	0.24%	0.026%
43	17.869	2526	2530	2535	rBV	26428	40398	0.66%	0.070%
44	18.098	2564	2569	2580	rBV	262173	481296	7.82%	0.840%
45	18.280	2597	2600	2608	rBV7	16243	24030	0.39%	0.042%
46	19.310	2767	2775	2784	rBV2	152257	280625	4.56%	0.489%
47	19.433	2793	2796	2807	rVB3	123856	193560	3.14%	0.338%
48	19.657	2828	2834	2843	rBV2	2611182	4063965	66.00%	7.089%
49	21.286	3107	3111	3118	rVB	296120	486147	7.90%	0.848%
50	21.621	3161	3168	3174	rBV2	3634245	5901265	95.84%	10.294%
51	24.727	3688	3696	3707	rVB2	1249047	3582431	58.18%	6.249%
52	24.974	3728	3738	3747	rVB	2409191	6157345	100.00%	10.740%




Sum of corrected areas: 57328978

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070824\
Data File : BP020846.D
Acq On : 09 Jul 2024 01:10
Operator : MA/JU
Sample : P3035-08
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4CX4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

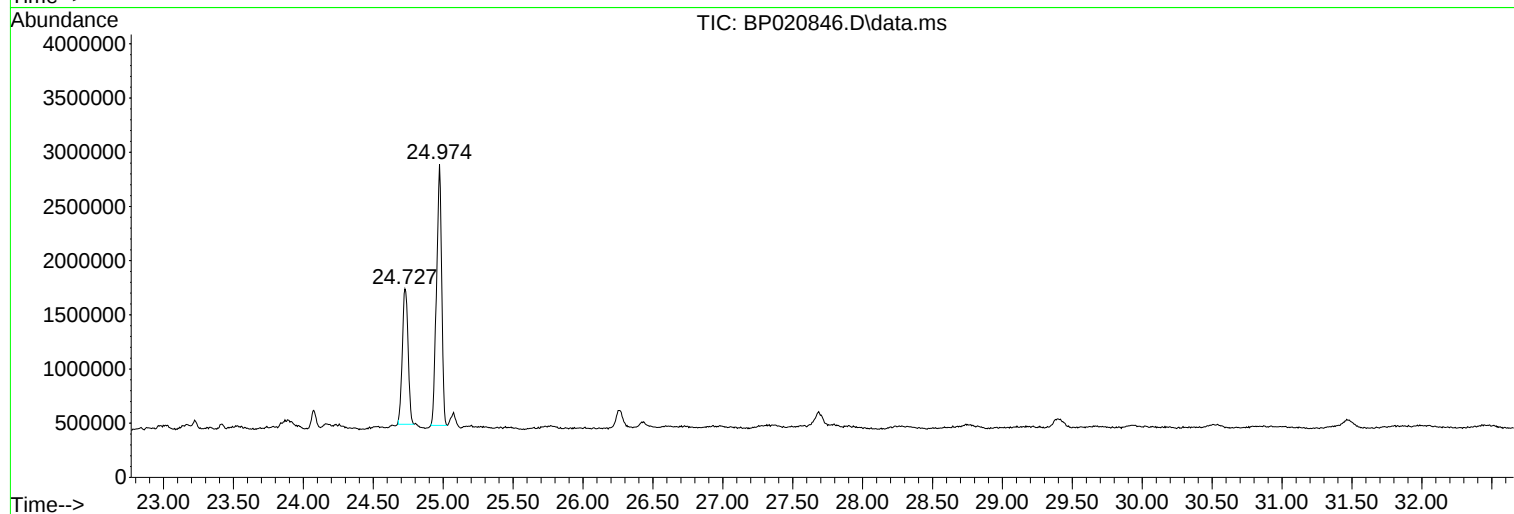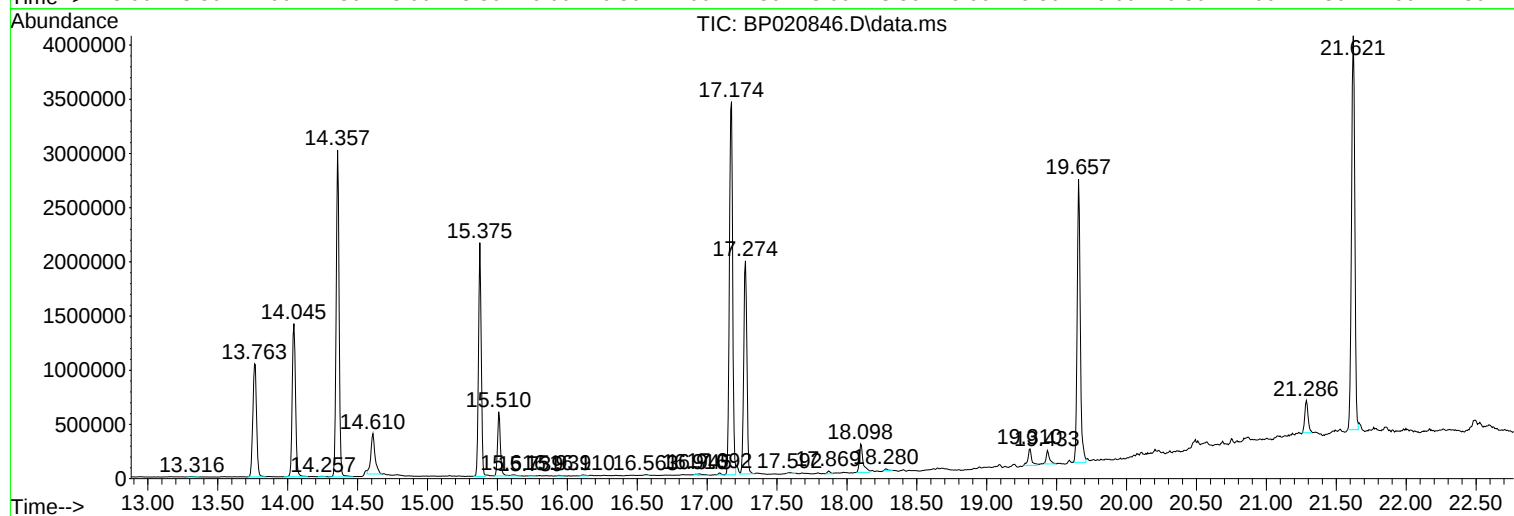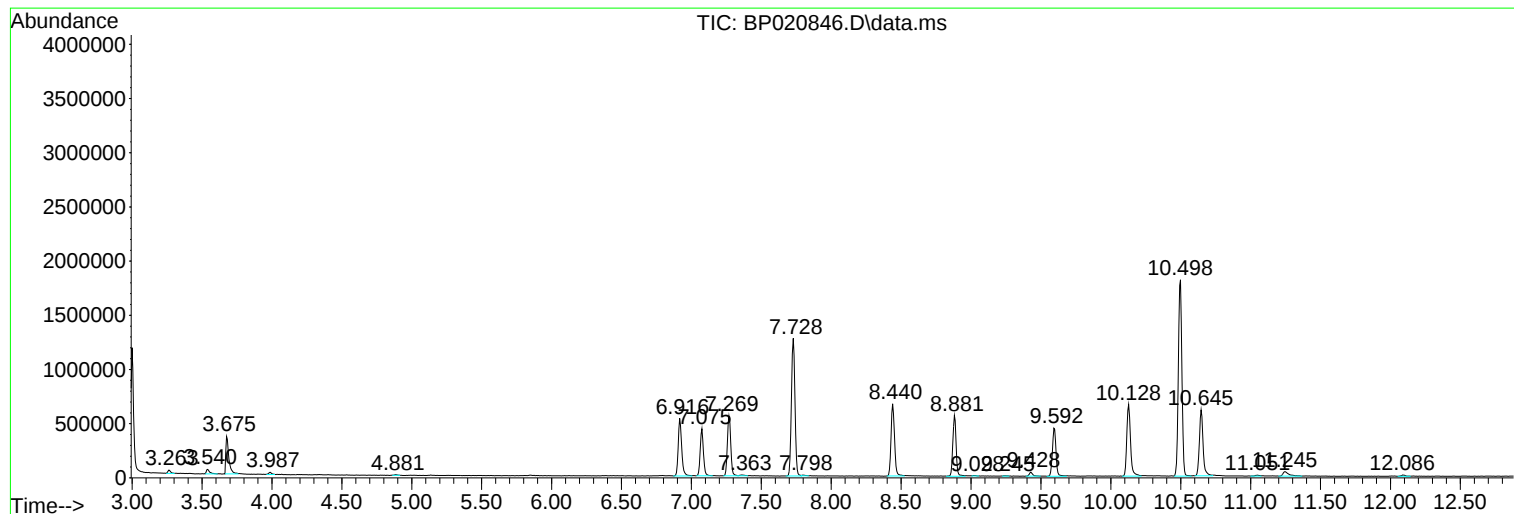

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070824\
Data File : BP020846.D
Acq On : 09 Jul 2024 01:10
Operator : MA/JU
Sample : P3035-08
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4CX4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070824\
Data File : BP020846.D
Acq On : 09 Jul 2024 01:10
Operator : MA/JU
Sample : P3035-08
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4CX4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
