

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070824\
 Data File : BP020856.D
 Acq On : 09 Jul 2024 08:59
 Operator : MA/JU
 Sample : PB161773BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK773

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020856.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	43	47	53	rBV	54060	73765	1.40%	0.137%
2	3.675	114	117	140	rBV	657237	1040880	19.75%	1.934%
3	3.987	167	170	174	rVB	11121	12396	0.24%	0.023%
4	6.922	661	669	684	rBV	741550	1367135	25.94%	2.540%
5	7.069	687	694	710	rVB	669611	1044687	19.82%	1.941%
6	7.269	721	728	743	rBV	795031	1381000	26.20%	2.566%
7	7.722	799	805	817	rBV	694178	1120885	21.27%	2.083%
8	8.440	919	927	947	rBV	991386	1718692	32.61%	3.193%
9	8.875	993	1001	1016	rBV	829342	1340670	25.44%	2.491%
10	9.587	1115	1122	1133	rBV	689470	1179308	22.38%	2.191%
11	10.128	1205	1214	1236	rBV	893368	1789735	33.96%	3.325%
12	10.493	1269	1276	1287	rBV	972770	1634601	31.02%	3.037%
13	10.640	1293	1301	1312	rBV	806955	1434199	27.21%	2.665%
14	12.081	1542	1546	1553	rBV3	12267	28937	0.55%	0.054%
15	12.316	1580	1586	1590	rBV8	3814	8255	0.16%	0.015%
16	13.310	1749	1755	1760	rBV8	3499	6481	0.12%	0.012%
17	13.763	1824	1832	1845	rBV	1709231	2639446	50.08%	4.904%
18	14.045	1872	1880	1896	rBV	1937779	3119577	59.19%	5.796%
19	14.351	1925	1932	1946	rVB	1592158	2282449	43.31%	4.241%
20	14.598	1966	1974	1992	rBV	600668	1240154	23.53%	2.304%
21	14.757	1997	2001	2005	rVB7	6089	12336	0.23%	0.023%
22	15.363	2097	2104	2121	rBV	2592039	3873470	73.50%	7.197%
23	15.498	2121	2127	2139	rVV	946872	1262699	23.96%	2.346%
24	15.604	2142	2145	2154	rVB2	12948	25092	0.48%	0.047%
25	15.875	2189	2191	2196	rVB4	6087	8494	0.16%	0.016%
26	16.163	2237	2240	2245	rVB4	11175	13603	0.26%	0.025%
27	16.828	2350	2353	2359	rBV7	5068	9810	0.19%	0.018%
28	16.945	2371	2373	2377	rVB4	5704	6078	0.12%	0.011%
29	17.169	2403	2411	2418	rBV	1696482	2851169	54.10%	5.297%
30	17.269	2421	2428	2439	rVV	3218436	4305902	81.70%	8.000%
31	17.863	2525	2529	2536	rBV10	7956	16442	0.31%	0.031%
32	18.092	2565	2568	2575	rBV9	10334	24630	0.47%	0.046%
33	19.192	2752	2755	2760	rBV	43418	60221	1.14%	0.112%
34	19.275	2765	2769	2776	rVV2	31795	54606	1.04%	0.101%
35	19.651	2827	2833	2843	rBV	3656179	5270197	100.00%	9.792%
36	21.621	3162	3168	3180	rBV2	1700433	3126690	59.33%	5.809%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070824\
Data File : BP020856.D
Acq On : 09 Jul 2024 08:59
Operator : MA/JU
Sample : PB161773BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK773

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Title : SVOA CALIBRATION

37	24.751	3691	3700	3711	rVB3	1832488	5212947	98.91%	9.686%
38	24.974	3730	3738	3750	rVB	1248229	3223800	61.17%	5.990%




Sum of corrected areas: 53821438

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070824\
Data File : BP020856.D
Acq On : 09 Jul 2024 08:59
Operator : MA/JU
Sample : PB161773BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK773

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

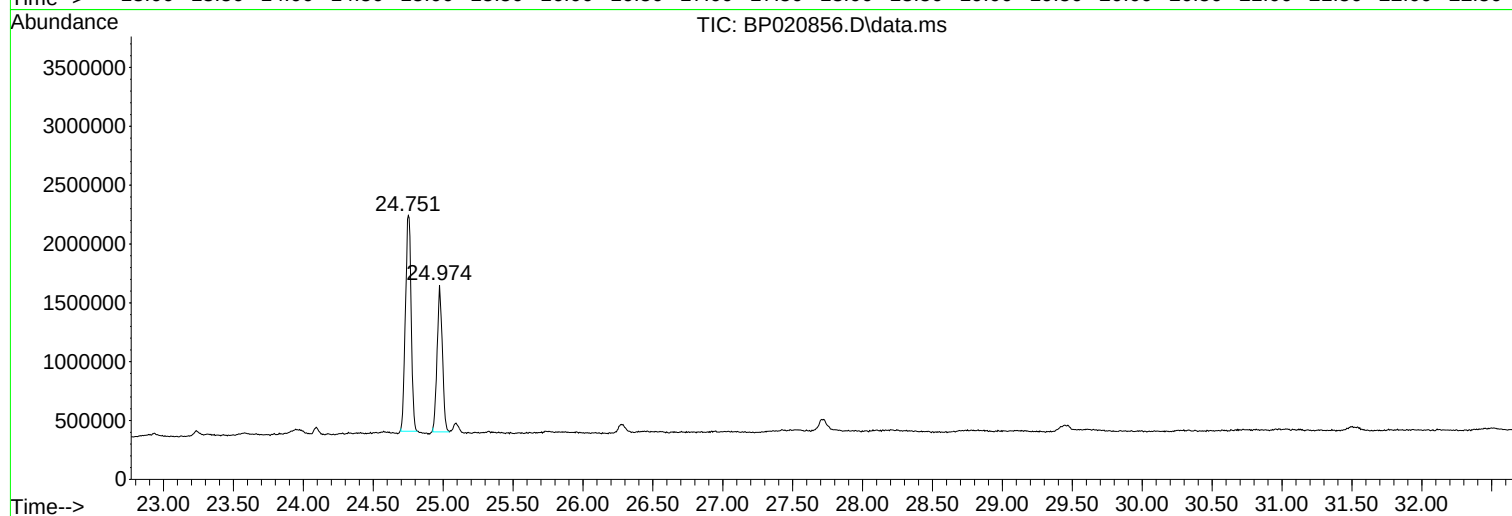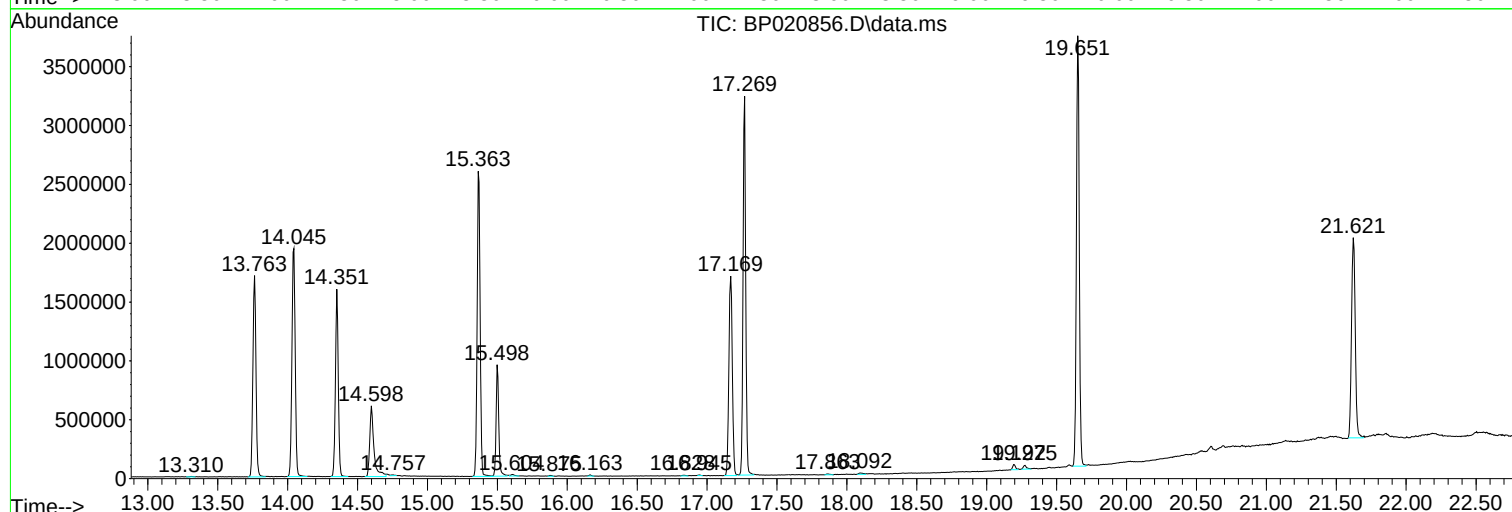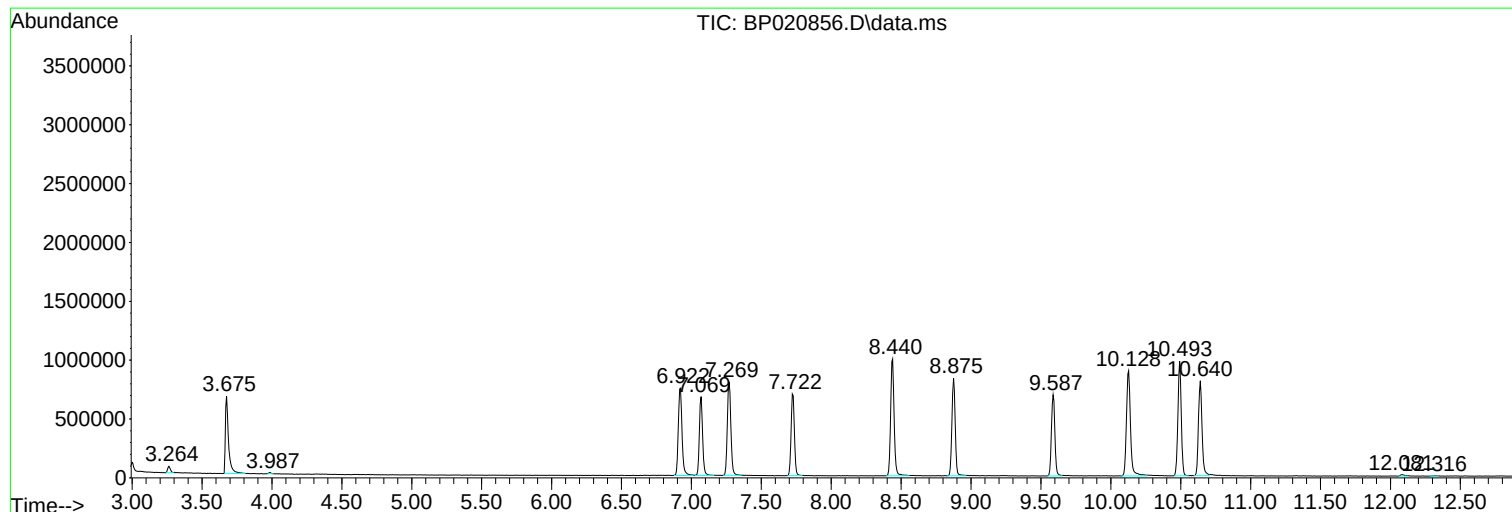

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070824\
Data File : BP020856.D
Acq On : 09 Jul 2024 08:59
Operator : MA/JU
Sample : PB161773BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK773

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070824\
Data File : BP020856.D
Acq On : 09 Jul 2024 08:59
Operator : MA/JU
Sample : PB161773BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK773

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc