

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070824\
 Data File : BP020871.D
 Acq On : 09 Jul 2024 20:36
 Operator : MA/JU
 Sample : PB161916BL
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK916

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020871.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	42	46	55	rVB	50239	73180	1.54%	0.137%
2	3.675	113	117	135	rBV	591235	942644	19.85%	1.761%
3	3.981	166	169	179	rVB	14240	24382	0.51%	0.046%
4	6.922	662	669	679	rBV	770068	1295665	27.29%	2.421%
5	7.069	687	694	706	rBV	627965	984926	20.74%	1.840%
6	7.269	721	728	740	rBV	831605	1324251	27.89%	2.474%
7	7.722	798	805	815	rBV	841283	1363793	28.72%	2.548%
8	8.434	918	926	937	rBV	941573	1634373	34.42%	3.053%
9	8.881	994	1002	1013	rBV	752737	1281368	26.98%	2.394%
10	9.593	1114	1123	1137	rBV	626217	1126077	23.71%	2.104%
11	10.128	1205	1214	1233	rBV	929661	1712222	36.06%	3.199%
12	10.493	1266	1276	1285	rBV	1286520	2008453	42.30%	3.752%
13	10.646	1293	1302	1319	rBV	722893	1459963	30.75%	2.728%
14	12.087	1541	1547	1554	rBV2	11365	26604	0.56%	0.050%
15	13.763	1826	1832	1847	rBV	1679333	2392470	50.38%	4.470%
16	14.051	1872	1881	1897	rBV	1824702	2967737	62.50%	5.544%
17	14.357	1926	1933	1948	rBV	1677465	2773005	58.40%	5.181%
18	14.604	1968	1975	1988	rBV	494590	1067209	22.47%	1.994%
19	14.781	2003	2005	2014	rVB9	8971	18179	0.38%	0.034%
20	14.875	2017	2021	2025	rVB5	3804	6651	0.14%	0.012%
21	15.369	2096	2105	2122	rBV	2285774	3706876	78.06%	6.925%
22	15.522	2124	2131	2140	rVV	611984	937079	19.73%	1.751%
23	15.610	2143	2146	2157	rVB5	13596	29089	0.61%	0.054%
24	15.892	2189	2194	2199	rVB6	6405	10790	0.23%	0.020%
25	16.175	2236	2242	2246	rBV5	10167	15649	0.33%	0.029%
26	16.839	2351	2355	2359	rBV7	5034	6589	0.14%	0.012%
27	16.945	2370	2373	2384	rBV7	6687	17415	0.37%	0.033%
28	17.175	2405	2412	2423	rBV	2225378	3371548	71.00%	6.299%
29	17.275	2423	2429	2440	rVV2	2403536	4015174	84.56%	7.501%
30	17.869	2526	2530	2536	rBV9	8962	16402	0.35%	0.031%
31	18.110	2567	2571	2577	rBV8	13019	24826	0.52%	0.046%
32	19.204	2753	2757	2761	rBV	36974	50010	1.05%	0.093%
33	19.280	2766	2770	2774	rBV	30741	46967	0.99%	0.088%
34	19.663	2828	2835	2843	rBV2	3007923	4748472	100.00%	8.871%
35	21.627	3163	3169	3185	rVB2	2018865	3636767	76.59%	6.794%
36	24.745	3689	3699	3712	rVB2	1637259	4665606	98.25%	8.716%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070824\
Data File : BP020871.D
Acq On : 09 Jul 2024 20:36
Operator : MA/JU
Sample : PB161916BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK916

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Title : SVOA CALIBRATION

37	24.974	3729	3738	3751	rVB	1222288	3744568	78.86%	6.996%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 53526979

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070824\
Data File : BP020871.D
Acq On : 09 Jul 2024 20:36
Operator : MA/JU
Sample : PB161916BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK916

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

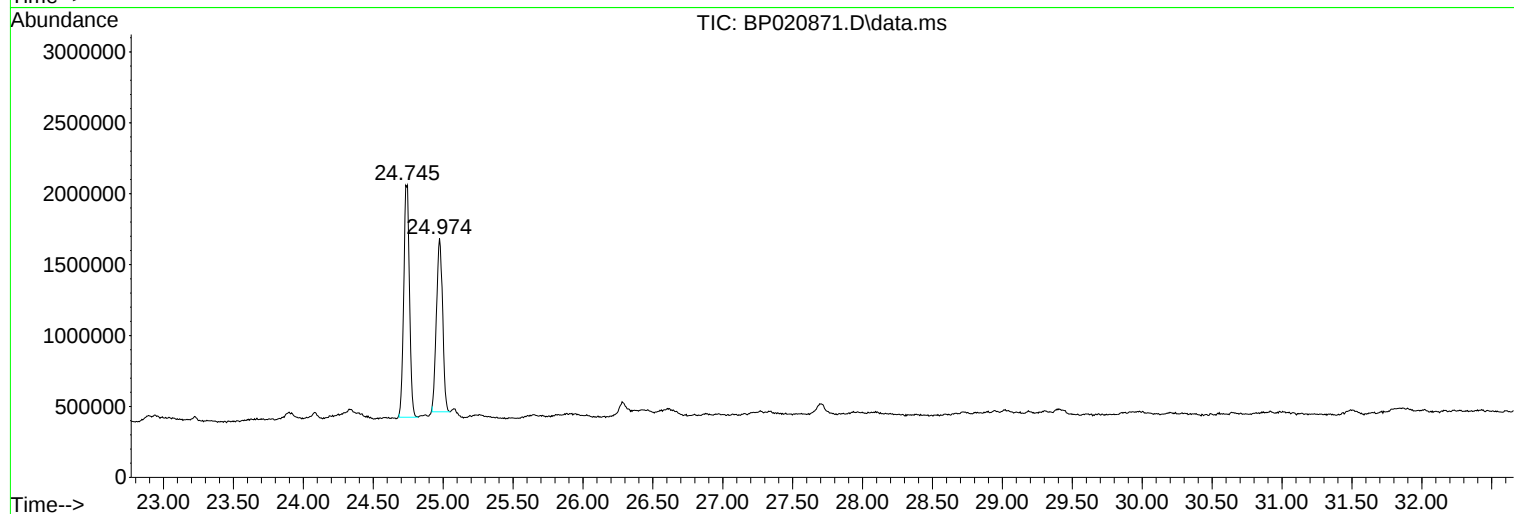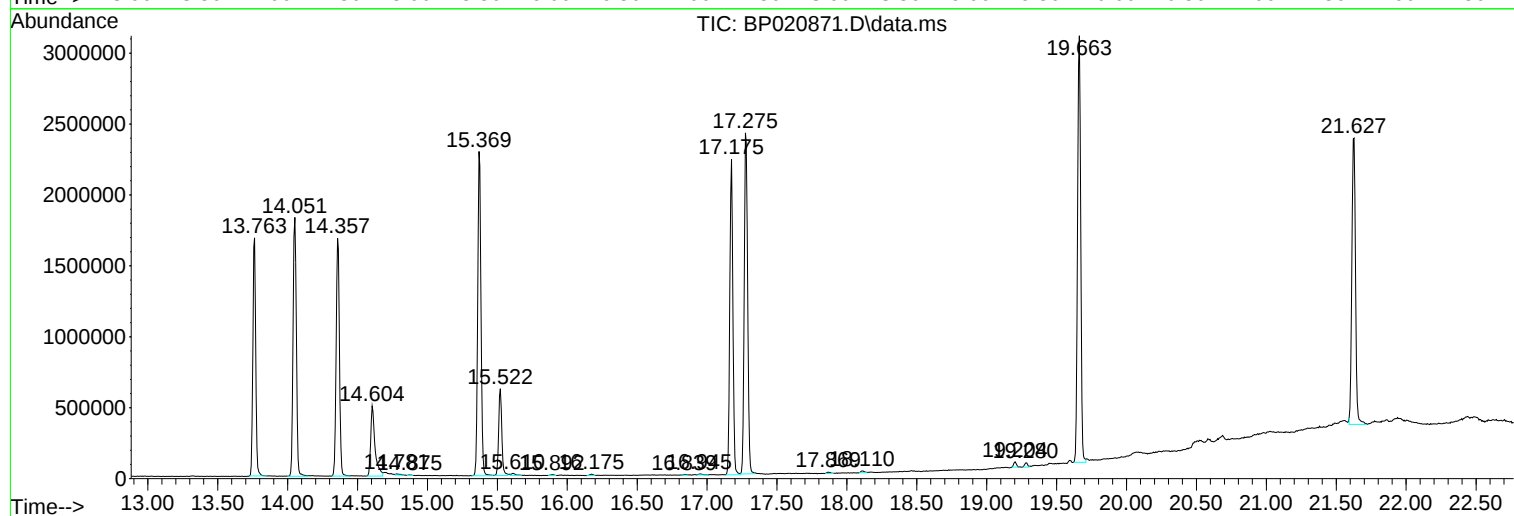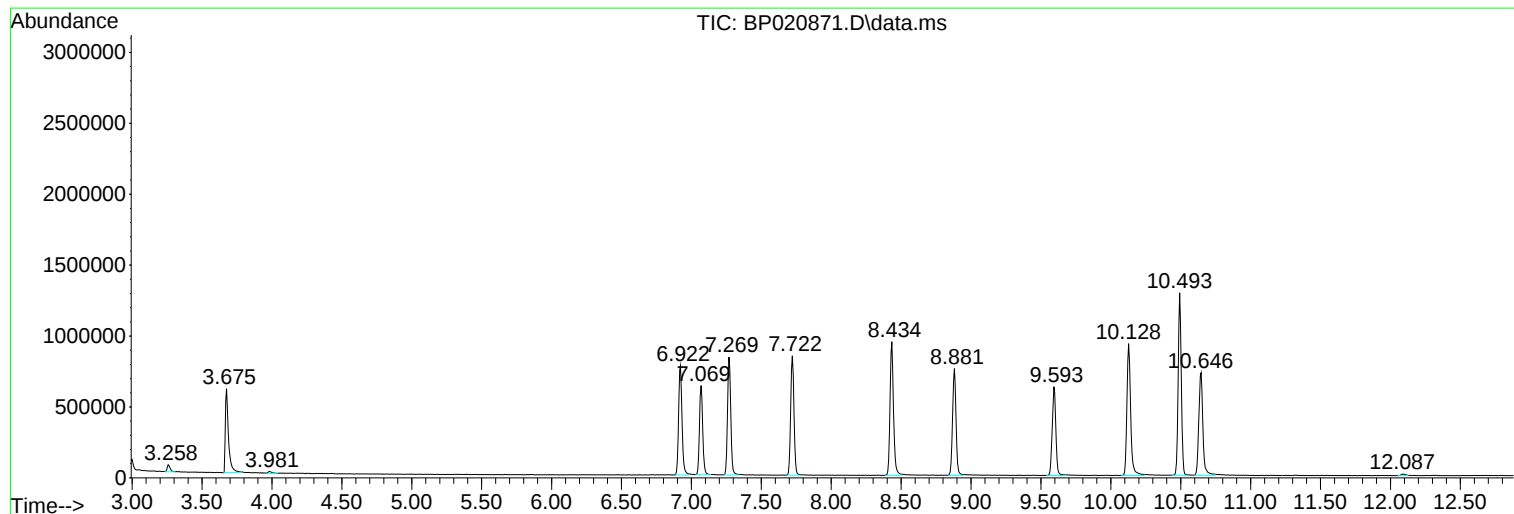

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070824\
Data File : BP020871.D
Acq On : 09 Jul 2024 20:36
Operator : MA/JU
Sample : PB161916BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK916

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070824\
Data File : BP020871.D
Acq On : 09 Jul 2024 20:36
Operator : MA/JU
Sample : PB161916BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK916

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc