
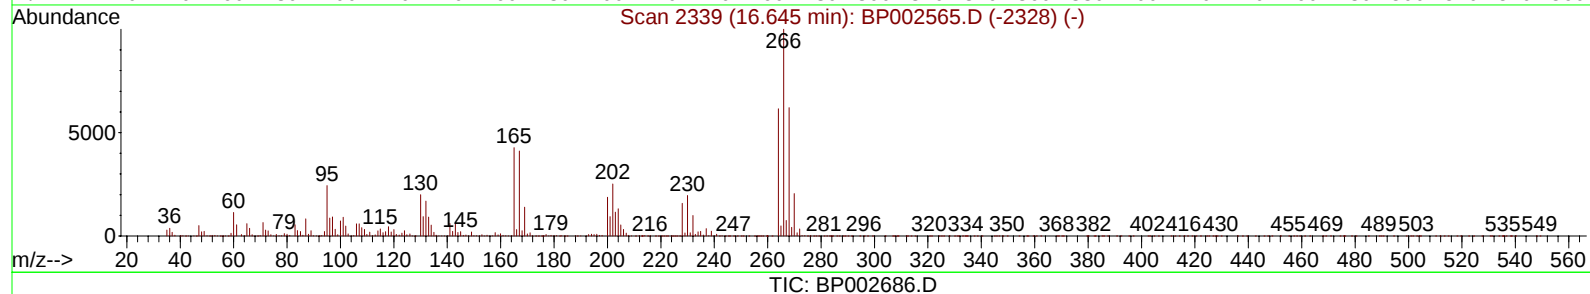
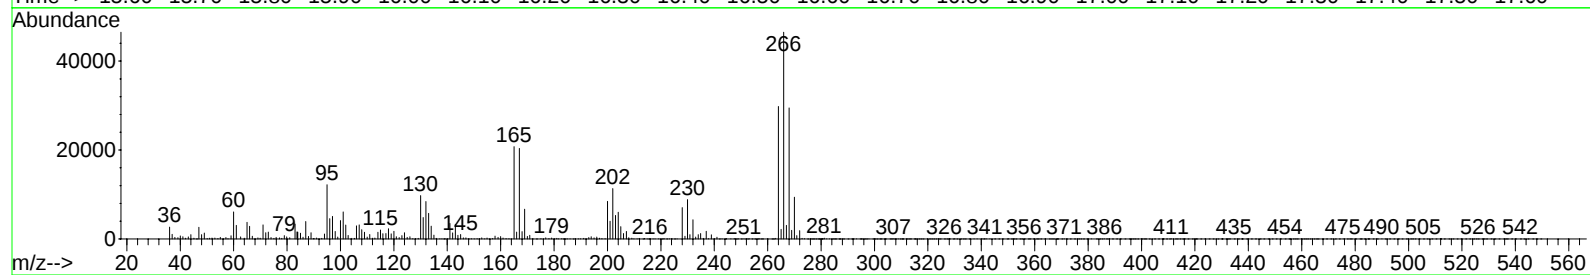


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP070920\
Data File : BP002686.D
Acq On : 09 Jul 2020 08:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 09 17:32:37 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP062920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 29 16:51:57 2020
Response via : Initial Calibration

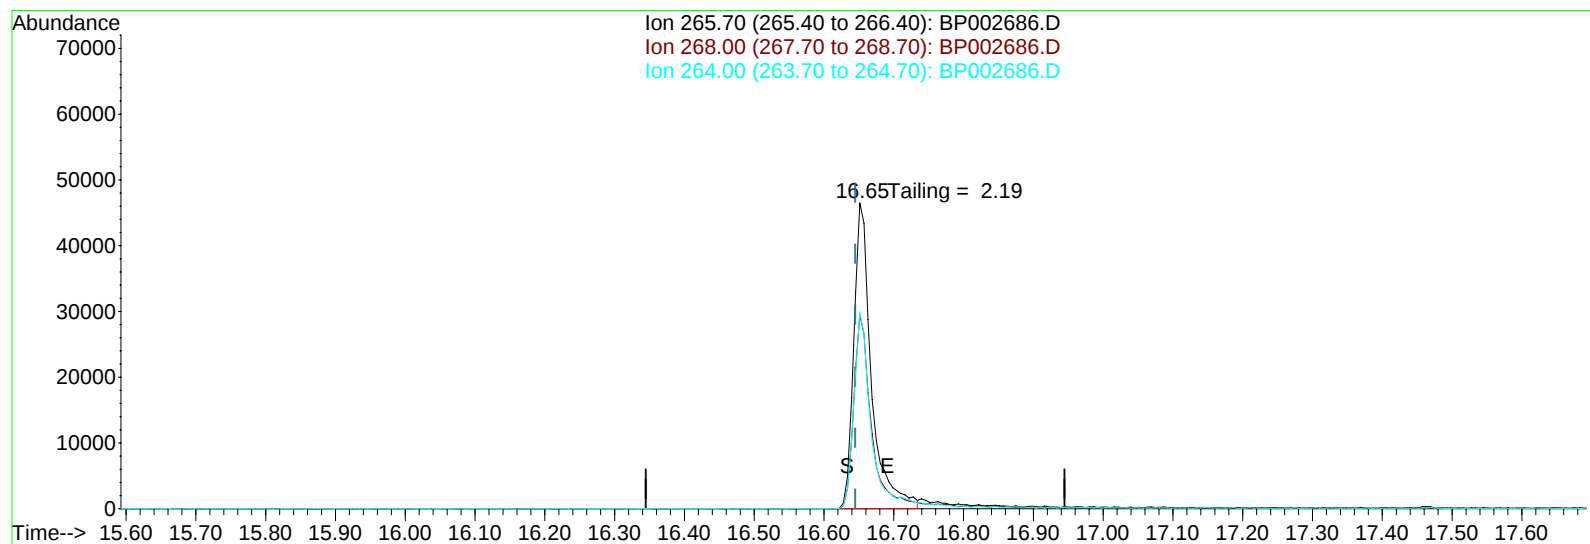

(70) Pentachlorophenol (C)




16.651min (+0.006) 221978.59ng

response 71090

Ion	Exp%	Act%
265.70	100	100
268.00	62.10	63.40
264.00	61.60	64.09
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP070920\
Data File : BP002686.D
Acq On : 09 Jul 2020 08:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 09 17:32:37 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP062920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 29 16:51:57 2020
Response via : Initial Calibration

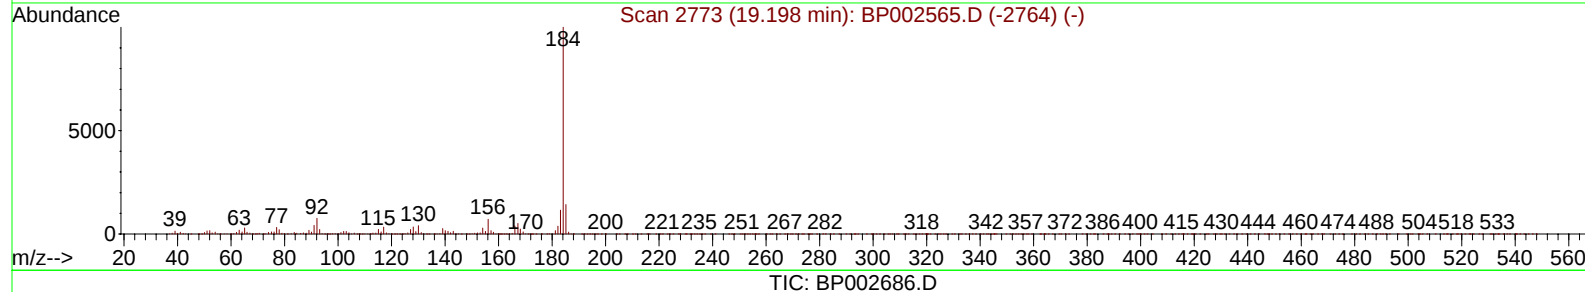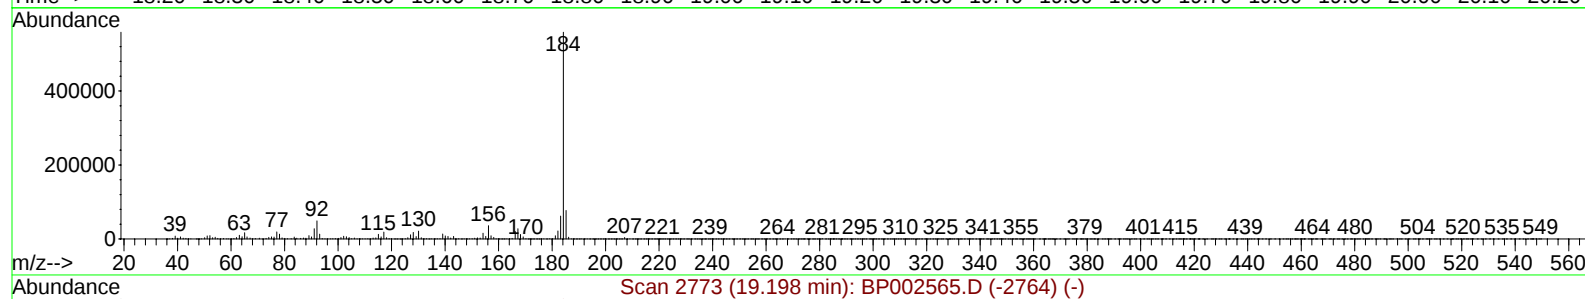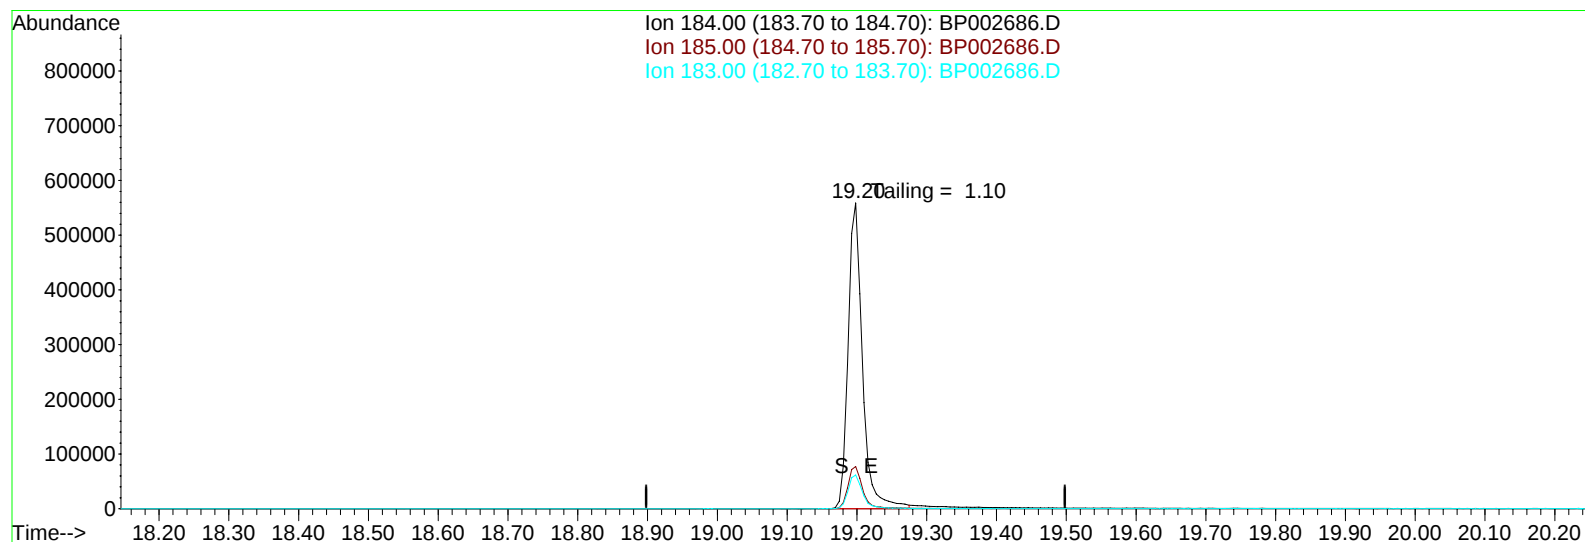

(77) Benzidine

19.198min (-19.198) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	14.30	0.00#
183.00	11.50	0.00#
0.00	0.00	0.00