
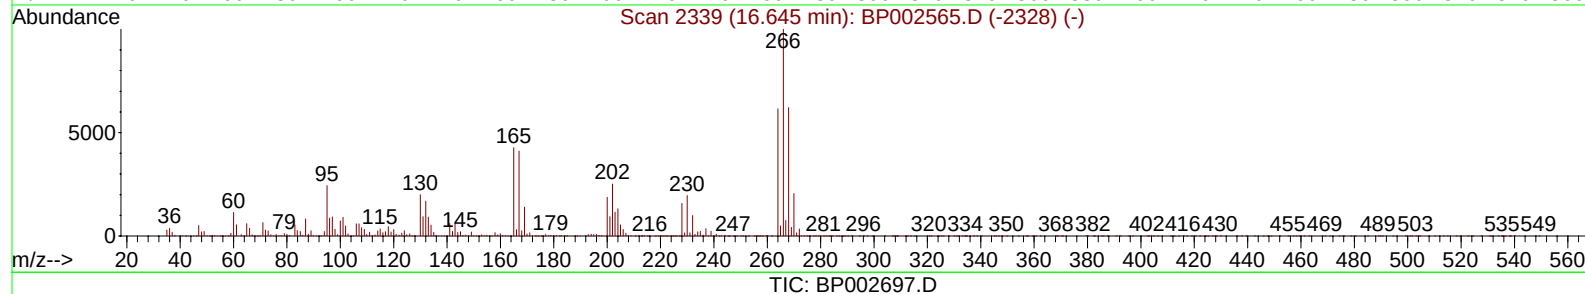
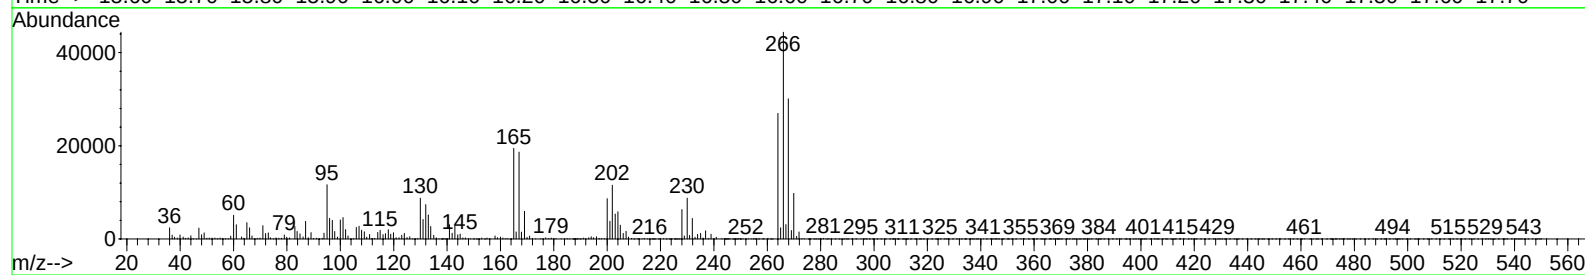


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP070920\
Data File : BP002697.D
Acq On : 09 Jul 2020 14:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 09 17:38:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP062920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 29 16:51:57 2020
Response via : Initial Calibration

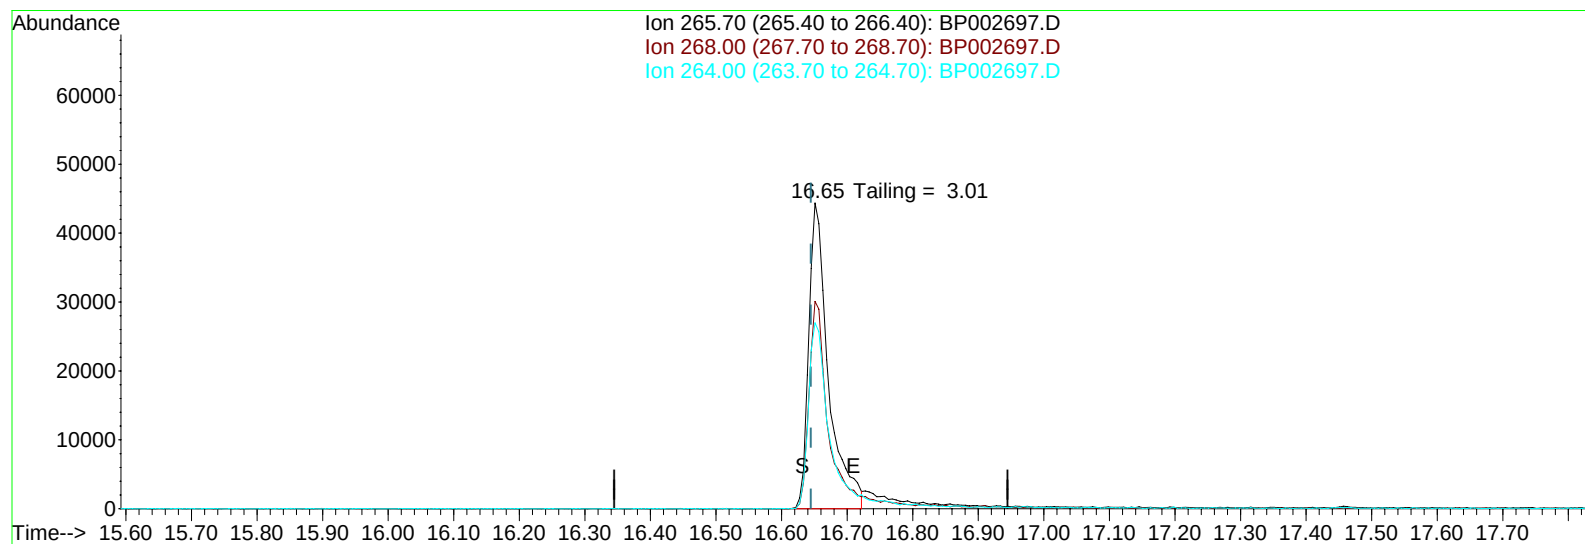

(70) Pentachlorophenol (C)




16.651min (+0.006) 24104.20ng

response 101373

Ion	Exp%	Act%
265.70	100	100
268.00	62.10	67.80
264.00	61.60	60.79
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP070920\
Data File : BP002697.D
Acq On : 09 Jul 2020 14:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 09 17:38:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP062920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 29 16:51:57 2020
Response via : Initial Calibration

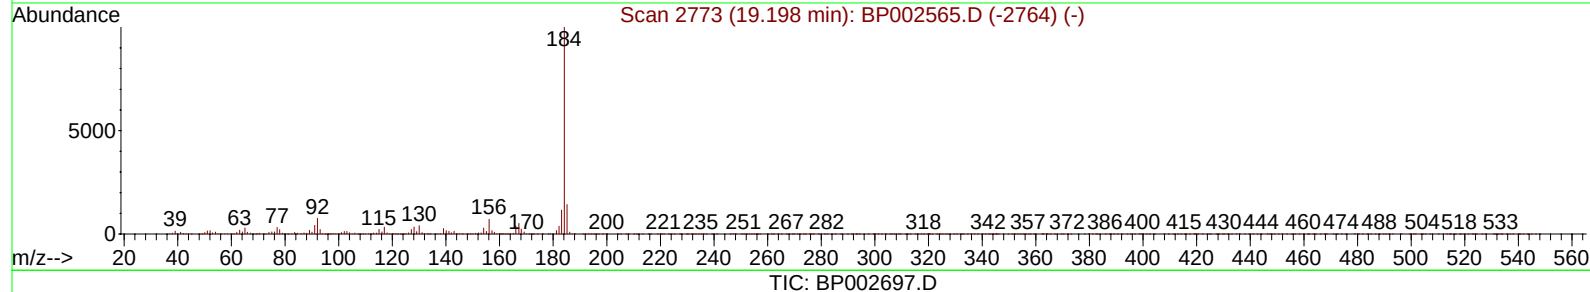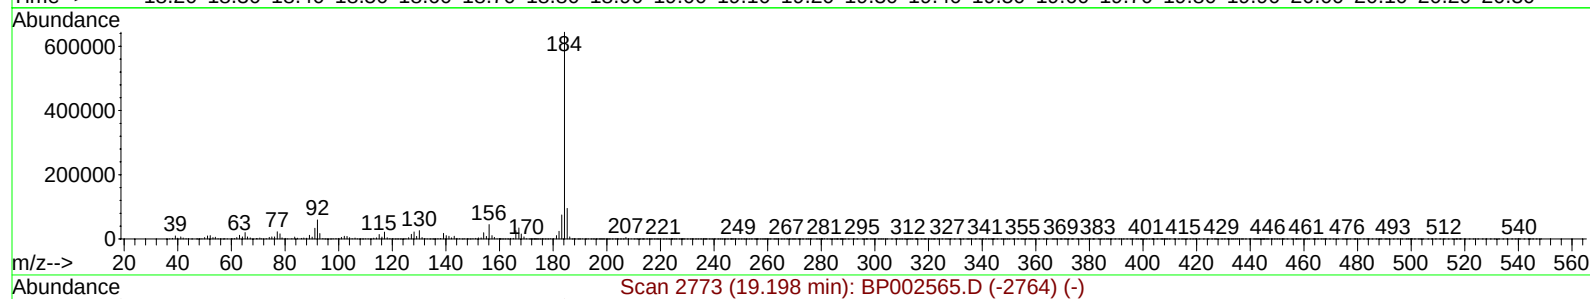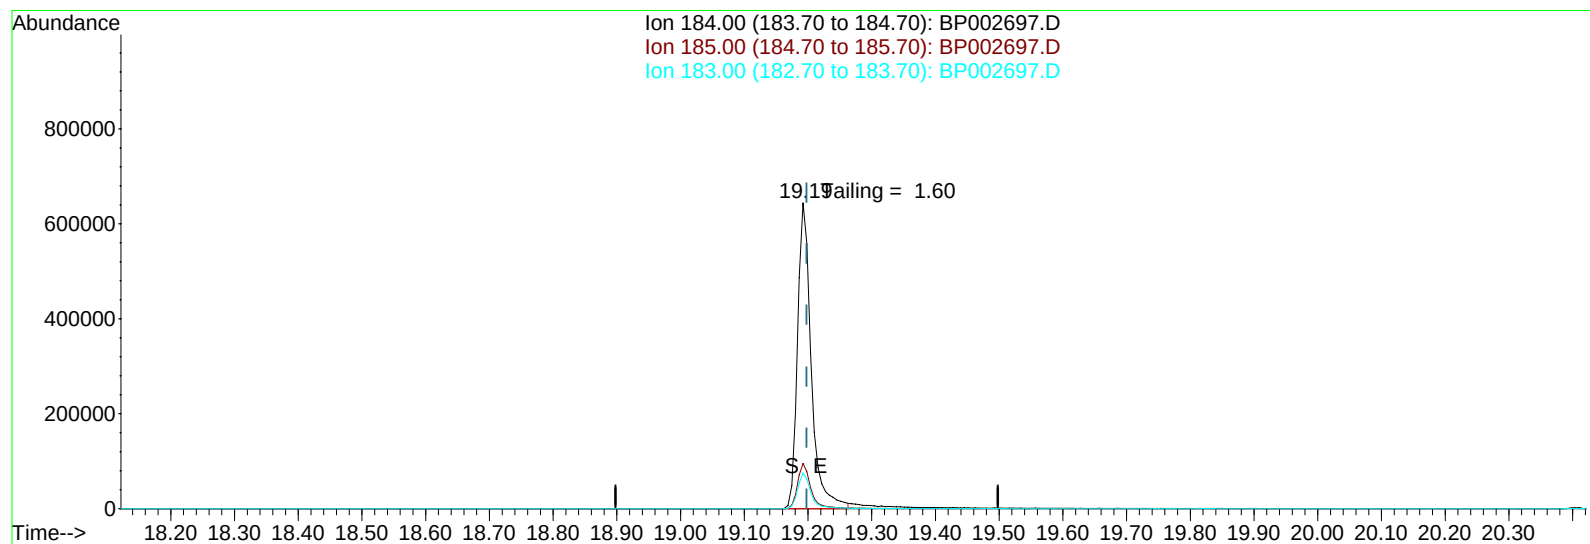

(77) Benzidine

19.192min (-0.006) -20.00ng

response 1005079

Ion	Exp%	Act%
184.00	100	100
185.00	14.30	14.80
183.00	11.50	11.65
0.00	0.00	0.00