

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP070920\
 Data File : BP002690.D
 Acq On : 09 Jul 2020 10:39
 Operator : CG/JU
 Sample : PB129999BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB129999BL

Quant Time: Jul 09 14:16:36 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP062920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 29 16:51:57 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	200736	20.00	ng	0.00
21) Naphthalene-d8	10.34	136	763823	20.00	ng	0.00
39) Acenaphthene-d10	14.22	164	448835	20.00	ng	0.00
64) Phenanthrene-d10	16.98	188	940687	20.00	ng	0.00
76) Chrysene-d12	21.09	240	902336	20.00	ng	0.00
86) Perylene-d12	23.28	264	945485	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.19	112	1436891	121.19	ng	0.00
7) Phenol-d6	6.77	99	1861727	112.50	ng	0.00
23) Nitrobenzene-d5	8.71	82	1236935	83.44	ng	-0.01
42) 2,4,6-Tribromophenol	15.72	330	636923	116.67	ng	0.00
45) 2-Fluorobiphenyl	12.83	172	2541146	83.33	ng	0.00
79) Terphenyl-d14	19.57	244	3611846	86.40	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP070920\
Data File : BP002690.D
Acq On : 09 Jul 2020 10:39
Operator : CG/JU
Sample : PB129999BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129999BL

Quant Time: Jul 09 14:16:36 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP062920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 29 16:51:57 2020
Response via : Initial Calibration

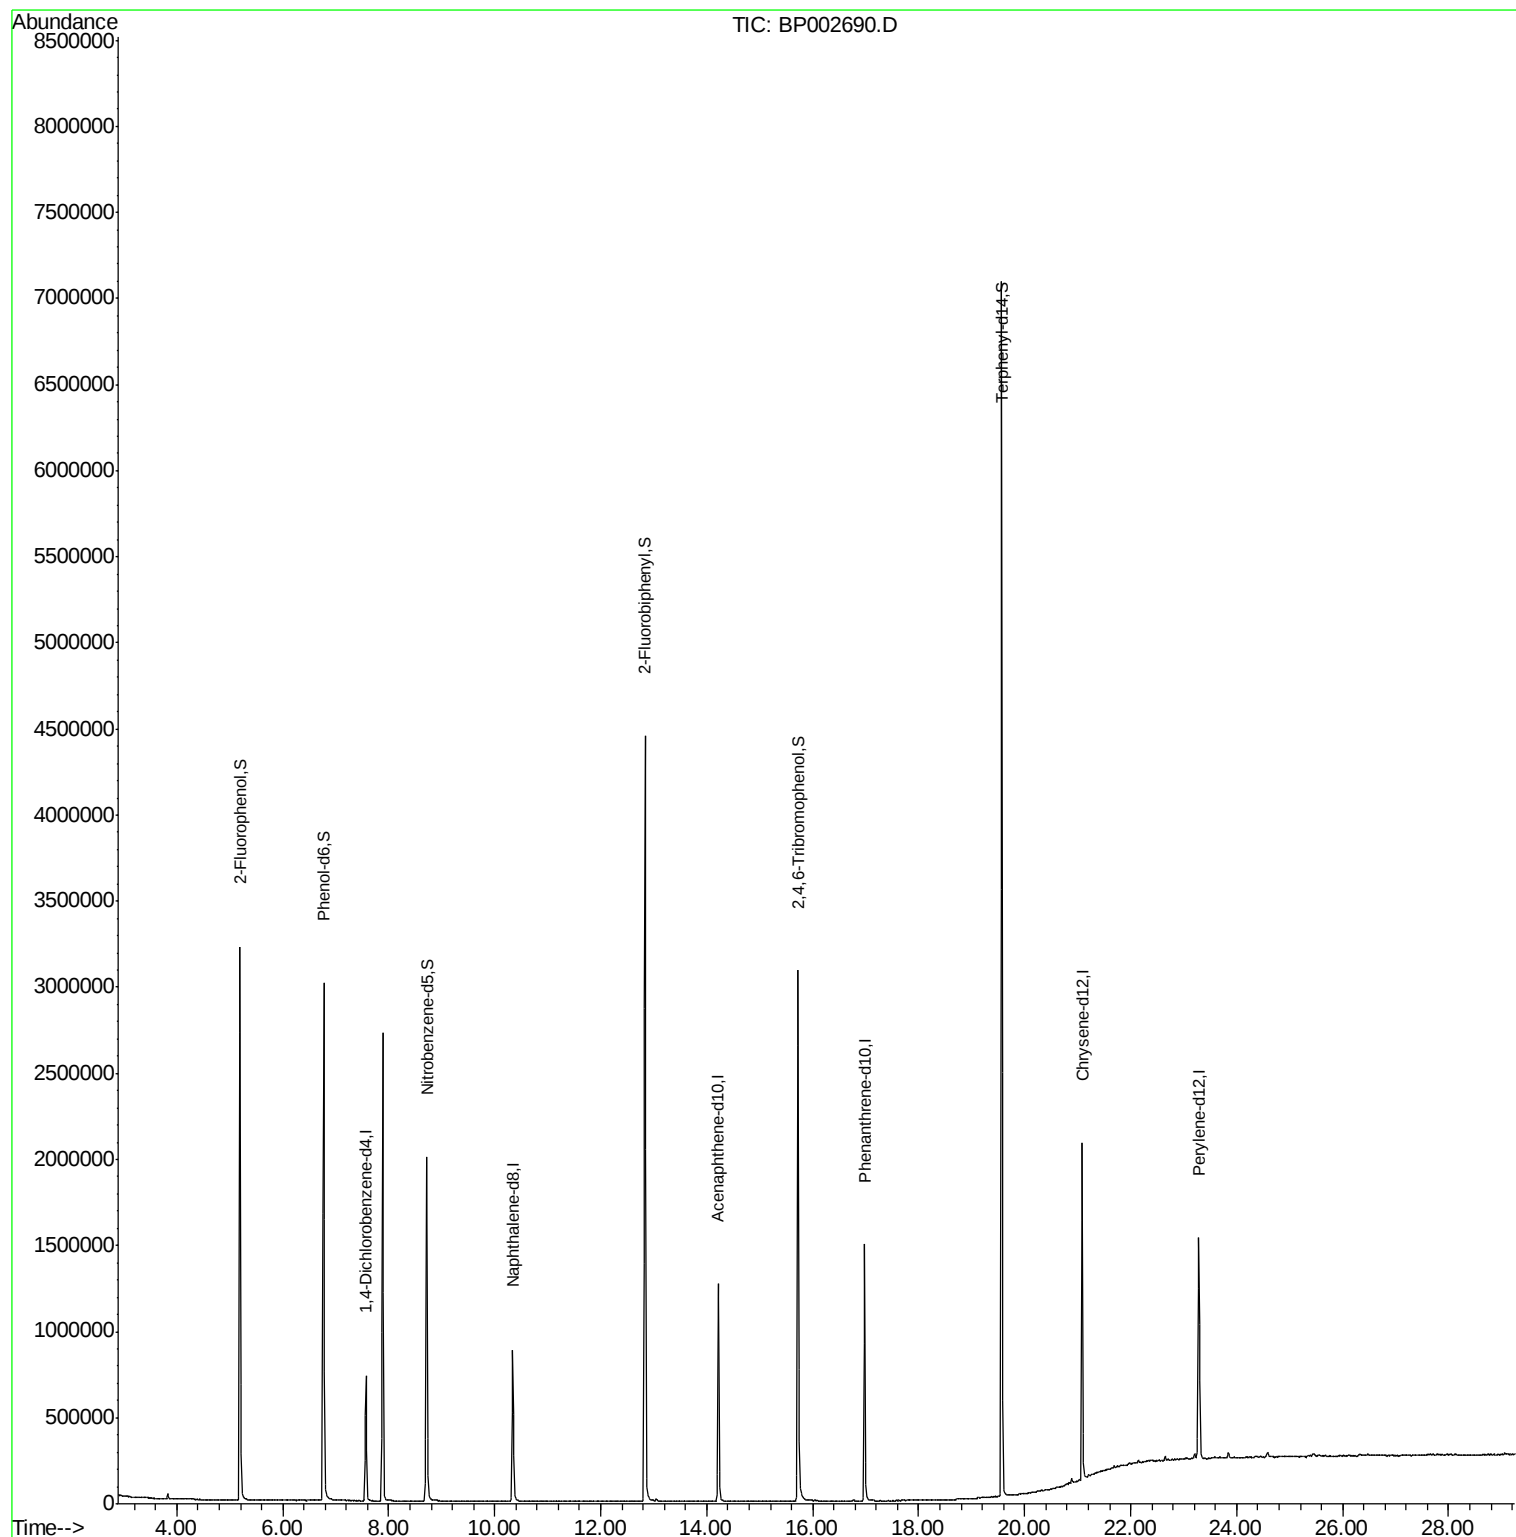







#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.57 min Scan# 796
Delta R.T. -0.01 min
Lab File: BP002690.D
Acq: 09 Jul 2020 10:39

Instrument :
BNA_P
ClientSampleId :
PB129999BL




Tot Ion	Ratio	Lower	Upper
152	100		
150	155.9	124.2	186.2
115	58.7	47.1	70.7

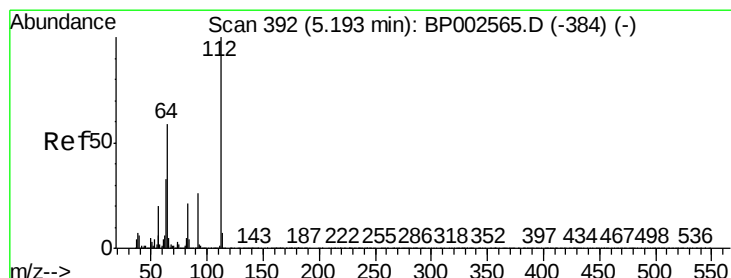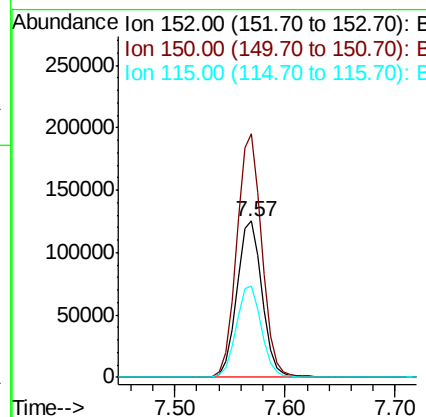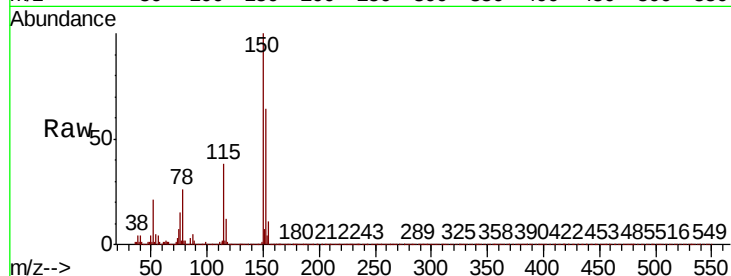


#5

2-Fluorophenol
Concen: 121.195 ng
RT: 5.19 min Scan# 392
Delta R.T. -0.00 min
Lab File: BP002690.D
Acq: 09 Jul 2020 10:39

Tgt Ion	Ratio	Lower	Upper
112	100		
64	57.4	47.0	70.6
63	30.0	26.1	39.1

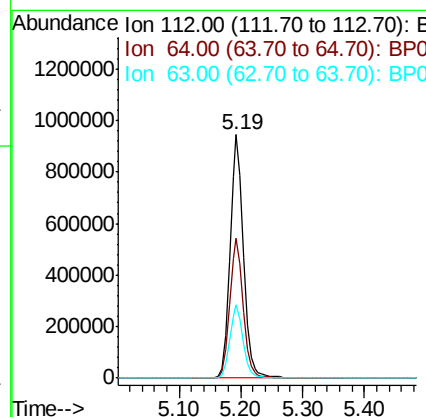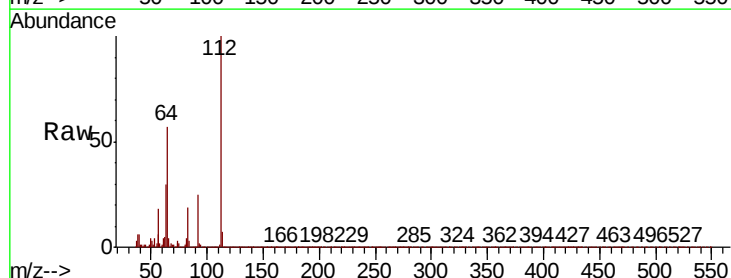

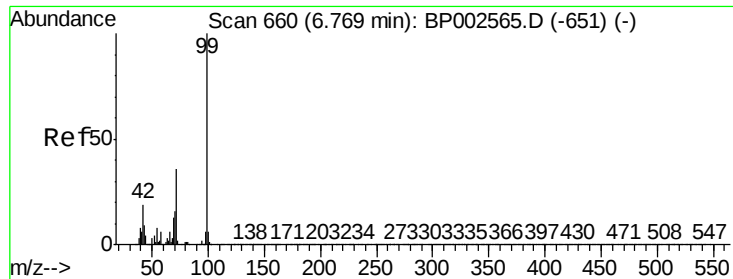

#7

Phenol-d6

Concen: 112.505 ng

RT: 6.77 min Scan# 660

Delta R.T. -0.00 min

Lab File: BP002690.D

Acq: 09 Jul 2020 10:39

Instrument :





BNA_P

ClientSampleId :

PB129999BL

Tot Ion: 99 Resp: 1861727

Ion	Ratio	Lower	Upper
99	100		
42	17.4	15.5	23.3
71	31.9	28.9	43.3

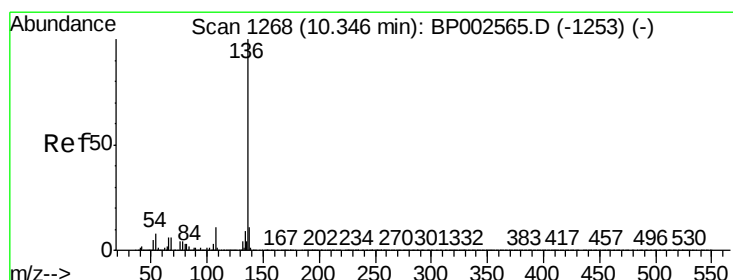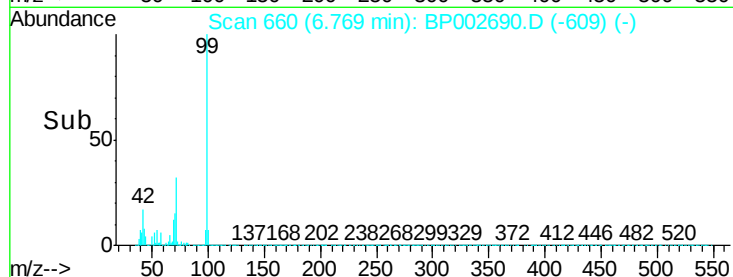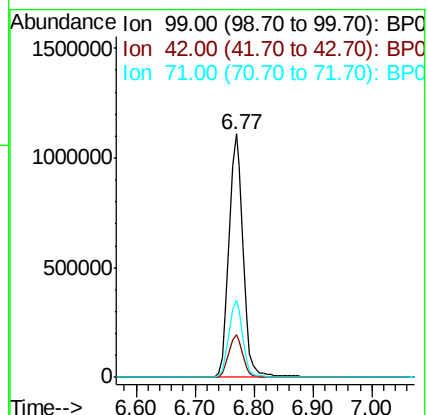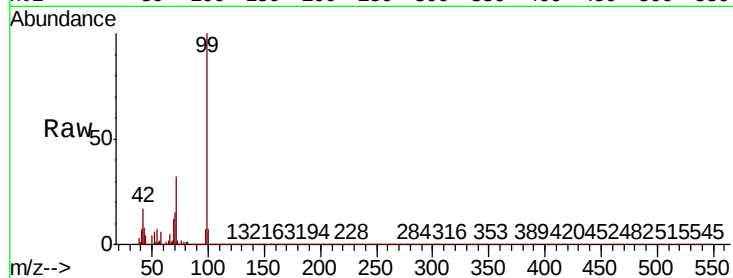

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.34 min Scan# 1267




Delta R.T. -0.01 min

Lab File: BP002690.D

Acq: 09 Jul 2020 10:39

Tgt Ion: 136 Resp: 763823

Ion	Ratio	Lower	Upper
136	100		
137	10.9	8.8	13.2
54	8.9	6.4	9.6
68	7.5	5.1	7.7


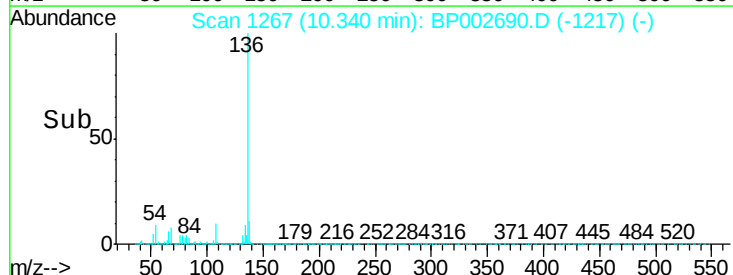
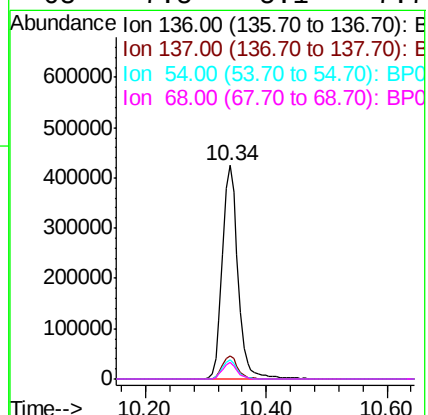
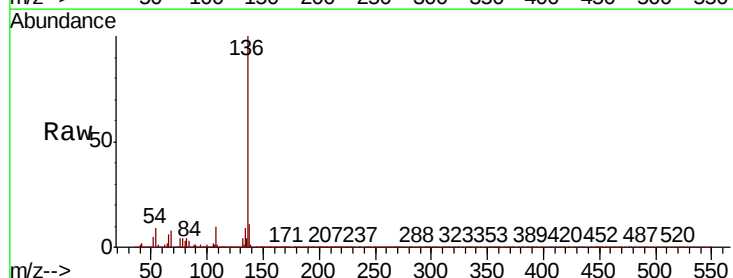




#23
Nitrobenzene-d5
Concen: 83.440 ng
RT: 8.71 min Scan# 990
Delta R.T. -0.01 min
Lab File: BP002690.D
Acq: 09 Jul 2020 10:39




Instrument :
BNA_P
ClientSampleId :
PB129999BL


Tot Ion: 82 Resp: 1236935
Ion Ratio Lower Upper
82 100
128 41.1 33.4 50.2
54 47.3 40.1 60.1

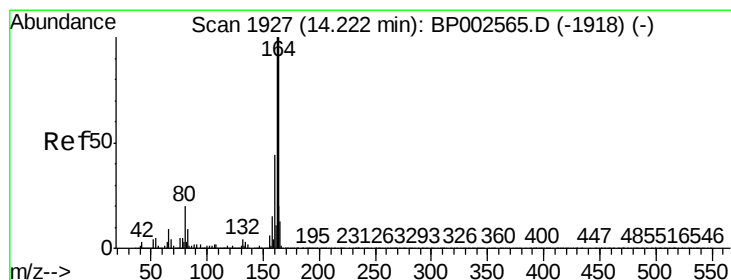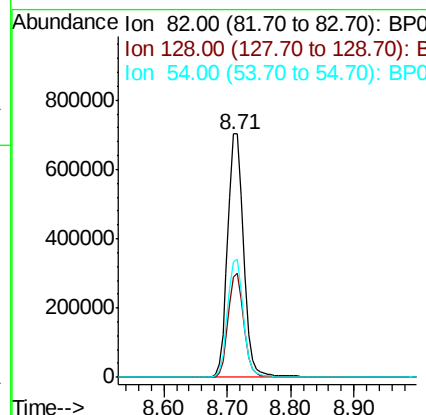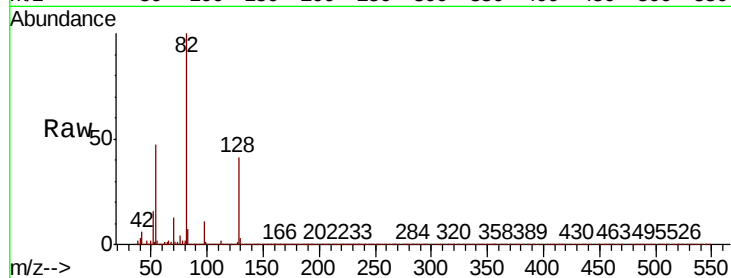

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.22 min Scan# 1926
Delta R.T. -0.01 min
Lab File: BP002690.D
Acq: 09 Jul 2020 10:39

Tgt Ion:164 Resp: 448835
Ion Ratio Lower Upper
164 100
162 100.0 80.3 120.5
160 44.5 35.0 52.6

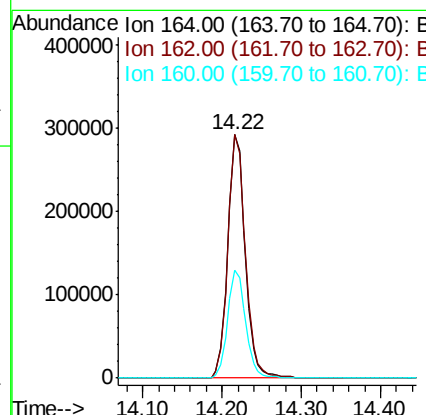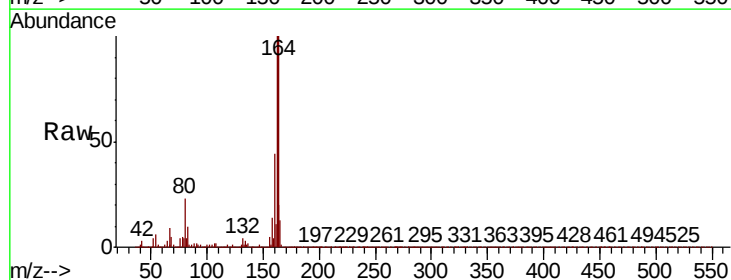


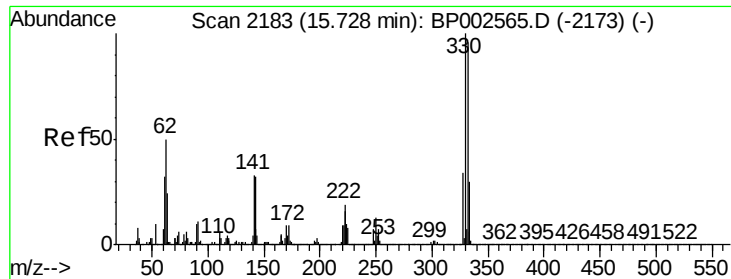




#42
2,4,6-Tribromophenol
Concen: 116.672 ng
RT: 15.72 min Scan# 2182
Delta R.T. -0.01 min
Lab File: BP002690.D
Acq: 09 Jul 2020 10:39

Instrument :
BNA_P
ClientSampleId :
PB129999BL

Tot Ion:330 Resp: 636923
Ion Ratio Lower Upper
330 100
332 95.1 77.7 116.5
141 33.9 29.0 43.6

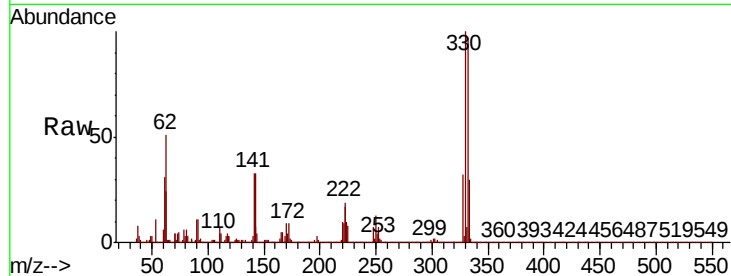


Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

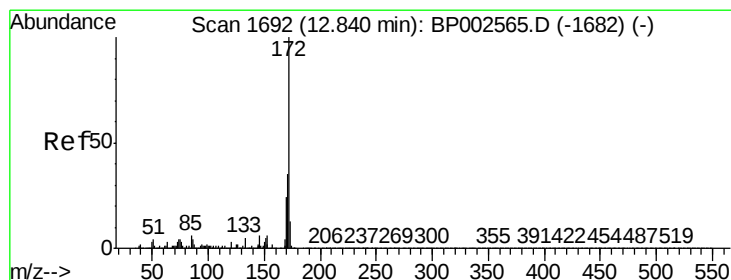
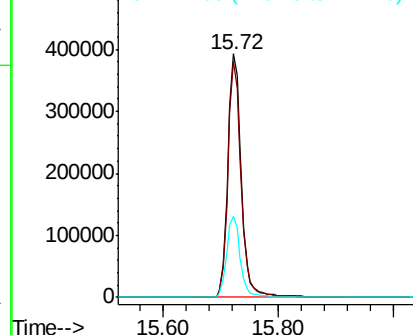



#45
2-Fluorobiphenyl
Concen: 83.330 ng
RT: 12.83 min Scan# 1691
Delta R.T. -0.01 min
Lab File: BP002690.D
Acq: 09 Jul 2020 10:39

Tgt Ion:172 Resp: 2541146
Ion Ratio Lower Upper
172 100
171 35.3 28.0 42.0
170 24.3 19.0 28.4

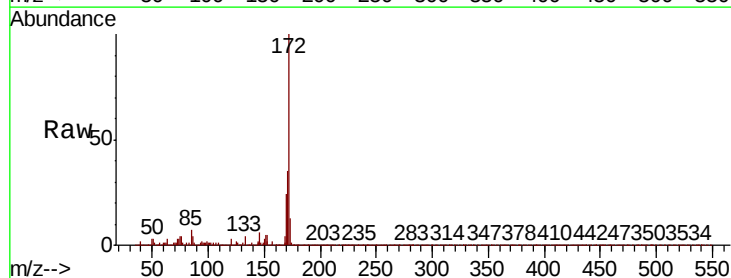

Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

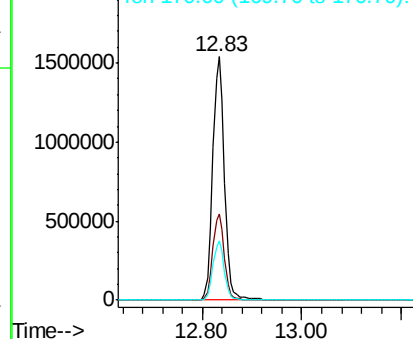



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 16.98 min Scan# 2396

Delta R.T. -0.00 min

Lab File: BP002690.D

Acq: 09 Jul 2020 10:39

Instrument :

BNA_P

ClientSampleId :

PB129999BL


Tot Ion:188 Resp: 940687

Ion Ratio Lower Upper

188 100

94 9.7 7.8 11.6




80 10.6 8.2 12.4

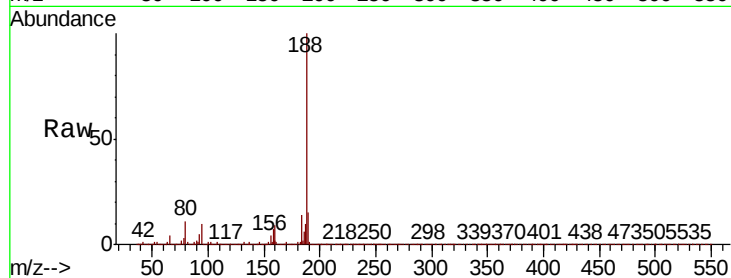

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BP0

Ion 80.00 (79.70 to 80.70): BP0

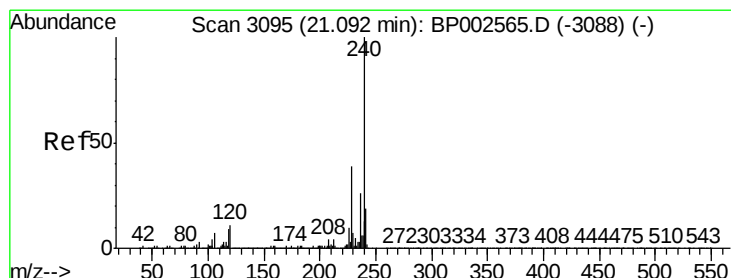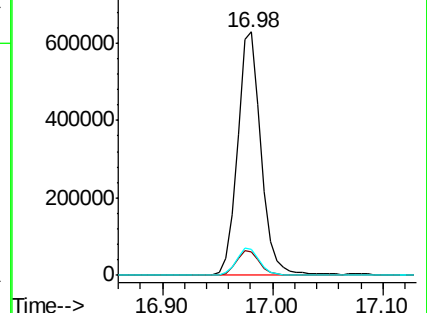

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.09 min Scan# 3094

Delta R.T. -0.01 min

Lab File: BP002690.D

Acq: 09 Jul 2020 10:39


Tgt Ion:240 Resp: 902336

Ion Ratio Lower Upper

240 100

120 11.7 8.6 13.0



236 27.5 20.8 31.2

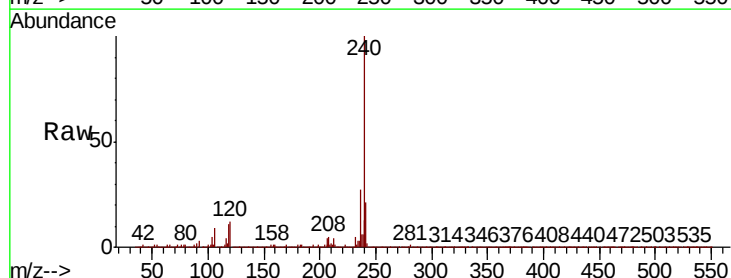


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

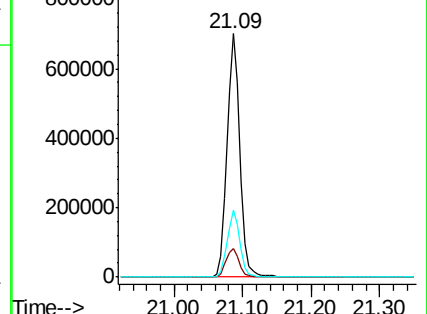

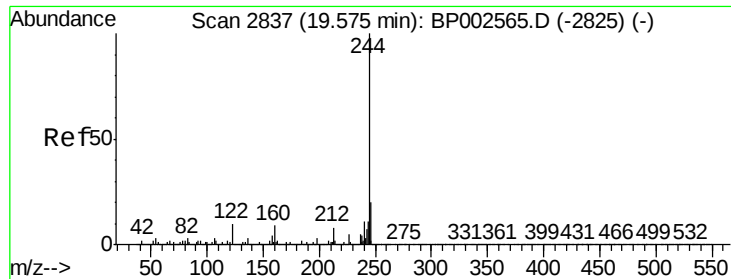

#79

Terphenyl-d14

Concen: 86.399 ng

RT: 19.57 min Scan# 2836

Delta R.T. -0.01 min

Lab File: BP002690.D

Acq: 09 Jul 2020 10:39

Instrument :

BNA_P

ClientSampleId :

PB129999BL


Tot Ion:244 Resp: 3611846

Ion Ratio Lower Upper

244 100

212 7.6 6.5 9.7




122 10.6 7.9 11.9

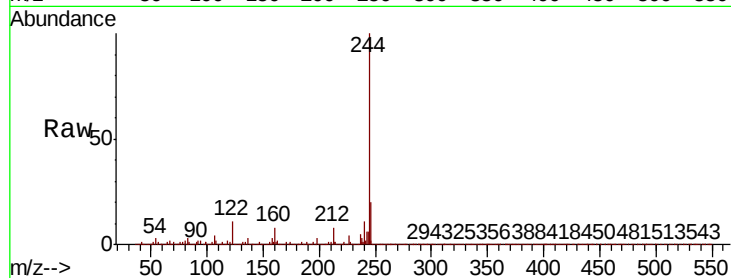

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

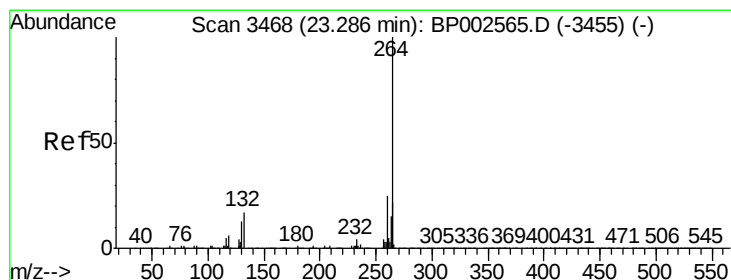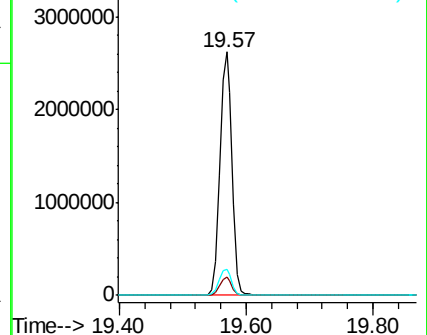

#86

Perylene-d12

Concen: 20.000 ng

RT: 23.28 min Scan# 3467

Delta R.T. -0.01 min

Lab File: BP002690.D

Acq: 09 Jul 2020 10:39


Tgt Ion:264 Resp: 945485

Ion Ratio Lower Upper

264 100

260 24.5 19.7 29.5

265 21.0 17.6 26.4

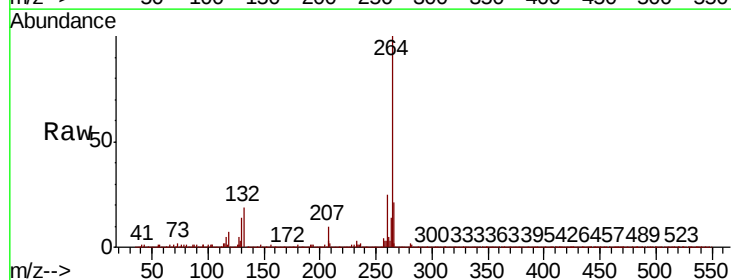

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

