

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP070920\
Data File : BP002688.D
Acq On : 09 Jul 2020 09:31
Operator : CG/JU
Sample : PB130021BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB130021BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.193	386	392	407	rBV	3317474	5016062	50.87%	9.389%
2	6.769	653	660	684	rBV	3072353	5196987	52.70%	9.728%
3	7.569	789	796	810	rBV	737200	1164765	11.81%	2.180%
4	7.887	842	850	864	rBV	2839996	4645696	47.11%	8.696%
5	8.716	982	991	1007	rBV	2111965	3619428	36.70%	6.775%
6	10.340	1259	1267	1287	rBV	883796	1543867	15.66%	2.890%
7	12.834	1683	1691	1715	rBV	4657871	7535718	76.42%	14.106%
8	14.216	1918	1926	1949	rBV	1250357	2015596	20.44%	3.773%
9	15.722	2173	2182	2214	rBV	3168437	5263547	53.38%	9.853%
10	16.981	2389	2396	2410	rBV	1538919	2287049	23.19%	4.281%
11	19.569	2830	2836	2856	rBV	7204053	9860959	100.00%	18.458%
12	21.086	3089	3094	3105	rBV	2085761	2631693	26.69%	4.926%
13	23.286	3461	3468	3479	rVB2	1397701	2641554	26.79%	4.945%




Sum of corrected areas: 53422921

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP070920\
Data File : BP002688.D
Acq On : 09 Jul 2020 09:31
Operator : CG/JU
Sample : PB130021BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB130021BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP062920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

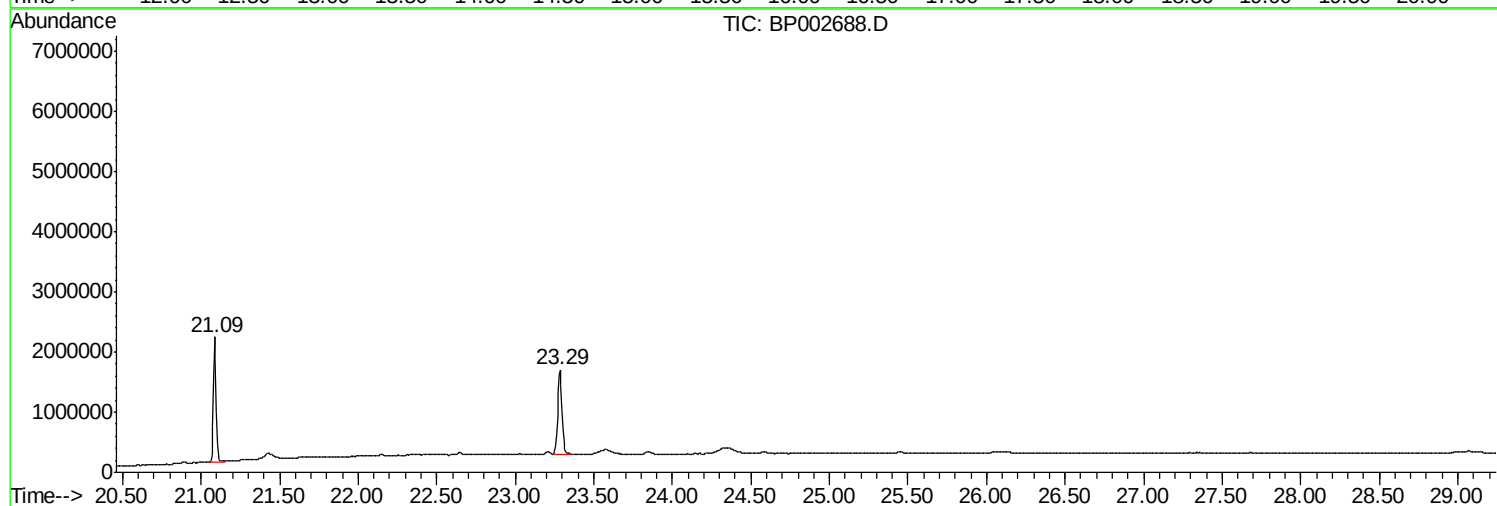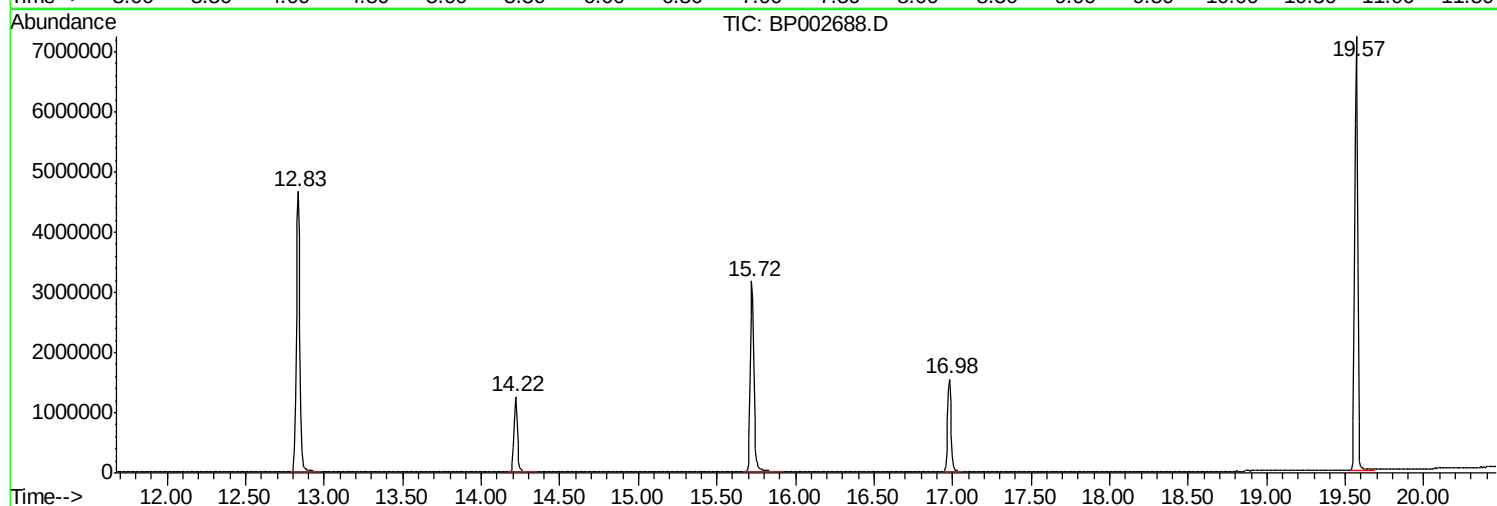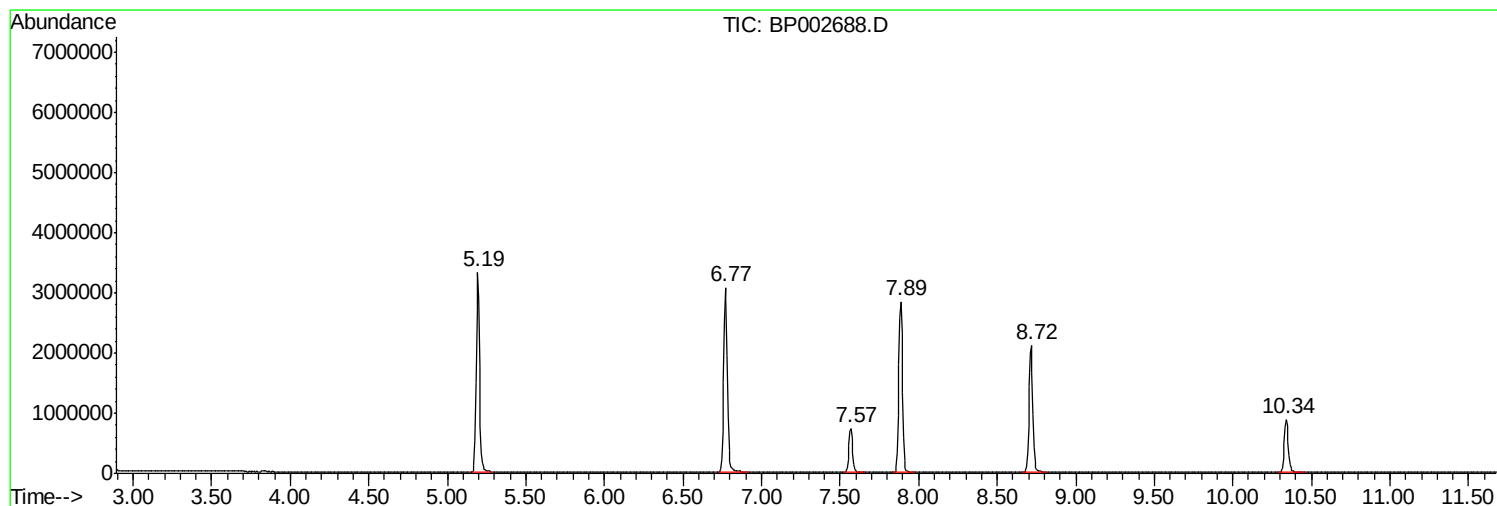

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP070920\
Data File : BP002688.D
Acq On : 09 Jul 2020 09:31
Operator : CG/JU
Sample : PB130021BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB130021BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP070920\
Data File : BP002688.D
Acq On : 09 Jul 2020 09:31
Operator : CG/JU
Sample : PB130021BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB130021BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc