

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP070920\  
 Data File : BP002689.D  
 Acq On : 09 Jul 2020 10:05  
 Operator : CG/JU  
 Sample : PB129997BL  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 PB129997BL

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP062920.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.193       | 386           | 392         | 416          | rBV      | 3249398        | 4962654       | 52.80%          | 9.620%        |
| 2         | 6.769       | 653           | 660         | 683          | rBV      | 3007946        | 5097697       | 54.24%          | 9.882%        |
| 3         | 7.569       | 789           | 796         | 806          | rBV      | 699676         | 1117745       | 11.89%          | 2.167%        |
| 4         | 7.887       | 842           | 850         | 862          | rBV      | 2763506        | 4535492       | 48.25%          | 8.792%        |
| 5         | 8.716       | 983           | 991         | 1014         | rBV      | 2031987        | 3527283       | 37.53%          | 6.838%        |
| 6         | 10.340      | 1258          | 1267        | 1287         | rBV      | 842538         | 1481227       | 15.76%          | 2.871%        |
| 7         | 12.834      | 1682          | 1691        | 1717         | rBV      | 4571317        | 7388984       | 78.61%          | 14.324%       |
| 8         | 14.216      | 1918          | 1926        | 1945         | rBV2     | 1177047        | 1913321       | 20.36%          | 3.709%        |
| 9         | 15.722      | 2175          | 2182        | 2216         | rBV      | 3020362        | 5031516       | 53.53%          | 9.754%        |
| 10        | 16.981      | 2388          | 2396        | 2410         | rBV      | 1437668        | 2185915       | 23.26%          | 4.237%        |
| 11        | 19.569      | 2830          | 2836        | 2854         | rBV      | 7032792        | 9399153       | 100.00%         | 18.220%       |
| 12        | 21.086      | 3089          | 3094        | 3103         | rBV      | 1902033        | 2453168       | 26.10%          | 4.756%        |
| 13        | 23.286      | 3461          | 3468        | 3484         | rVB2     | 1252989        | 2491592       | 26.51%          | 4.830%        |




Sum of corrected areas: 51585747

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP070920\  
Data File : BP002689.D  
Acq On : 09 Jul 2020 10:05  
Operator : CG/JU  
Sample : PB129997BL  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB129997BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP062920.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

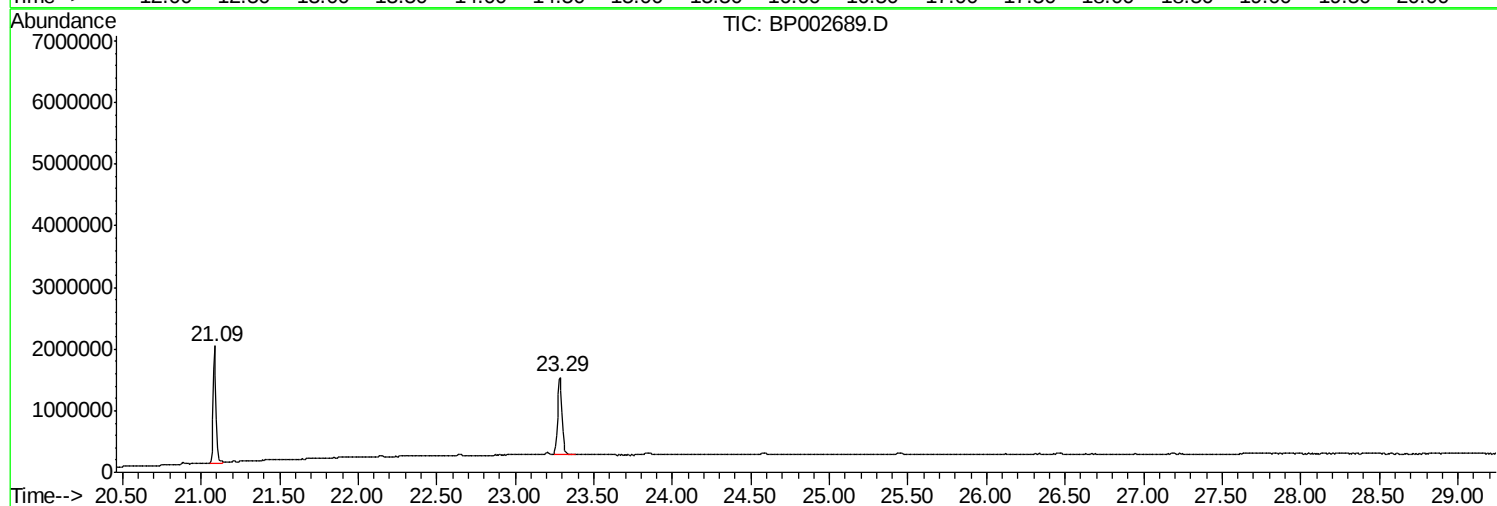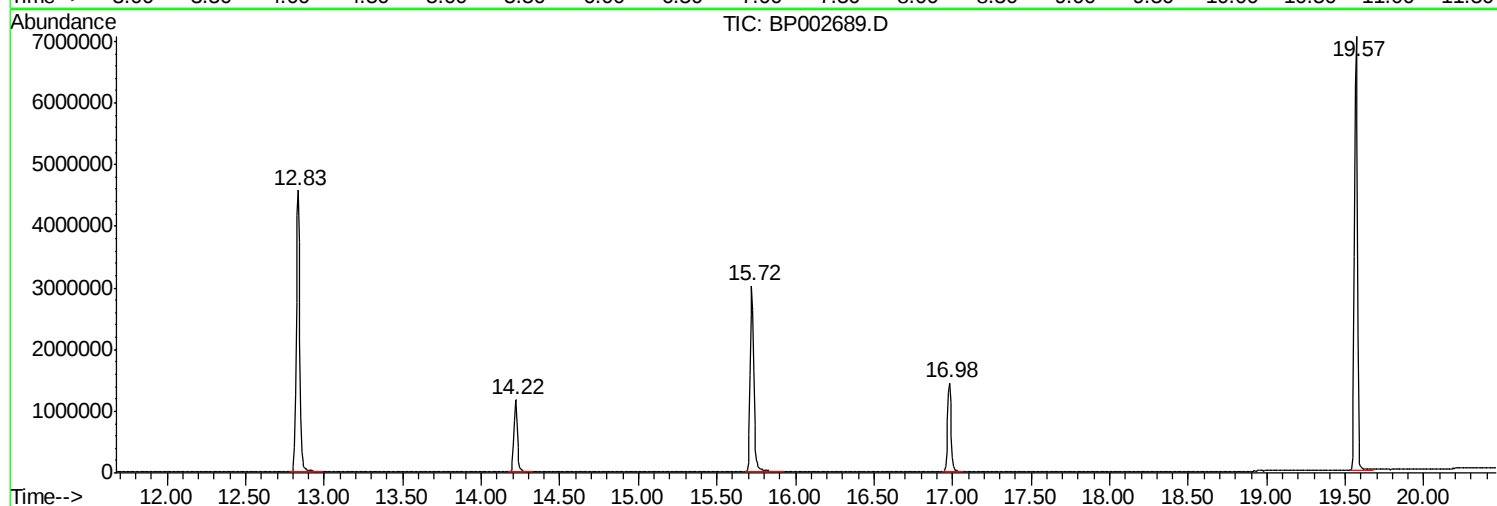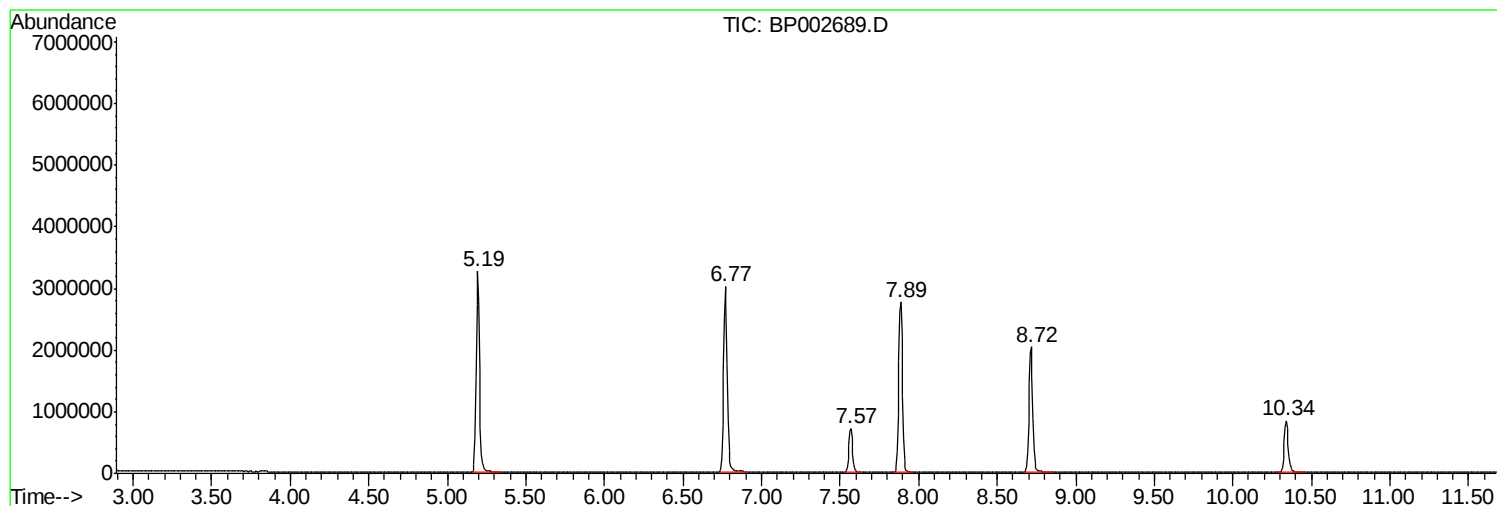

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_P\DATA\BP070920\  
Data File : BP002689.D  
Acq On : 09 Jul 2020 10:05  
Operator : CG/JU  
Sample : PB129997BL  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB129997BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP062920.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_P\DATA\BP070920\  
Data File : BP002689.D  
Acq On : 09 Jul 2020 10:05  
Operator : CG/JU  
Sample : PB129997BL  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB129997BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP062920.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |