

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP070920\
 Data File : BP002701.D
 Acq On : 09 Jul 2020 17:23
 Operator : CG/JU
 Sample : PB130037BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB130037BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.193	386	392	410	rBV	1062605	1794872	22.81%	5.947%
2	6.769	652	660	687	rBV	1101560	2074501	26.36%	6.874%
3	7.569	789	796	804	rBV	246439	409639	5.21%	1.357%
4	7.881	841	849	862	rBV	1038716	1764896	22.43%	5.848%
5	8.710	982	990	1019	rBV	839749	1545776	19.64%	5.122%
6	10.340	1260	1267	1286	rBV	353320	659820	8.38%	2.186%
7	12.828	1681	1690	1718	rBV	2306659	3872168	49.21%	12.831%
8	14.216	1919	1926	1946	rBV	638867	1052674	13.38%	3.488%
9	15.716	2175	2181	2205	rBV	1776463	3073823	39.06%	10.185%
10	16.975	2389	2395	2409	rBV	917425	1398083	17.77%	4.633%
11	19.563	2830	2835	2849	rBV	5863481	7869298	100.00%	26.075%
12	21.086	3089	3094	3104	rBV	1675161	2139852	27.19%	7.090%
13	23.280	3460	3467	3482	rVB2	1347344	2523937	32.07%	8.363%




Sum of corrected areas: 30179339

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP070920\
Data File : BP002701.D
Acq On : 09 Jul 2020 17:23
Operator : CG/JU
Sample : PB130037BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB130037BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP062920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

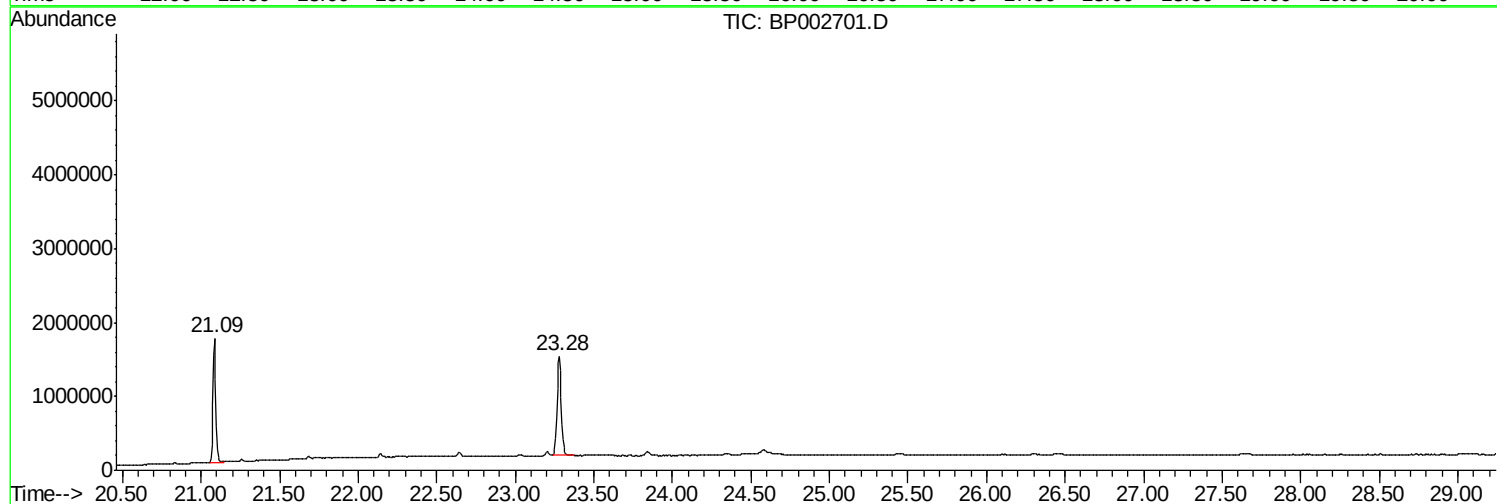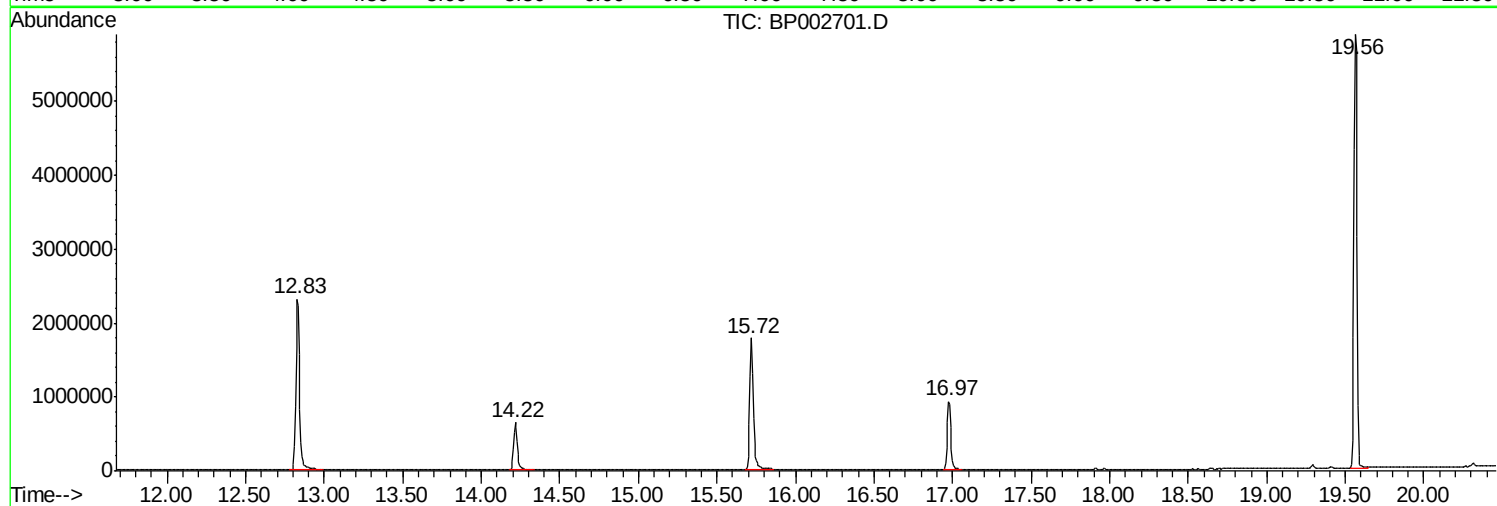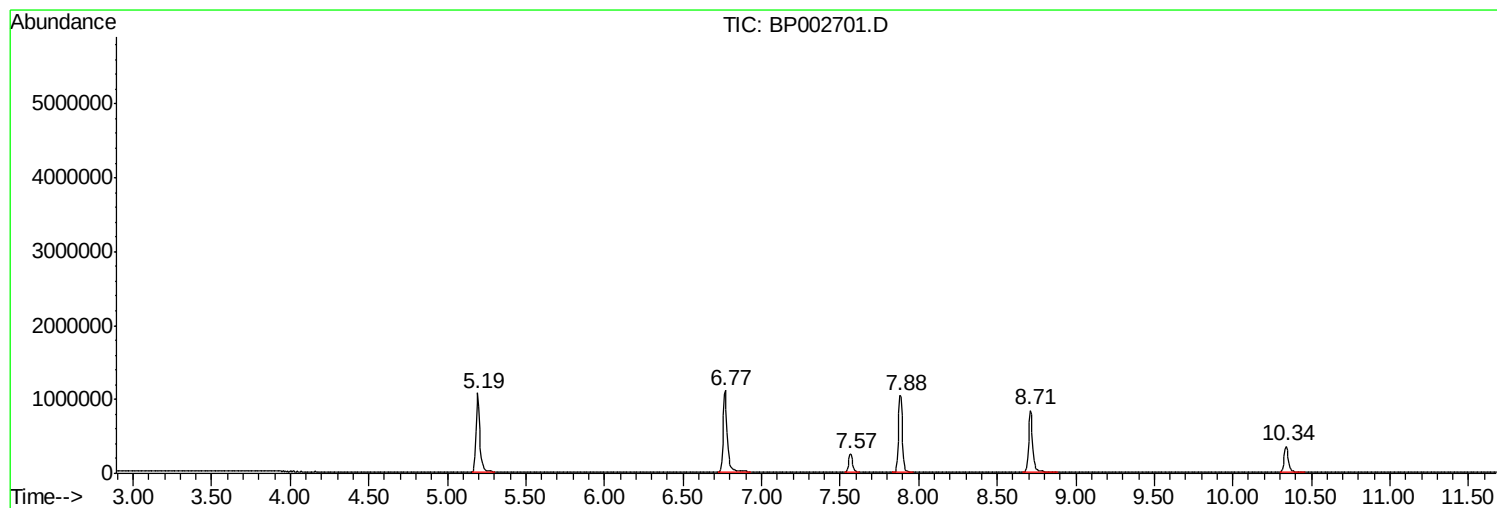

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP070920\
Data File : BP002701.D
Acq On : 09 Jul 2020 17:23
Operator : CG/JU
Sample : PB130037BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB130037BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP070920\
Data File : BP002701.D
Acq On : 09 Jul 2020 17:23
Operator : CG/JU
Sample : PB130037BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB130037BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc