


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP070920\
 Data File : BP002697.D
 Acq On : 09 Jul 2020 14:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 29 16:51:57 2020

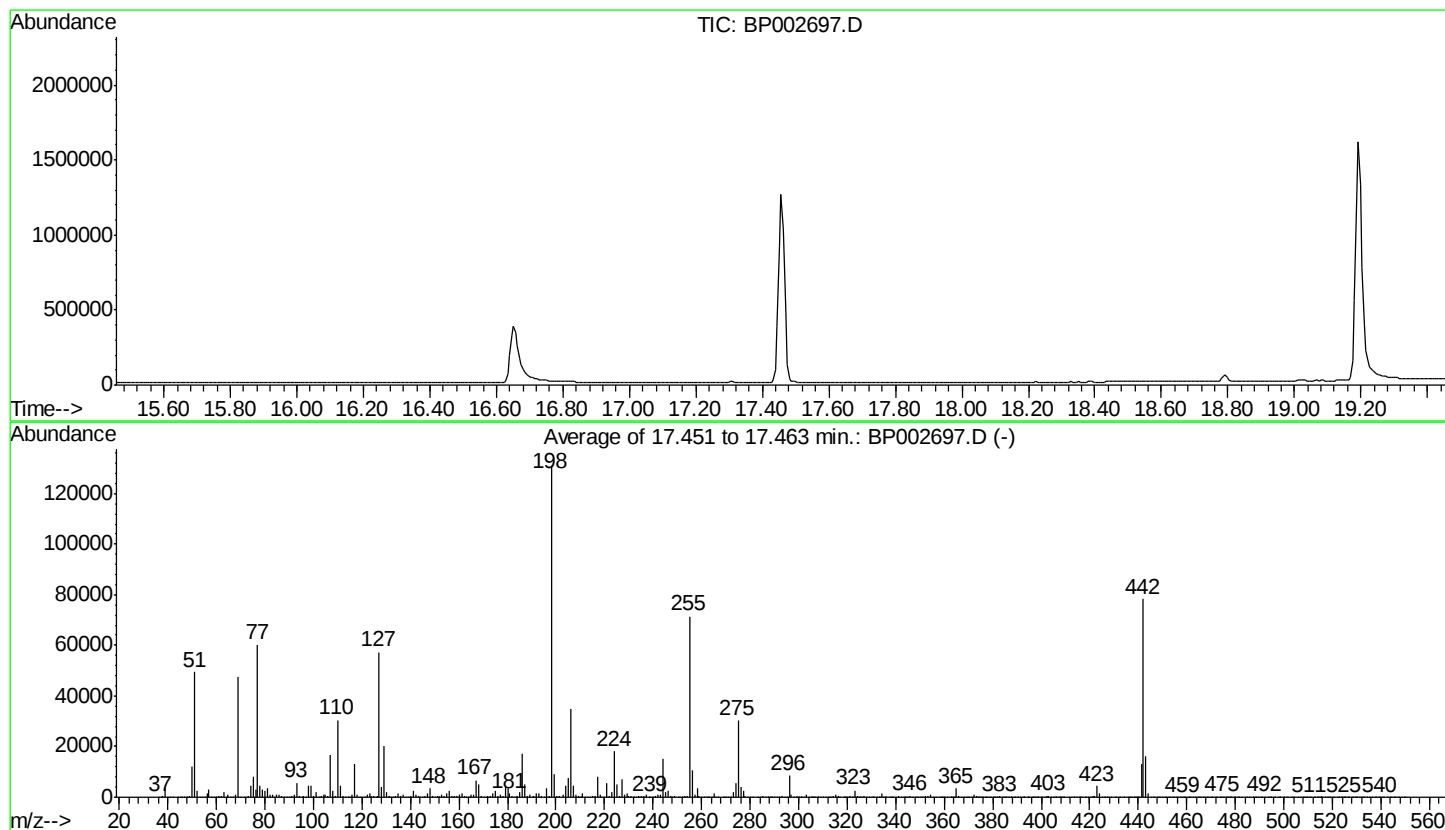

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.8	49543	PASS
68	69	0.00	2	1.7	788	PASS
69	198	0.00	100	36.2	47370	PASS
70	69	0.00	2	0.5	249	PASS
127	198	10	80	43.7	57197	PASS
197	198	0.00	2	0.3	348	PASS
198	198	100	100	100.0	131029	PASS
199	198	5	9	6.9	9087	PASS
275	198	10	60	23.1	30268	PASS
365	198	1	100	2.6	3431	PASS
441	198	0.01	100	9.9	12970	PASS
442	198	50	100	59.8	78317	PASS
443	442	15	24	20.6	16107	PASS