
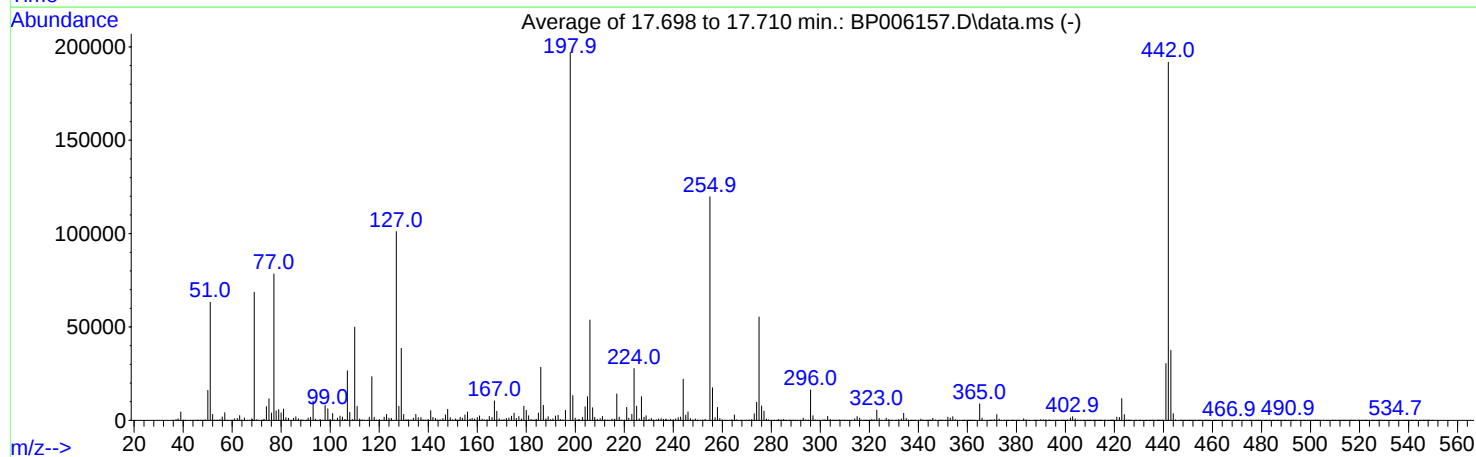


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070921\
 Data File : BP006157.D
 Acq On : 09 Jul 2021 12:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 07 16:08:13 2021

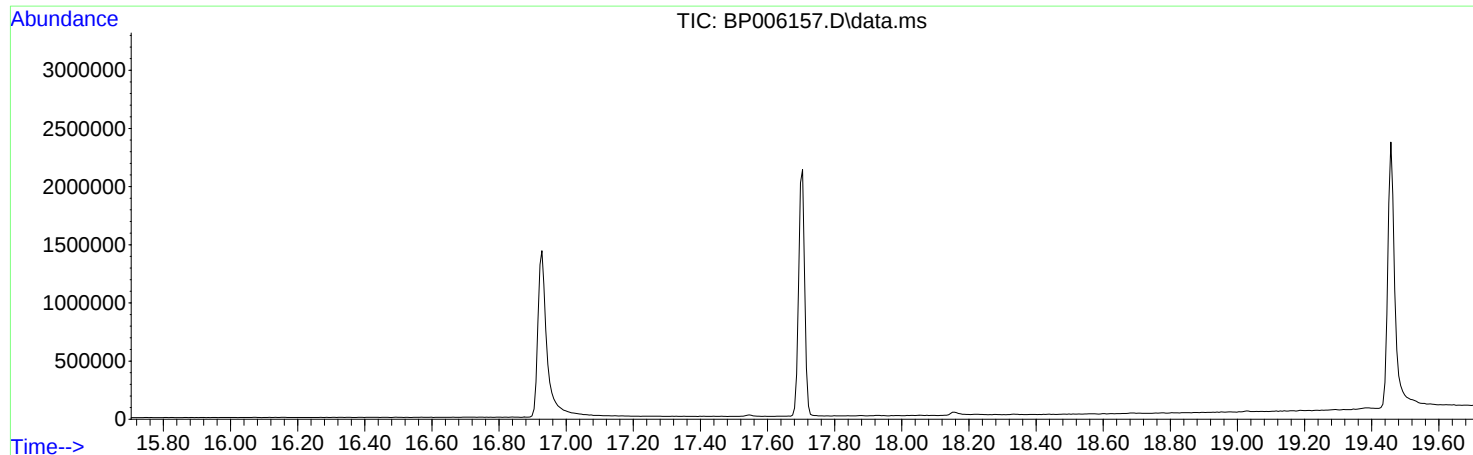




AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.1	63209	PASS
68	69	0.00	2	1.2	848	PASS
69	198	0.00	100	34.8	68625	PASS
70	69	0.00	2	0.5	367	PASS
127	198	10	80	51.3	101065	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	196989	PASS
199	198	5	9	6.7	13263	PASS
275	198	10	60	28.1	55361	PASS
365	198	1	100	4.5	8866	PASS
441	198	0.01	100	15.4	30404	PASS
442	442	100	100	100.0	191723	PASS
443	442	15	24	19.5	37410	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070921\
Data File : BP006157.D
Acq On : 09 Jul 2021 12:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 09 13:46:38 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 07 16:08:13 2021
Response via : Initial Calibration

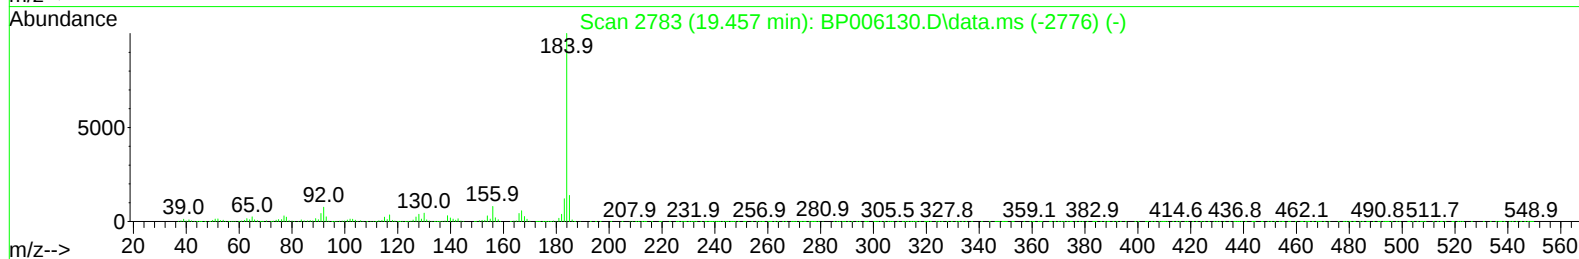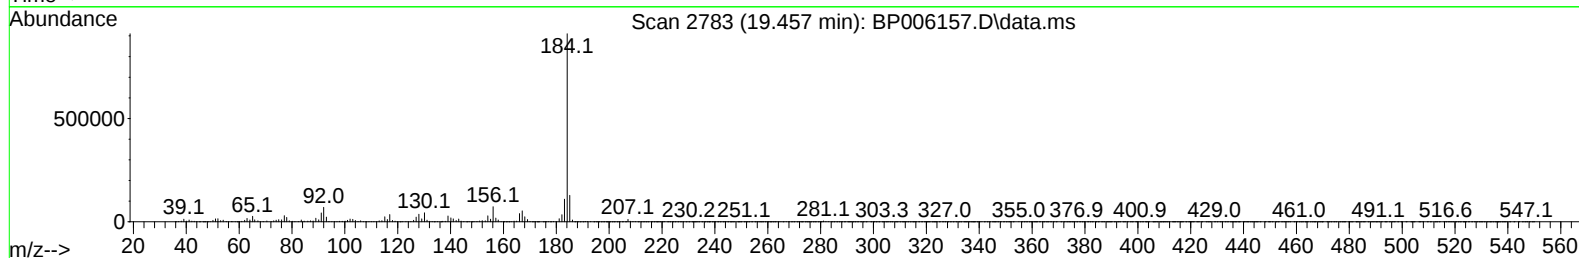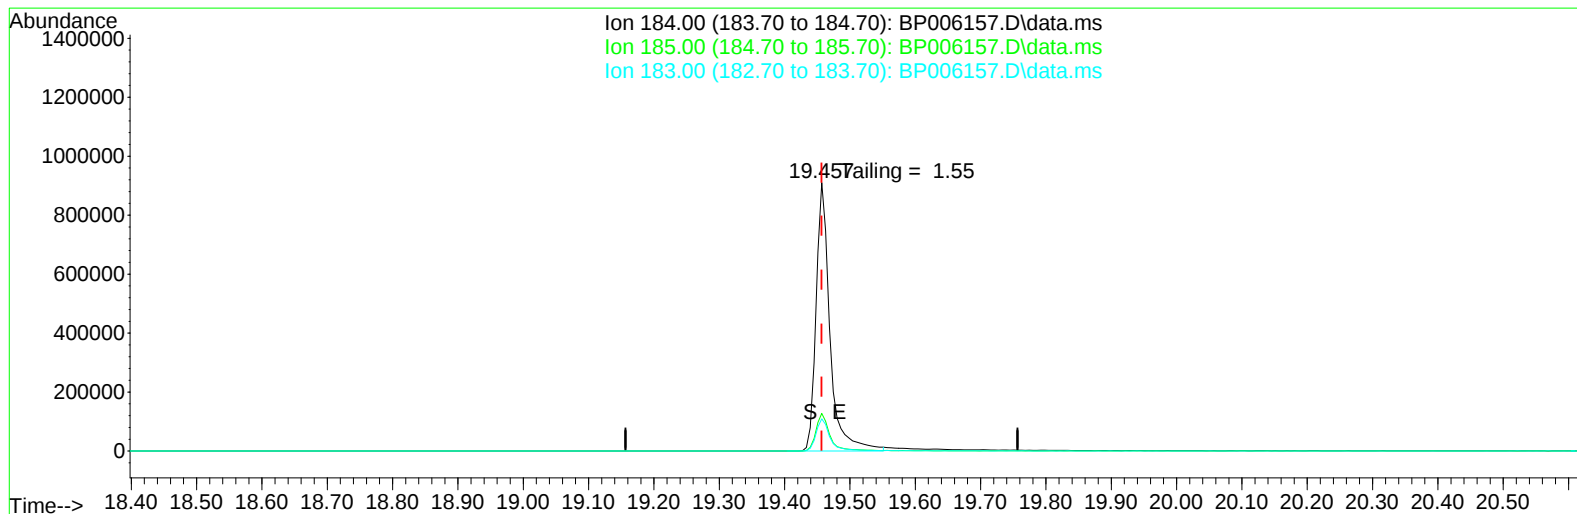

TIC: BP006157.D\data.ms

(77) Benzidine

19.457min (+ 0.000) 37286.74 ng




response 1383163

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.02
183.00	11.90	12.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070921\
 Data File : BP006157.D
 Acq On : 09 Jul 2021 12:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jul 09 13:46:38 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 07 16:08:13 2021
 Response via : Initial Calibration

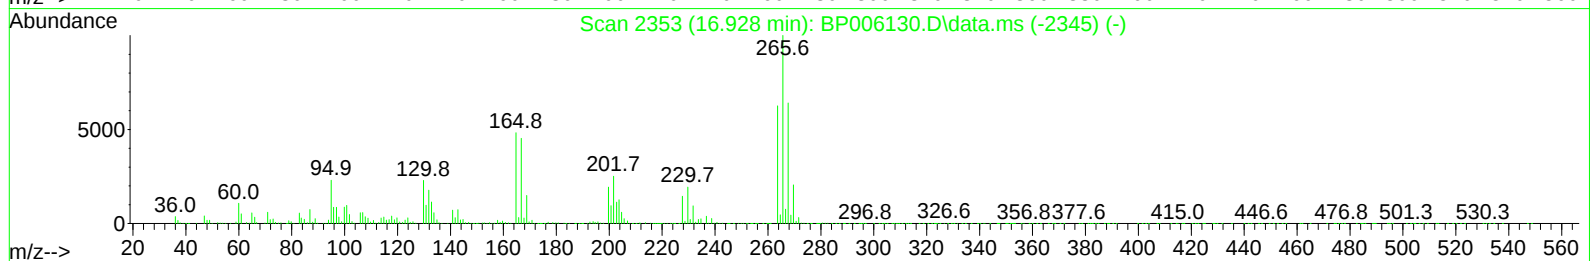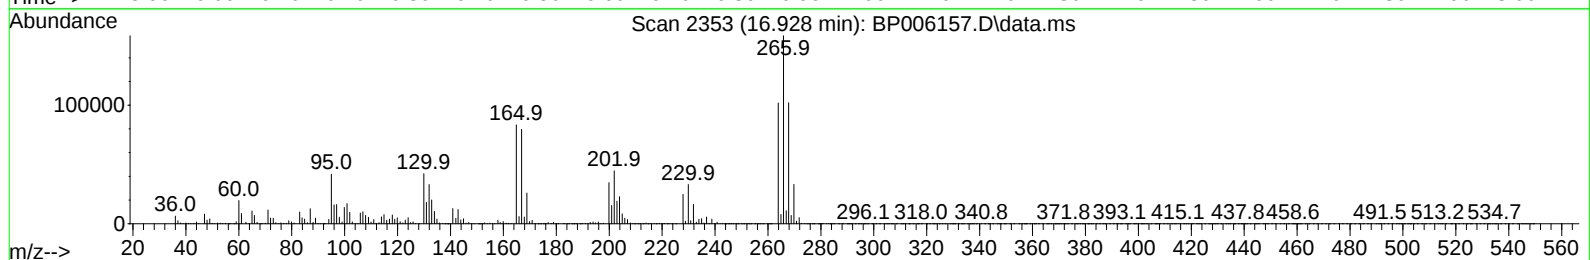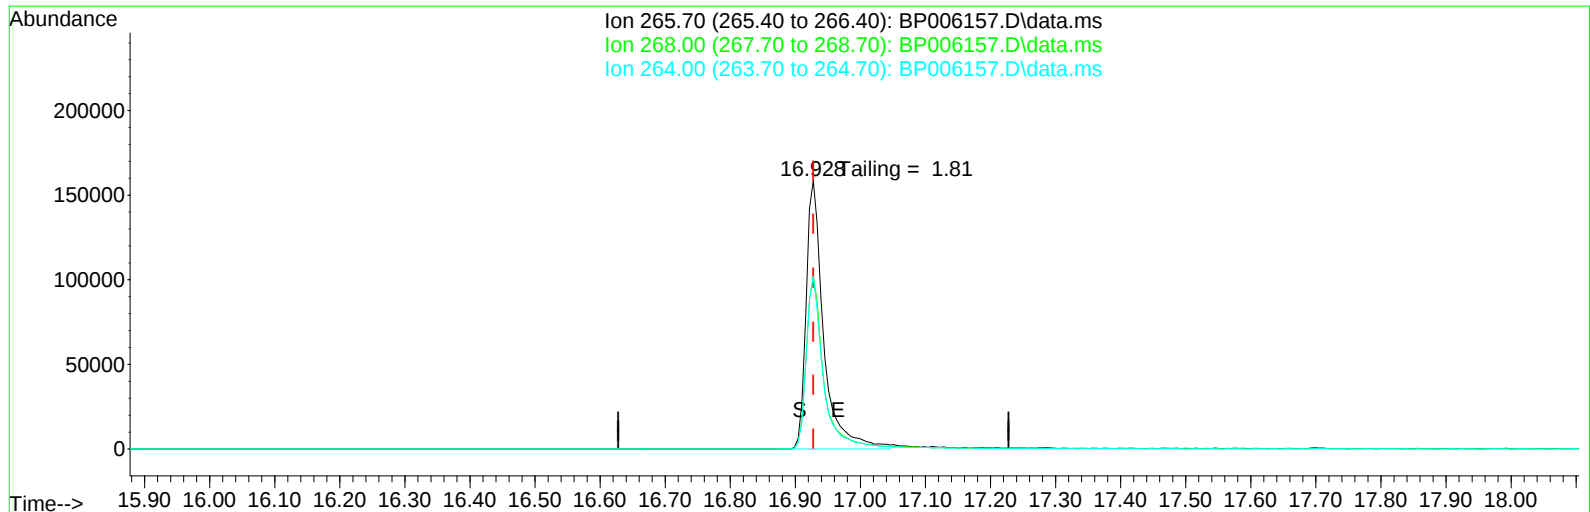

TIC: BP006157.D\data.ms

(70) Pentachlorophenol (C)

16.928min (+ 0.000) 136280.40 ng

response 304702

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.32
264.00	62.90	64.23
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/9/2021	BNA_P	<u>BP006157.D</u>
Compound Name	Response	Retention Time
DDT	670506	20.65
DDD	2194	20.22
DDE	2175	19.72
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4369	674875	0.65