
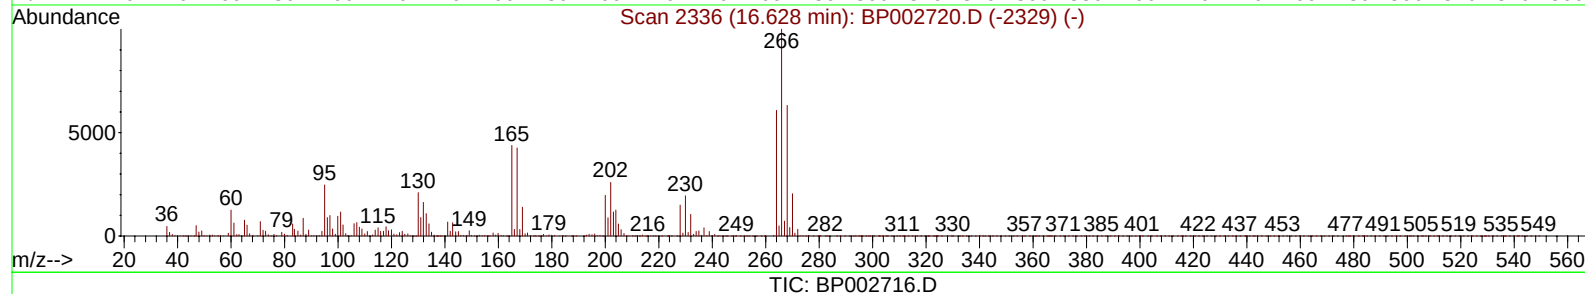
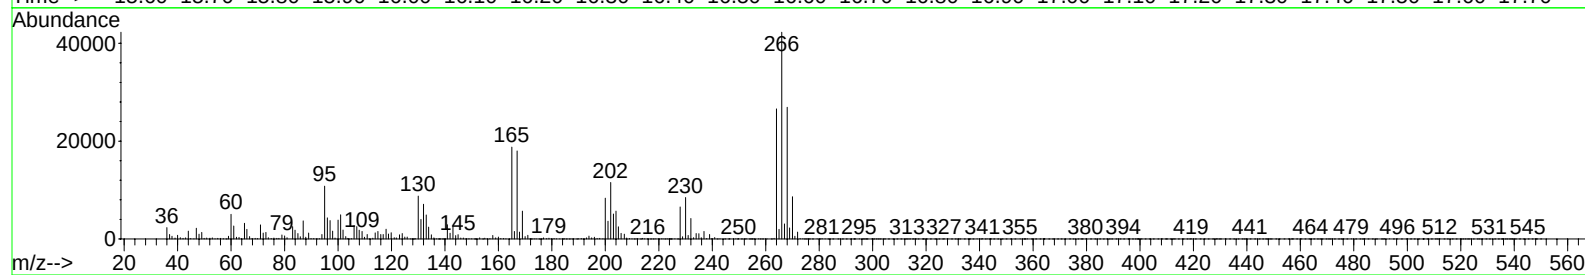


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP071020\
Data File : BP002716.D
Acq On : 10 Jul 2020 11:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 10 17:53:05 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP071020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 10 16:36:06 2020
Response via : Initial Calibration

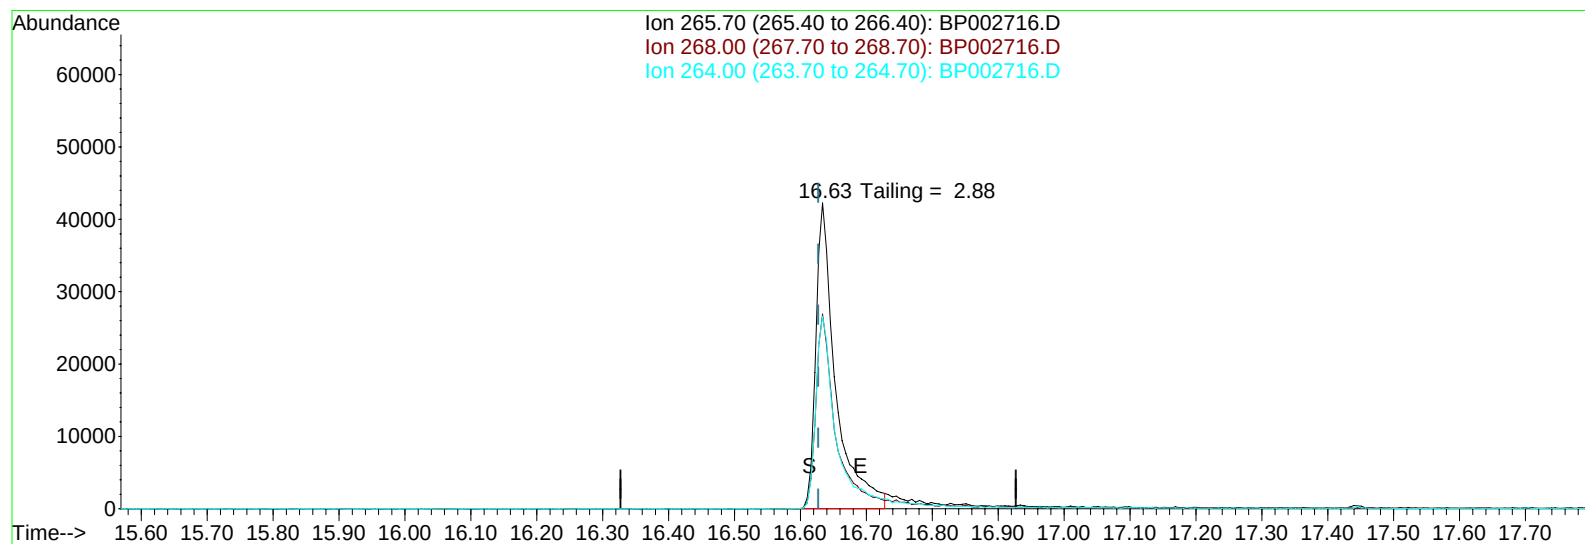

(70) Pentachlorophenol (C)




16.634min (+0.007) 346819.11ng

response 93392

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	63.67
264.00	60.70	62.93
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP071020\
 Data File : BP002716.D
 Acq On : 10 Jul 2020 11:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 10 17:53:05 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP071020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 10 16:36:06 2020
 Response via : Initial Calibration

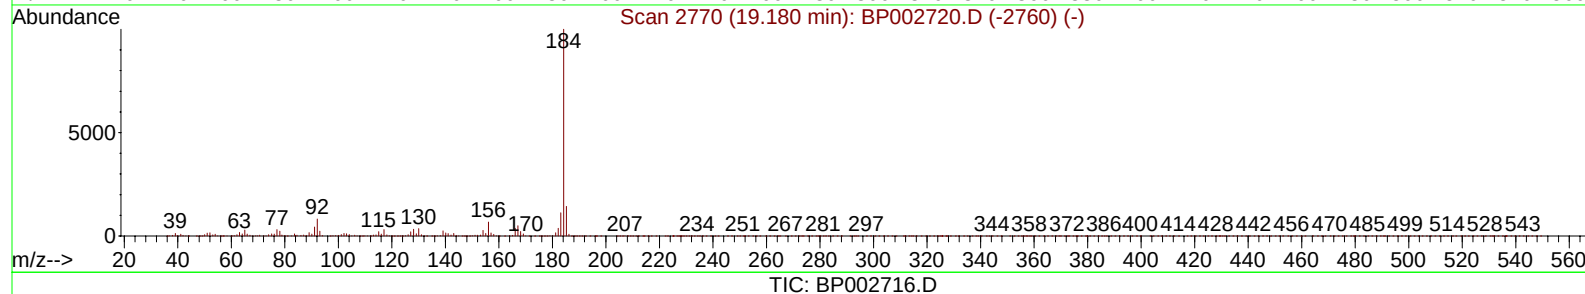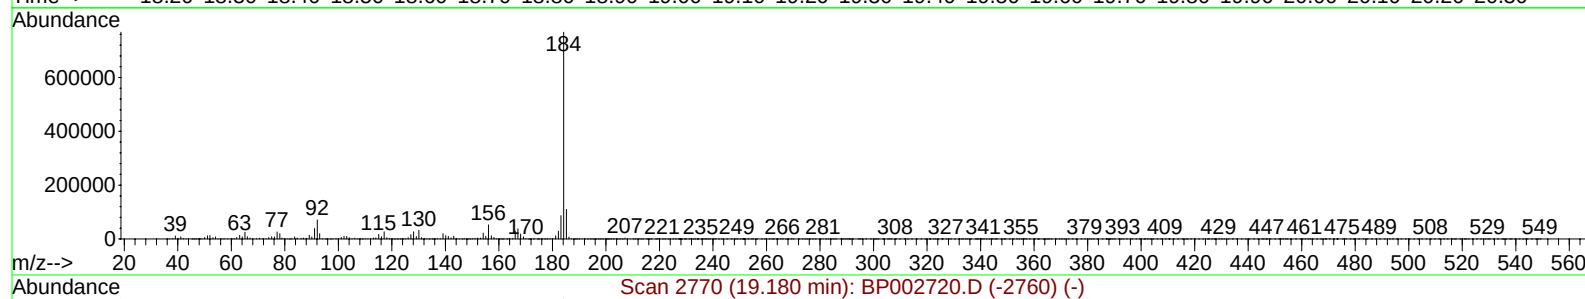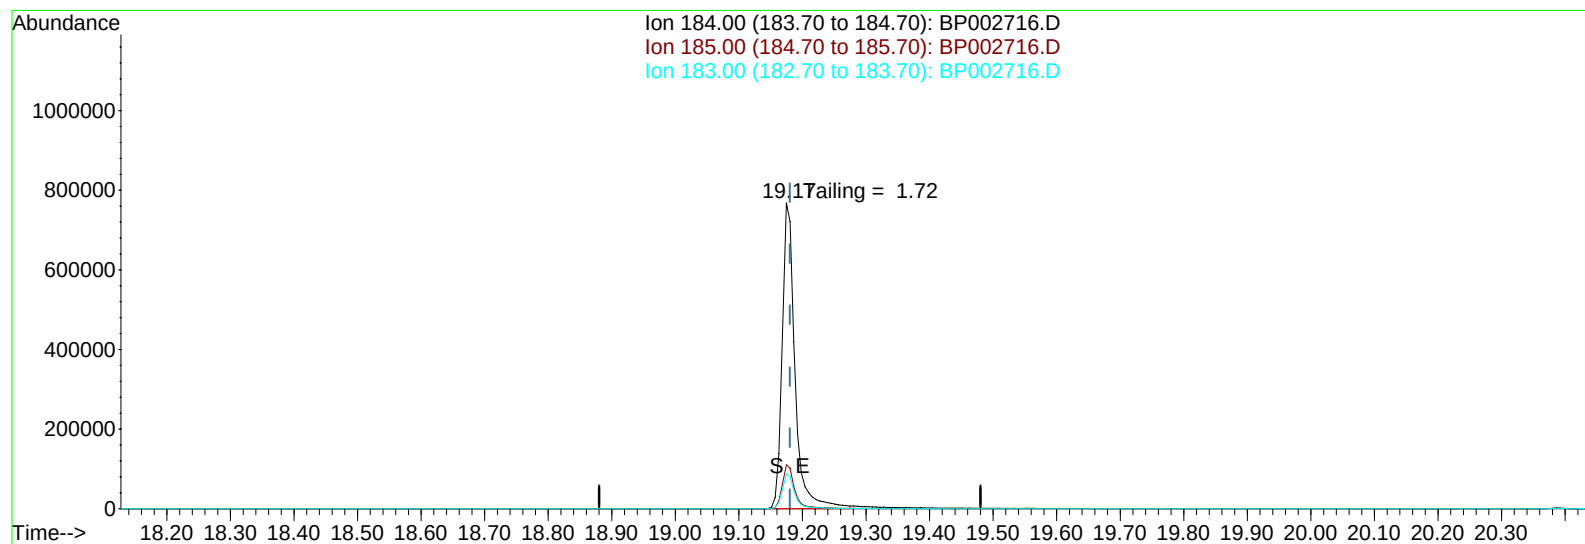

TIC: BP002716.D

(77) Benzidine

19.175min (-0.006) 3736386.24ng

response 1111362

Ion	Exp%	Act%
184.00	100	100
185.00	14.30	14.36
183.00	11.20	11.34
0.00	0.00	0.00