


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071020\
 Data File : BP002716.D
 Acq On : 10 Jul 2020 11:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP071020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 10 18:21:37 2020

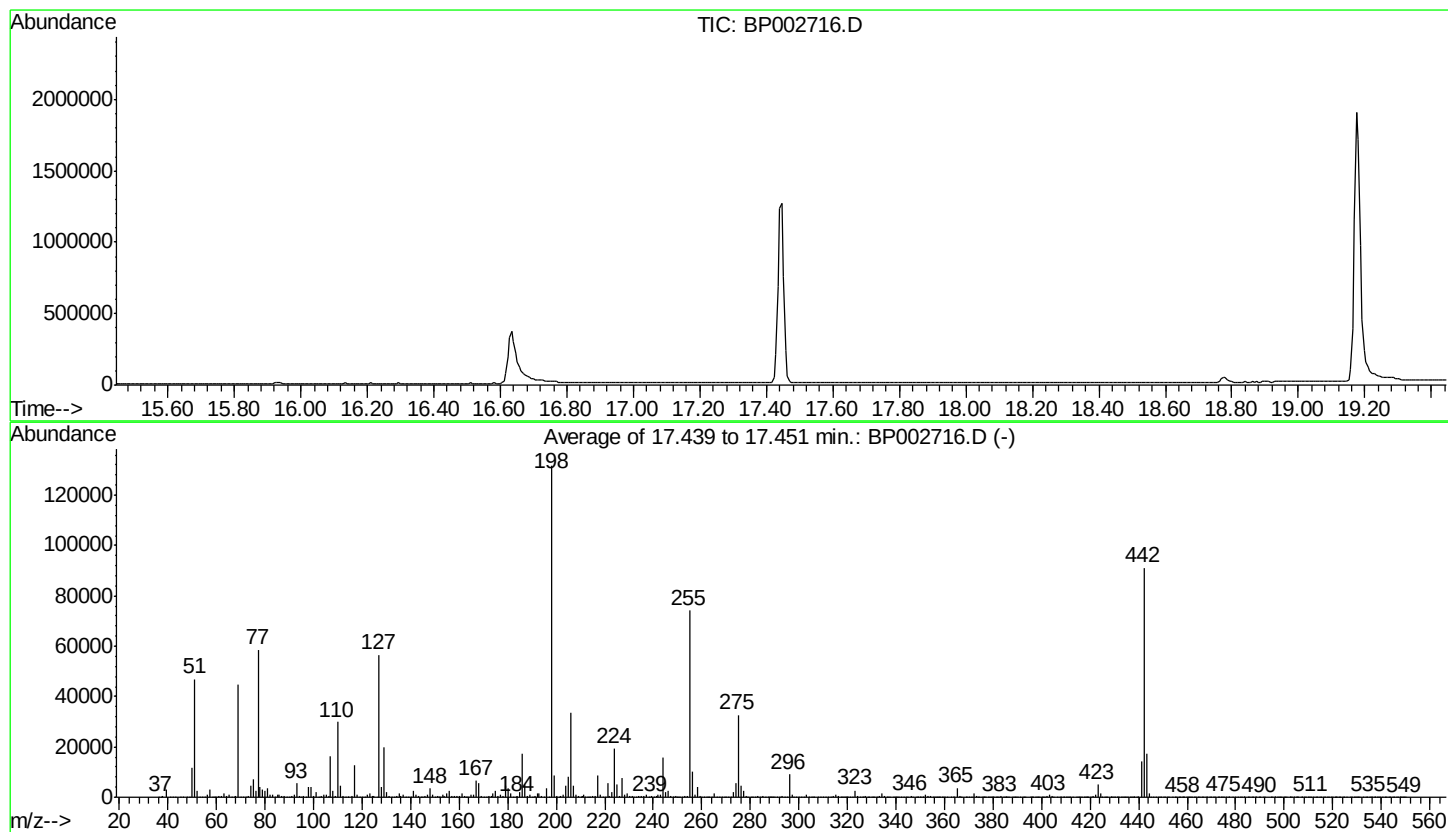

AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.6	46906	PASS
68	69	0.00	2	1.6	700	PASS
69	198	0.00	100	34.0	44761	PASS
70	69	0.00	2	0.5	211	PASS
127	198	10	80	43.0	56679	PASS
197	198	0.00	2	0.1	111	PASS
198	198	100	100	100.0	131754	PASS
199	198	5	9	6.5	8560	PASS
275	198	10	60	24.8	32617	PASS
365	198	1	100	2.8	3637	PASS
441	198	0.01	100	10.7	14139	PASS
442	198	50	100	69.3	91247	PASS
443	442	15	24	18.8	17113	PASS