
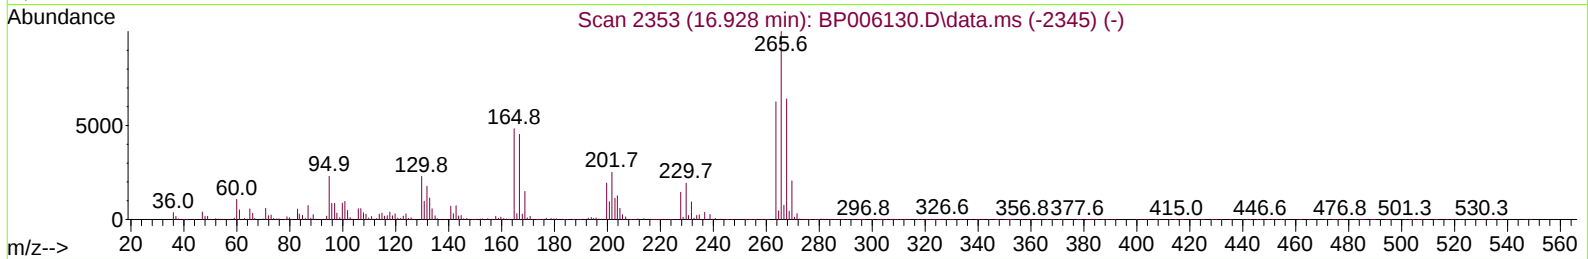
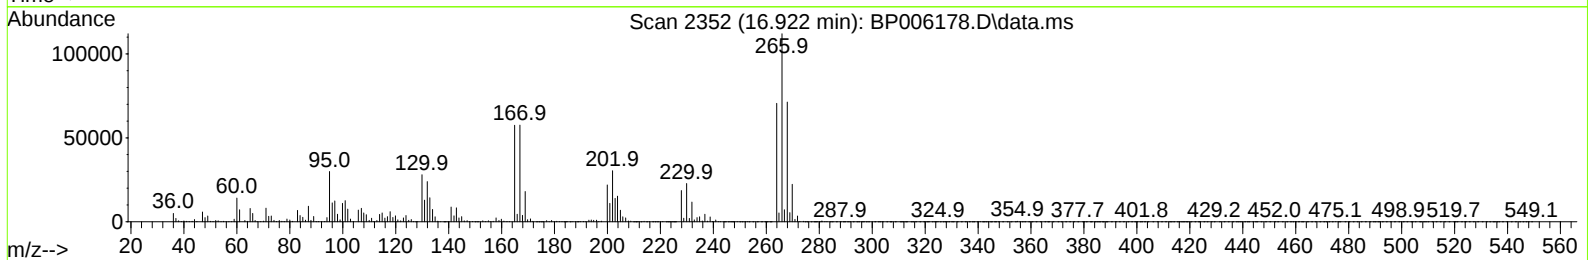


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071021\
 Data File : BP006178.D
 Acq On : 10 Jul 2021 14:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 11 06:04:01 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 07 16:08:13 2021
 Response via : Initial Calibration

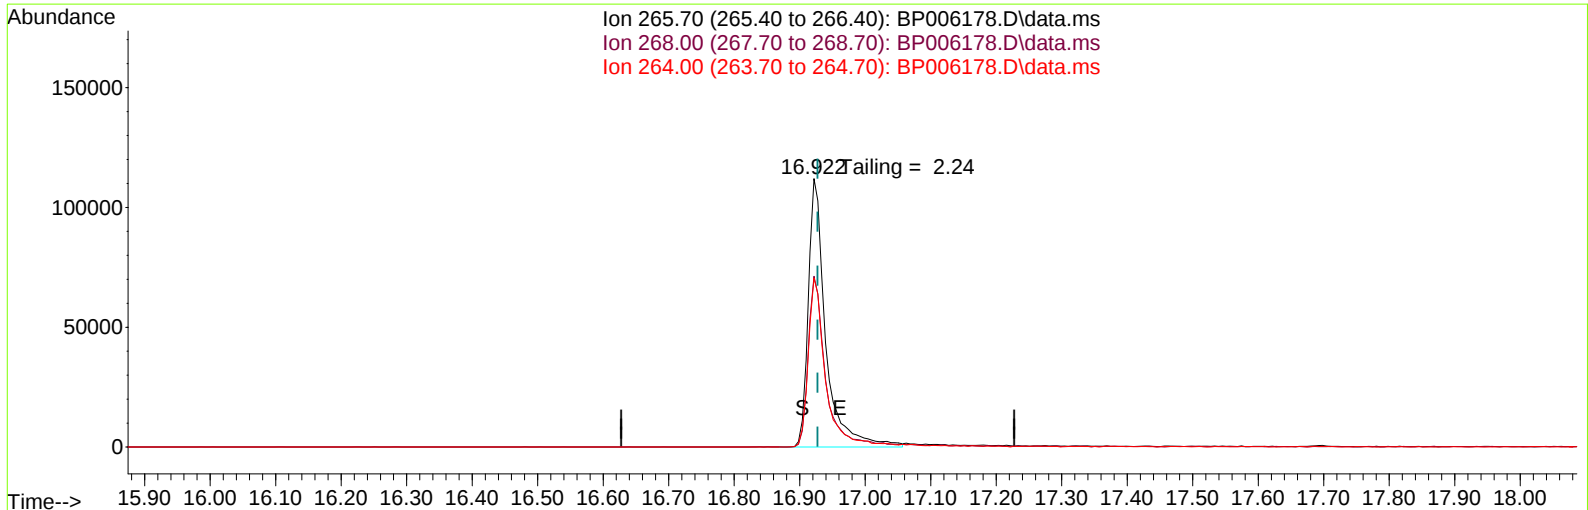

TIC: BP006178.D\data.ms

(70) Pentachlorophenol (C)




16.922min (-0.006) 3537674.55 ng

response 210161

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.64
264.00	62.90	62.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071021\
 Data File : BP006178.D
 Acq On : 10 Jul 2021 14:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 11 06:04:01 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 07 16:08:13 2021
 Response via : Initial Calibration

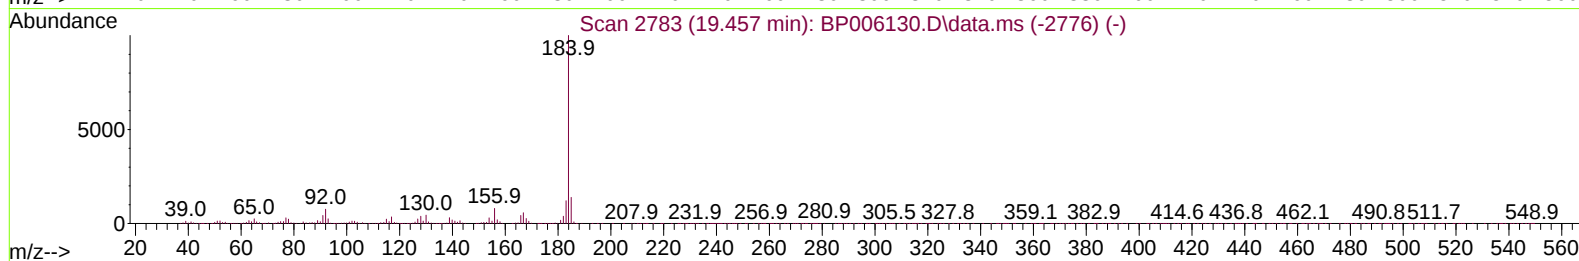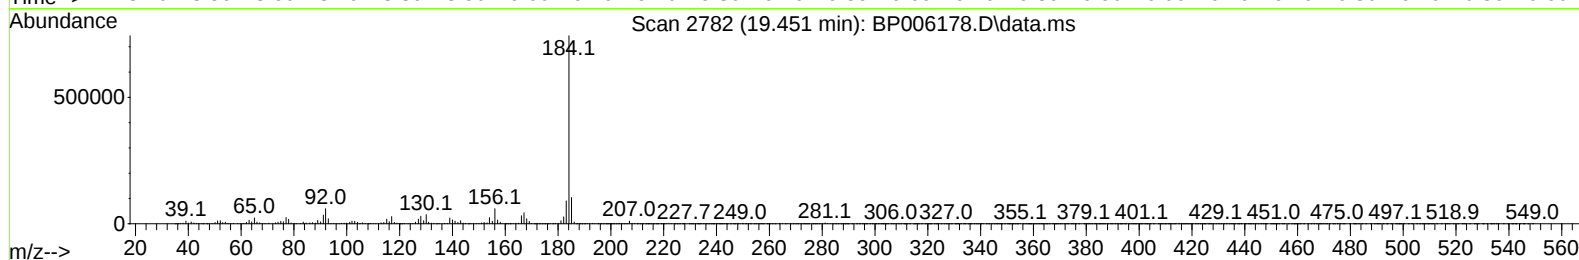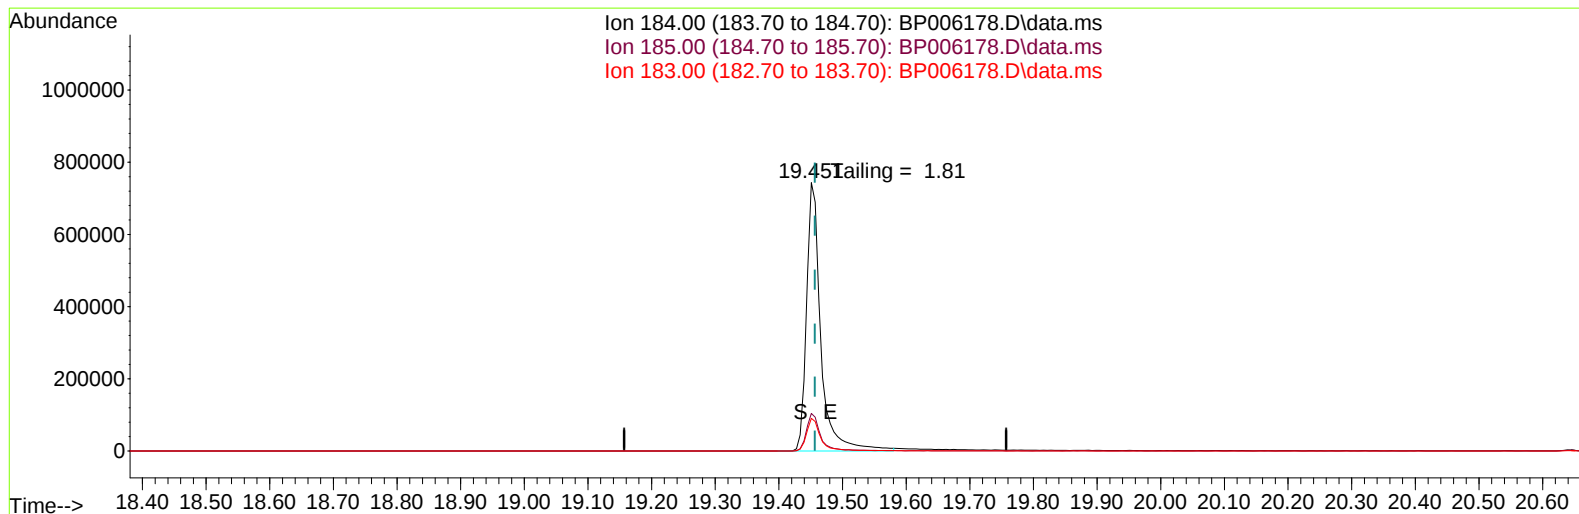

TIC: BP006178.D\data.ms

(77) Benzidine**19.451min (-0.006) 352066.41 ng****response 1190121**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.00
183.00	11.90	12.17
0.00	0.00	0.00