

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071021\
 Data File : BP006181.D
 Acq On : 10 Jul 2021 16:02
 Operator : CG/JU
 Sample : M2969-13
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SB07

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006181.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.975	316	321	330	rVB	220502	326803	5.01%	0.768%
2	5.446	393	401	417	rBV	966615	1596017	24.46%	3.752%
3	7.057	668	675	698	rBV	2058833	3700238	56.70%	8.699%
4	7.869	804	813	828	rBV	685403	1159460	17.77%	2.726%
5	9.040	1005	1012	1032	rBV	1397305	2466703	37.80%	5.799%
6	10.469	1249	1255	1272	rBV2	92840	246481	3.78%	0.579%
7	10.669	1278	1289	1297	rBV	903205	1573118	24.11%	3.698%
8	13.134	1701	1708	1718	rBV	3646512	5494019	84.19%	12.917%
9	13.328	1737	1741	1748	rVB2	47816	80391	1.23%	0.189%
10	13.834	1822	1827	1831	rBV2	62238	112911	1.73%	0.265%
11	13.981	1849	1852	1856	rVB	53837	69978	1.07%	0.165%
12	14.398	1919	1923	1928	rBV2	121290	171930	2.63%	0.404%
13	14.504	1932	1941	1947	rVV	1309669	2035945	31.20%	4.787%
14	14.569	1949	1952	1960	rVB	80542	144400	2.21%	0.339%
15	14.728	1974	1979	1985	rVB6	36730	84619	1.30%	0.199%
16	14.904	2005	2009	2019	rBV3	86104	170686	2.62%	0.401%
17	15.128	2043	2047	2053	rBV2	44973	85584	1.31%	0.201%
18	15.292	2070	2075	2077	rBV5	51383	88548	1.36%	0.208%
19	15.328	2077	2081	2083	rBV	160224	224168	3.44%	0.527%
20	15.551	2115	2119	2123	rBV3	55136	87600	1.34%	0.206%
21	15.757	2151	2154	2160	rVB3	80041	119423	1.83%	0.281%
22	16.004	2192	2196	2202	rVB	408340	569334	8.72%	1.339%
23	16.216	2227	2232	2233	rBV	225080	265993	4.08%	0.625%
24	17.010	2363	2367	2372	rVV2	235720	292106	4.48%	0.687%
25	17.063	2372	2376	2385	rVB2	177139	343306	5.26%	0.807%
26	17.257	2404	2409	2413	rBV	1467686	2116679	32.44%	4.976%
27	17.298	2413	2416	2422	rVB	812252	1169869	17.93%	2.750%
28	17.392	2428	2432	2438	rVB	177164	247064	3.79%	0.581%
29	17.675	2476	2480	2484	rVB2	110313	157228	2.41%	0.370%
30	17.751	2489	2493	2497	rBV	299089	353509	5.42%	0.831%
31	17.922	2518	2522	2526	rBV2	149980	186510	2.86%	0.438%
32	17.969	2527	2530	2536	rVB4	102806	155599	2.38%	0.366%
33	18.145	2554	2560	2564	rBV2	947134	1420596	21.77%	3.340%
34	18.316	2585	2589	2592	rBV2	131300	199888	3.06%	0.470%
35	18.422	2603	2607	2612	rBV2	381755	526015	8.06%	1.237%
36	19.027	2705	2710	2712	rBV2	332480	511222	7.83%	1.202%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071021\
Data File : BP006181.D
Acq On : 10 Jul 2021 16:02
Operator : CG/JU
Sample : M2969-13
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SB07

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	19.269	2747	2751	2757	rVB	1277151	1718225	26.33%	4.040%
38	19.374	2766	2769	2774	rBV	463882	561659	8.61%	1.320%
39	19.592	2802	2806	2808	rBV2	439908	579166	8.88%	1.362%
40	19.622	2808	2811	2819	rVB	1109563	1720813	26.37%	4.046%
41	19.816	2839	2844	2849	rVB	5301364	6525583	100.00%	15.342%
42	20.104	2891	2893	2898	rVB	417700	447735	6.86%	1.053%
43	20.586	2973	2975	2979	rVB	348143	336513	5.16%	0.791%
44	21.345	3100	3104	3108	rVB2	1600213	2090418	32.03%	4.915%


Sum of corrected areas: 42534052

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071021\
Data File : BP006181.D
Acq On : 10 Jul 2021 16:02
Operator : CG/JU
Sample : M2969-13
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampled :
SB07

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

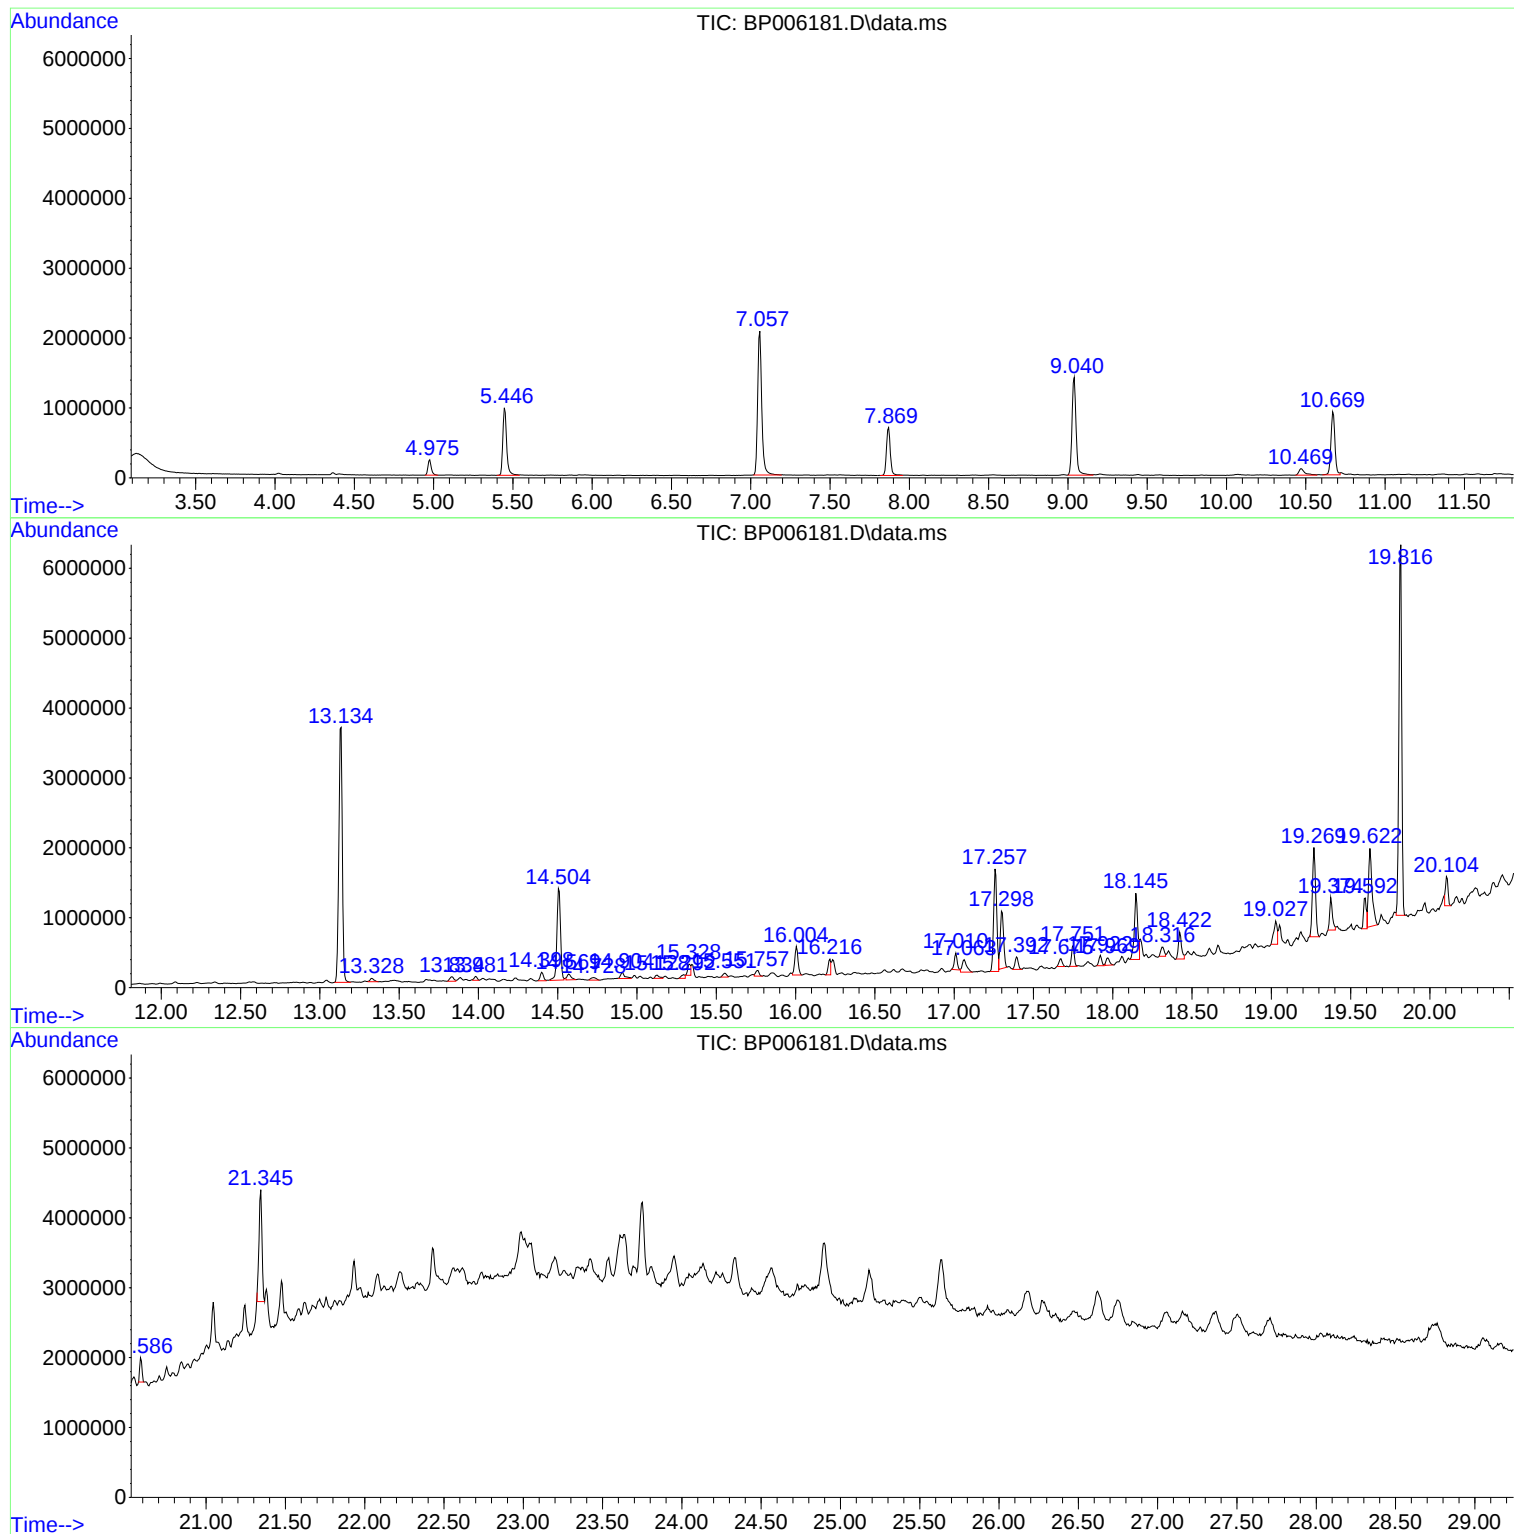

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071021\
Data File : BP006181.D
Acq On : 10 Jul 2021 16:02
Operator : CG/JU
Sample : M2969-13
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SB07

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071021\
Data File : BP006181.D
Acq On : 10 Jul 2021 16:02
Operator : CG/JU
Sample : M2969-13
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SB07

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------