
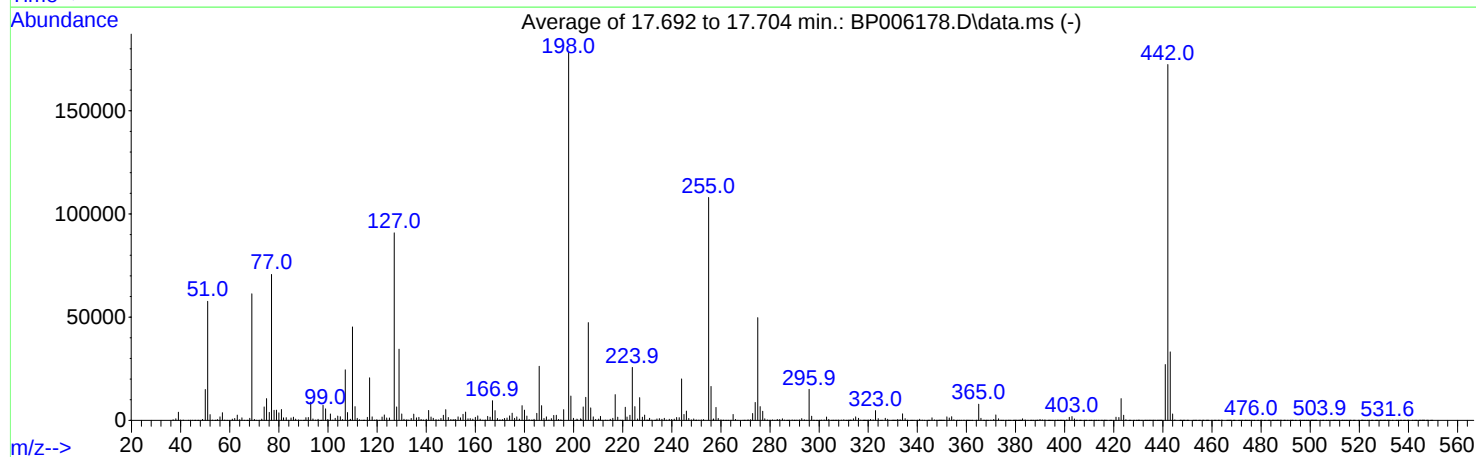


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071021\
 Data File : BP006178.D
 Acq On : 10 Jul 2021 14:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 07 16:08:13 2021

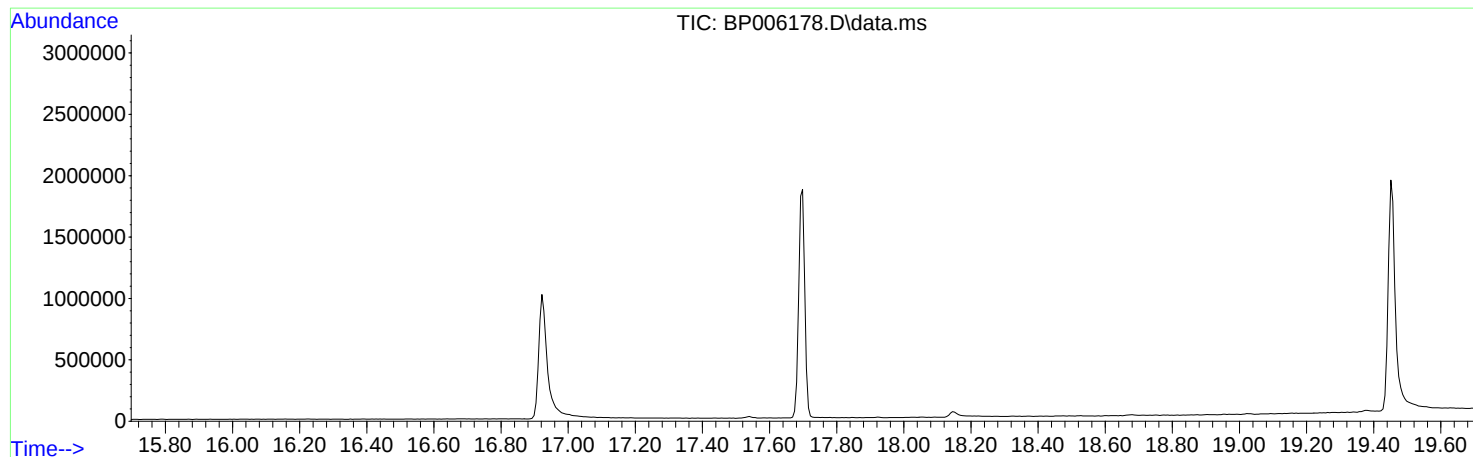




AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.4	57704	PASS
68	69	0.00	2	1.6	1008	PASS
69	198	0.00	100	34.4	61326	PASS
70	69	0.00	2	0.7	435	PASS
127	198	10	80	51.0	90843	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	178213	PASS
199	198	5	9	6.6	11758	PASS
275	198	10	60	27.9	49752	PASS
365	198	1	100	4.4	7857	PASS
441	198	0.01	100	15.2	27043	PASS
442	442	100	100	100.0	172395	PASS
443	442	15	24	19.3	33199	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071021\
 Data File : BP006178.D
 Acq On : 10 Jul 2021 14:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jul 11 06:04:01 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 07 16:08:13 2021
 Response via : Initial Calibration

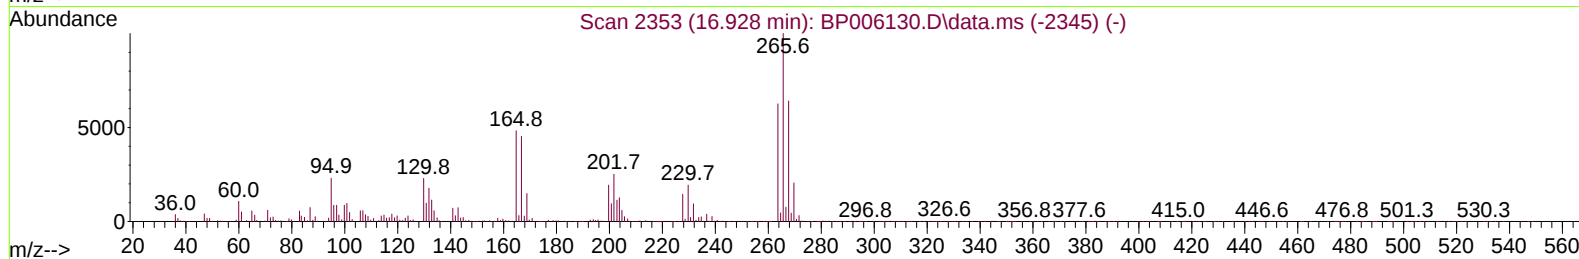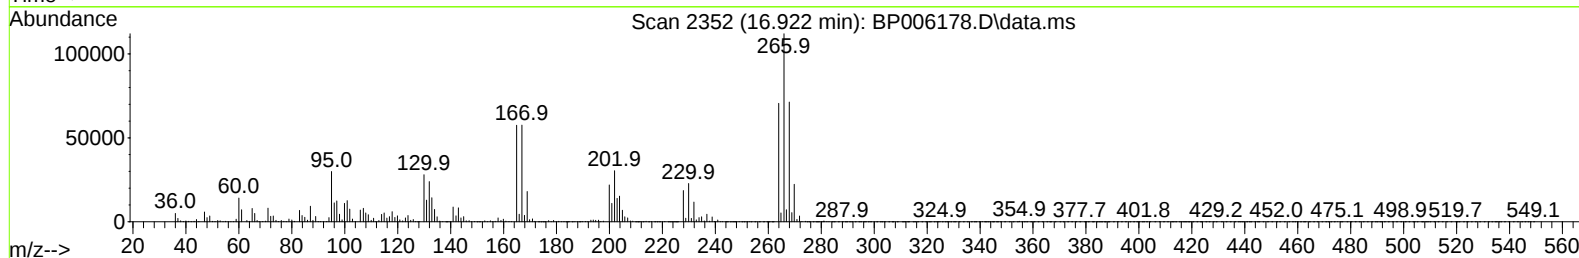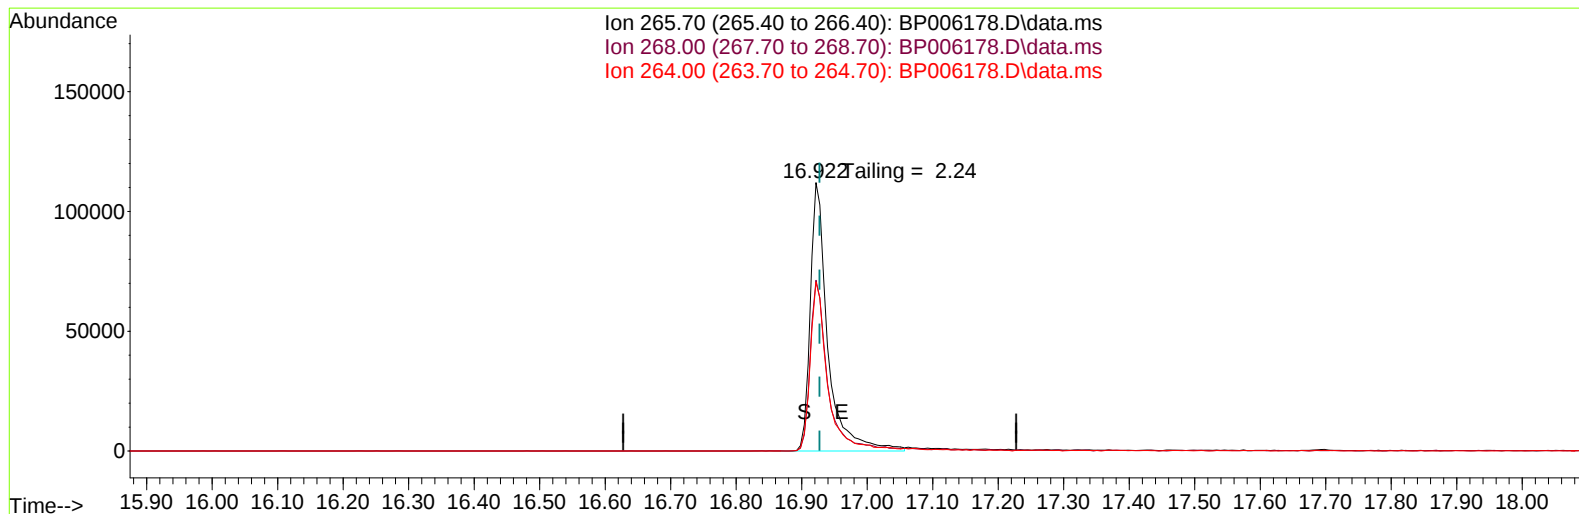

TIC: BP006178.D\data.ms

(70) Pentachlorophenol (C)

16.922min (-0.006) 3537674.55 ng




response 210161

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.64
264.00	62.90	62.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071021\
 Data File : BP006178.D
 Acq On : 10 Jul 2021 14:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jul 11 06:04:01 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 07 16:08:13 2021
 Response via : Initial Calibration

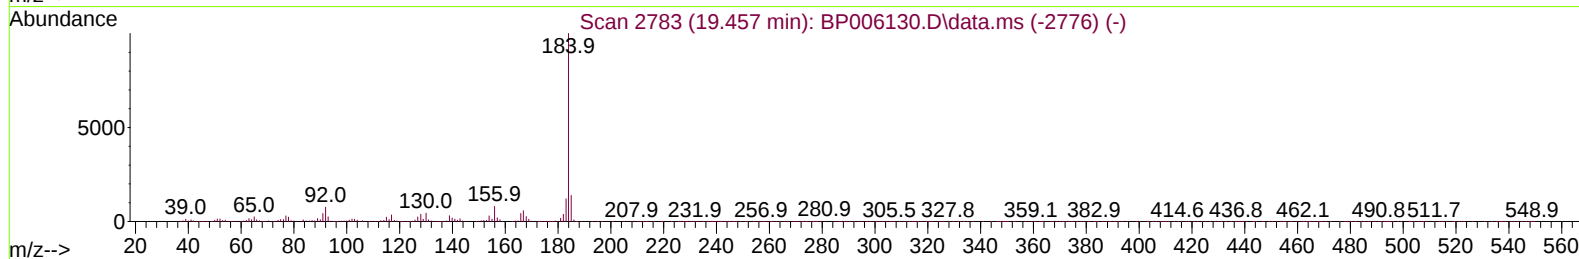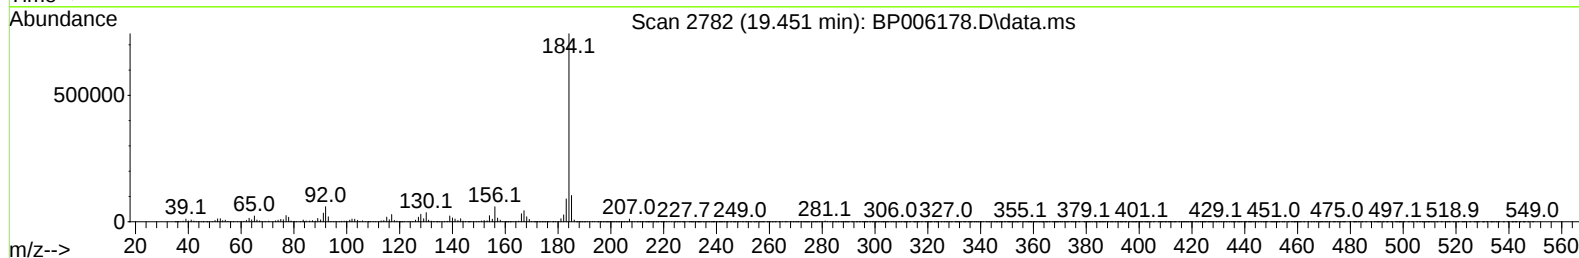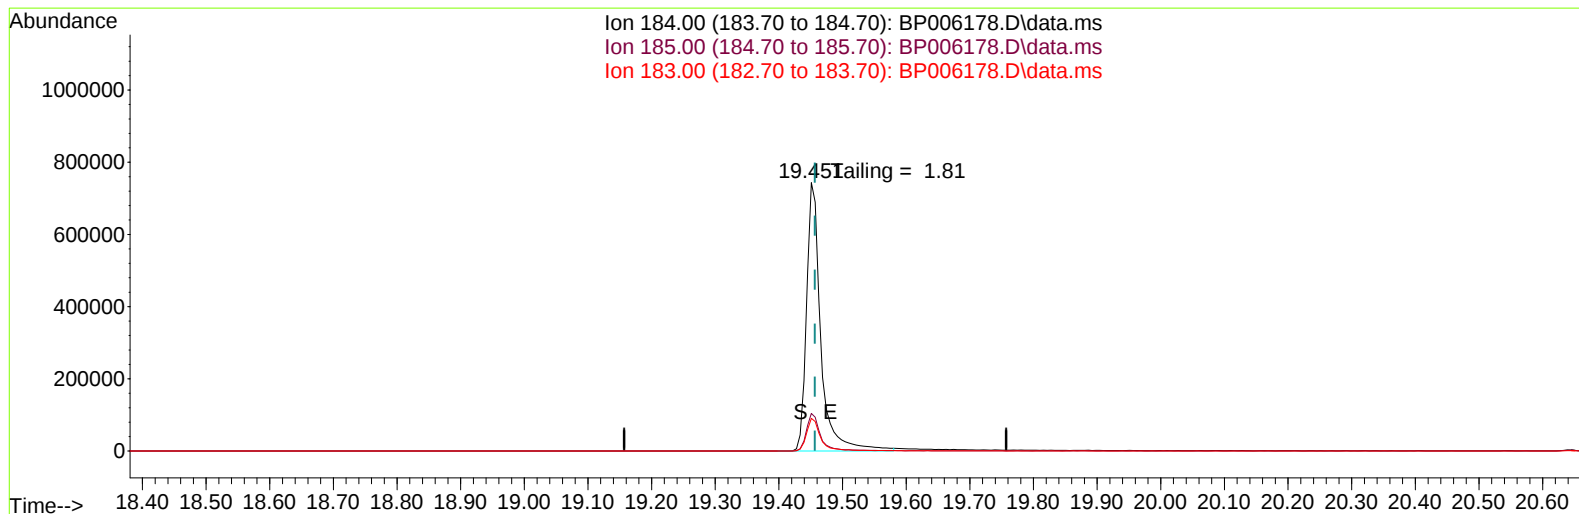

TIC: BP006178.D\data.ms

(77) Benzidine

19.451min (-0.006) 352066.41 ng

response 1190121

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.00
183.00	11.90	12.17
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/10/2021	BNA_P	<u>BP006178.D</u>
Compound Name	Response	Retention Time
DDT	688818	20.645
DDD	7912	20.222
DDE	1496	19.727
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9408	698226	1.35