

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071024\
 Data File : BP020887.D
 Acq On : 10 Jul 2024 19:36
 Operator : MA/JU
 Sample : PB161835BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK835

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020887.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	41	45	51	rVB	66533	78114	1.21%	0.121%
2	3.664	112	115	131	rBV	755074	1119572	17.29%	1.728%
3	3.975	164	168	173	rVB	11393	16152	0.25%	0.025%
4	6.916	661	668	685	rBV	920576	1555568	24.02%	2.401%
5	7.063	687	693	707	rVB	787066	1243060	19.20%	1.919%
6	7.269	720	728	739	rBV	1004327	1591898	24.59%	2.457%
7	7.722	797	805	816	rBV	865859	1341972	20.73%	2.072%
8	8.428	918	925	944	rBV	1218447	2017087	31.15%	3.114%
9	8.869	993	1000	1013	rBV	938972	1633529	25.23%	2.522%
10	9.581	1113	1121	1136	rBV	833926	1453456	22.45%	2.244%
11	10.122	1204	1213	1234	rBV	1111492	2150611	33.21%	3.320%
12	10.493	1266	1276	1285	rBV	1146890	2101016	32.45%	3.243%
13	10.640	1293	1301	1325	rBV	949091	1869331	28.87%	2.886%
14	11.322	1410	1417	1424	rBV	5015	14451	0.22%	0.022%
15	12.087	1541	1547	1557	rBV3	15937	38023	0.59%	0.059%
16	13.316	1752	1756	1767	rVB5	5097	9937	0.15%	0.015%
17	13.763	1825	1832	1845	rBV	2381342	3624663	55.98%	5.595%
18	14.045	1871	1880	1896	rBV2	2505338	4058339	62.68%	6.265%
19	14.357	1925	1933	1944	rBV	2005465	3142279	48.53%	4.851%
20	14.604	1968	1975	1985	rBV	747339	1447716	22.36%	2.235%
21	14.763	1998	2002	2006	rVB6	6011	8800	0.14%	0.014%
22	14.851	2014	2017	2022	rVB6	4616	6851	0.11%	0.011%
23	15.369	2098	2105	2122	rBV	3671880	5126674	79.18%	7.914%
24	15.510	2123	2129	2144	rVV	1252424	1855137	28.65%	2.864%
25	15.616	2144	2147	2154	rVB4	17659	30276	0.47%	0.047%
26	15.892	2190	2194	2199	rVB3	8359	12750	0.20%	0.020%
27	16.169	2237	2241	2248	rVB3	12852	19961	0.31%	0.031%
28	16.839	2351	2355	2360	rVB6	6583	9909	0.15%	0.015%
29	16.951	2370	2374	2382	rVB5	8168	14762	0.23%	0.023%
30	17.169	2404	2411	2421	rBV	2606570	3901817	60.26%	6.023%
31	17.269	2422	2428	2447	rVB2	3980346	5602032	86.52%	8.647%
32	17.869	2526	2530	2534	rBV7	10994	15239	0.24%	0.024%
33	18.098	2565	2569	2578	rBV9	21581	58012	0.90%	0.090%
34	19.198	2752	2756	2764	rBV2	49791	81038	1.25%	0.125%
35	19.275	2765	2769	2777	rBV	41452	66365	1.02%	0.102%
36	19.657	2828	2834	2841	rBV	4396217	6475070	100.00%	9.995%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071024\
Data File : BP020887.D
Acq On : 10 Jul 2024 19:36
Operator : MA/JU
Sample : PB161835BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK835

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Title : SVOA CALIBRATION

37	21.621	3162	3168	3179	rBV2	2005298	3539428	54.66%	5.464%
38	24.745	3690	3699	3712	rVB2	1786969	4630125	71.51%	7.147%
39	24.974	3731	3738	3750	rVB2	1108671	2821461	43.57%	4.355%




Sum of corrected areas: 64782481

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071024\
Data File : BP020887.D
Acq On : 10 Jul 2024 19:36
Operator : MA/JU
Sample : PB161835BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK835

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

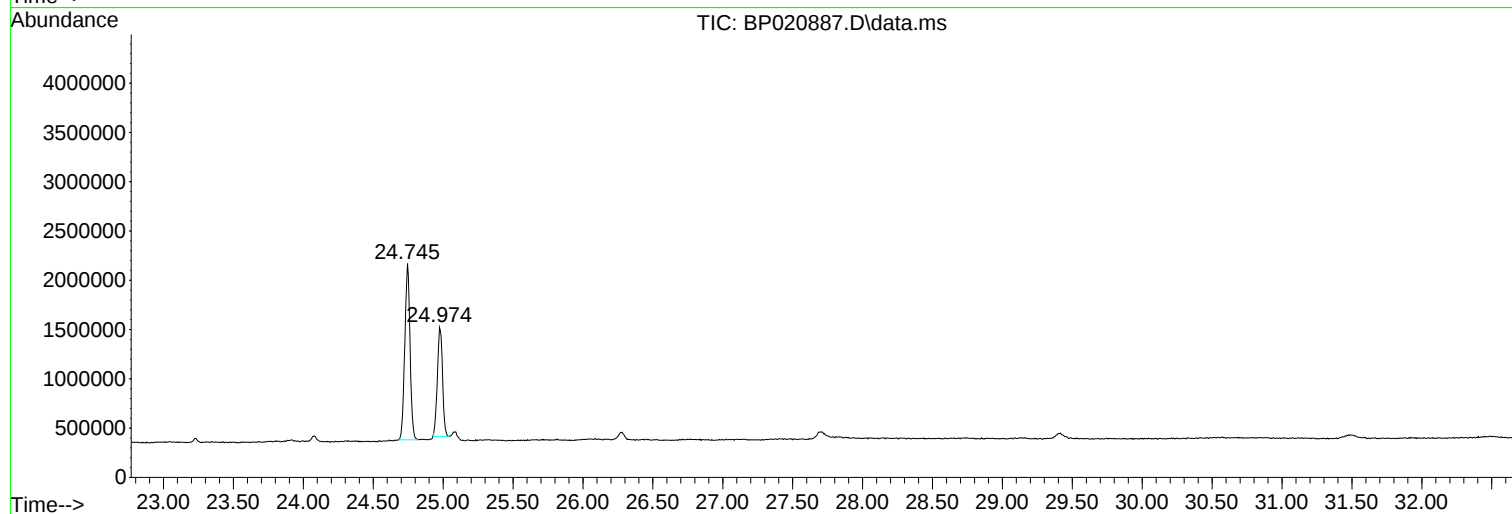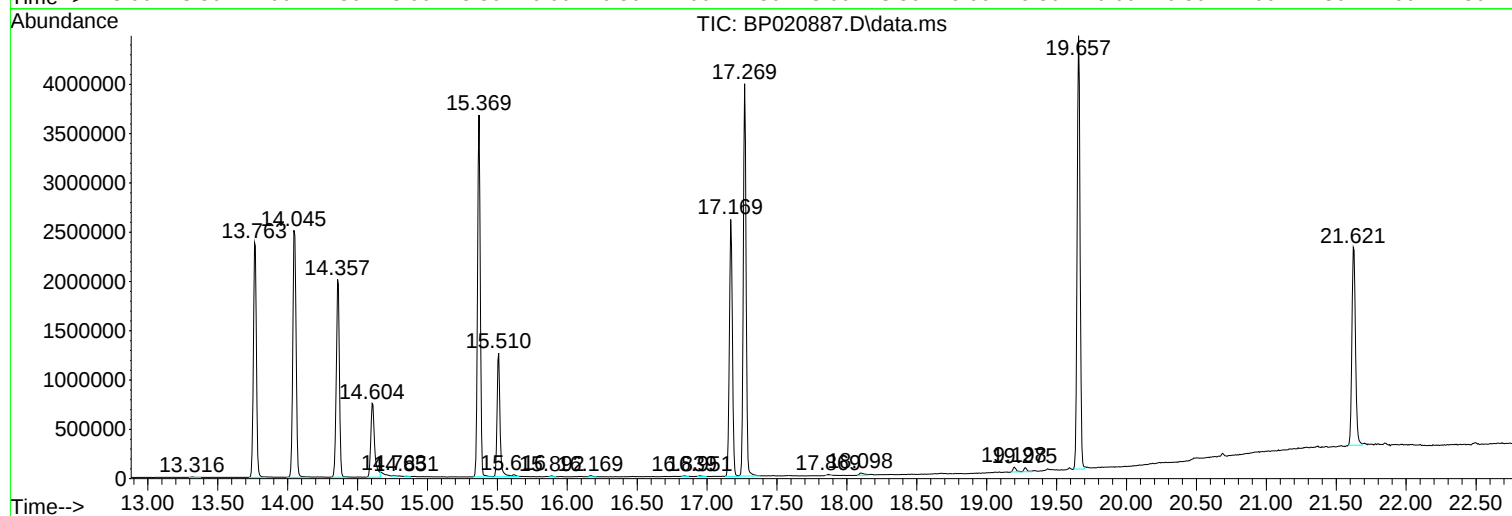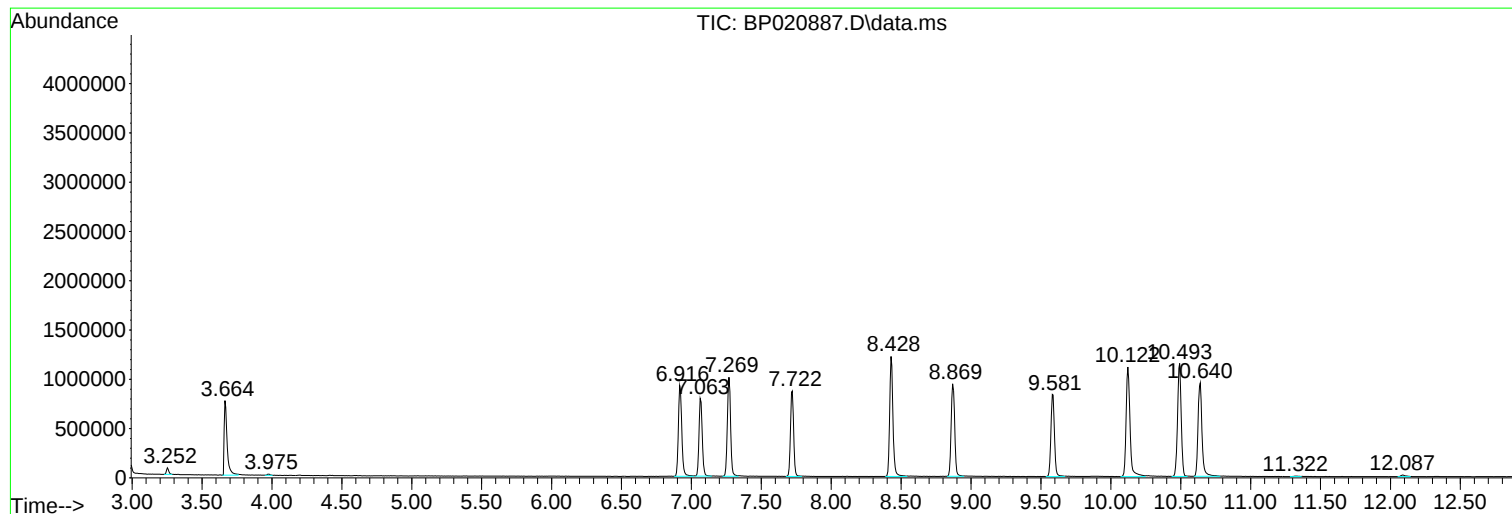

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071024\
Data File : BP020887.D
Acq On : 10 Jul 2024 19:36
Operator : MA/JU
Sample : PB161835BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK835

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071024\
Data File : BP020887.D
Acq On : 10 Jul 2024 19:36
Operator : MA/JU
Sample : PB161835BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK835

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc