

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071024\
 Data File : BP020888.D
 Acq On : 10 Jul 2024 20:20
 Operator : MA/JU
 Sample : PB161825BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK825

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020888.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	42	46	56	rVB	68350	92976	1.62%	0.146%
2	3.670	113	116	132	rBV	803294	1177086	20.49%	1.854%
3	3.981	166	169	173	rVB	13241	16934	0.29%	0.027%
4	4.199	204	206	213	rVB7	4907	5866	0.10%	0.009%
5	6.911	661	667	685	rBV	968826	1587259	27.63%	2.499%
6	7.064	687	693	707	rVB	791312	1281375	22.30%	2.018%
7	7.264	720	727	740	rBV	1018521	1615882	28.13%	2.544%
8	7.722	797	805	817	rBV	852275	1461235	25.43%	2.301%
9	8.428	918	925	943	rBV	1137973	2069468	36.02%	3.259%
10	8.875	992	1001	1011	rBV	940067	1685672	29.34%	2.654%
11	9.587	1114	1122	1135	rBV	834720	1489207	25.92%	2.345%
12	10.122	1203	1213	1235	rBV	1143314	2178613	37.92%	3.431%
13	10.493	1267	1276	1285	rBV	1389044	2220911	38.66%	3.497%
14	10.640	1293	1301	1322	rBV	860771	1822510	31.72%	2.870%
15	12.099	1542	1549	1557	rBV2	15867	34844	0.61%	0.055%
16	13.310	1750	1755	1758	rBV7	3724	5802	0.10%	0.009%
17	13.757	1824	1831	1847	rBV	2311442	3528987	61.43%	5.557%
18	14.051	1871	1881	1894	rBV	2675655	4033901	70.21%	6.352%
19	14.357	1926	1933	1946	rBV	2271755	3227209	56.17%	5.082%
20	14.604	1968	1975	1989	rBV	599180	1415721	24.64%	2.229%
21	14.698	1989	1991	1997	rVB5	9447	20968	0.36%	0.033%
22	14.781	2002	2005	2009	rVB6	7809	11608	0.20%	0.018%
23	15.369	2096	2105	2121	rBV	3164809	5092191	88.64%	8.018%
24	15.516	2124	2130	2140	rVV	1059243	1688848	29.40%	2.659%
25	15.610	2143	2146	2151	rVB4	18950	33440	0.58%	0.053%
26	15.887	2189	2193	2198	rVB2	10085	16811	0.29%	0.026%
27	16.169	2236	2241	2247	rBV3	13709	22124	0.39%	0.035%
28	16.834	2349	2354	2359	rBV6	6618	10683	0.19%	0.017%
29	16.951	2366	2374	2382	rBV5	8649	24066	0.42%	0.038%
30	17.169	2403	2411	2421	rBV	2530683	3812389	66.36%	6.003%
31	17.275	2421	2429	2446	rVV2	3316484	5329590	92.77%	8.392%
32	17.863	2524	2529	2533	rBV8	8412	11638	0.20%	0.018%
33	18.098	2565	2569	2576	rBV6	29531	51506	0.90%	0.081%
34	19.198	2751	2756	2764	rBV2	49719	88952	1.55%	0.140%
35	19.275	2765	2769	2776	rVV	35603	57443	1.00%	0.090%
36	19.586	2820	2822	2824	rBV2	16556	14970	0.26%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071024\
Data File : BP020888.D
Acq On : 10 Jul 2024 20:20
Operator : MA/JU
Sample : PB161825BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK825

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Title : SVOA CALIBRATION

37	19.657	2827	2834	2848	rBV	3921686	5745090	100.00%	9.047%
38	21.622	3162	3168	3182	rVB	1995487	3108754	54.11%	4.895%
39	24.739	3690	3698	3716	rVB2	1673648	4546505	79.14%	7.159%
40	24.974	3730	3738	3749	rVB	1027547	2867088	49.91%	4.515%




Sum of corrected areas: 63506122

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071024\
Data File : BP020888.D
Acq On : 10 Jul 2024 20:20
Operator : MA/JU
Sample : PB161825BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK825

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

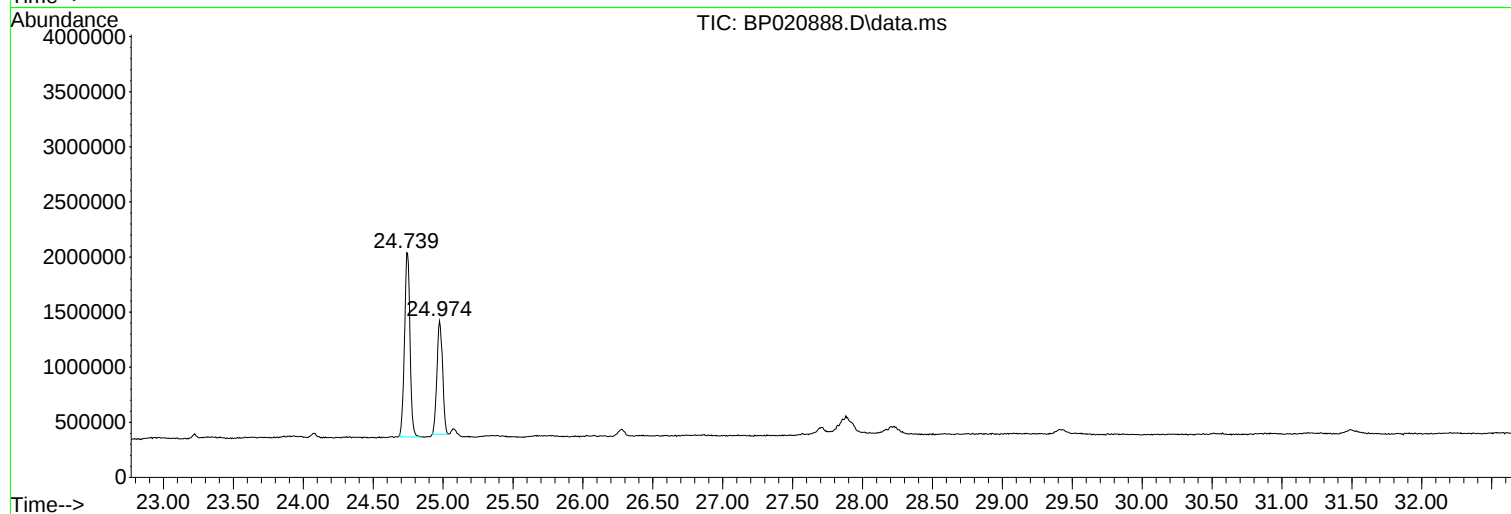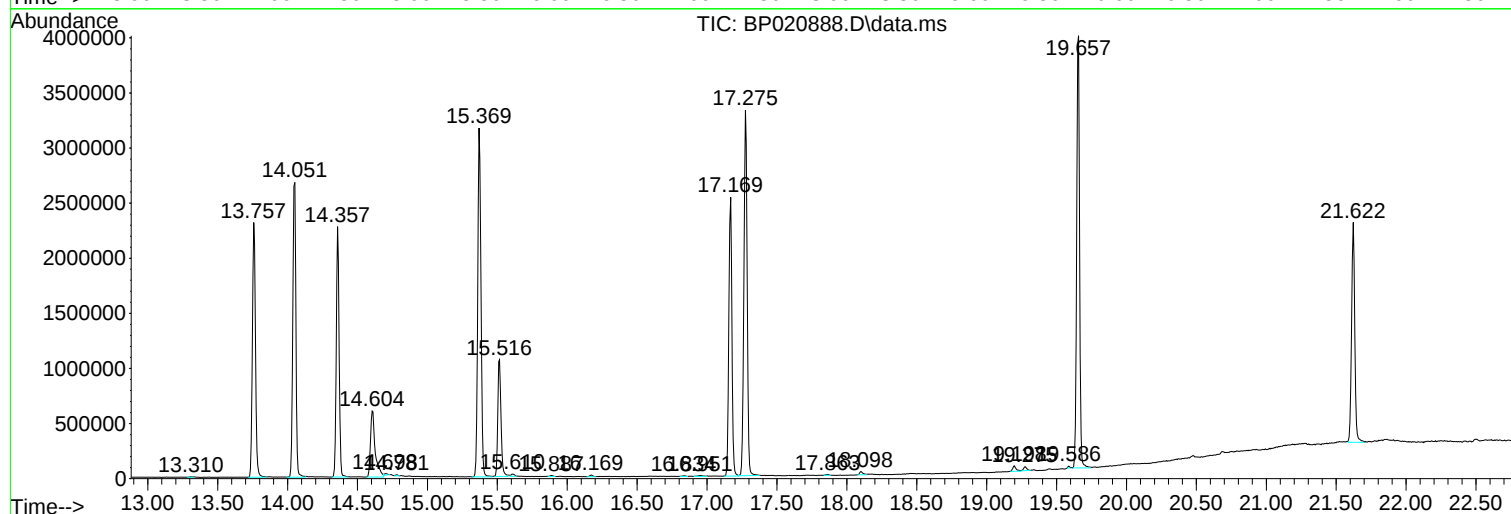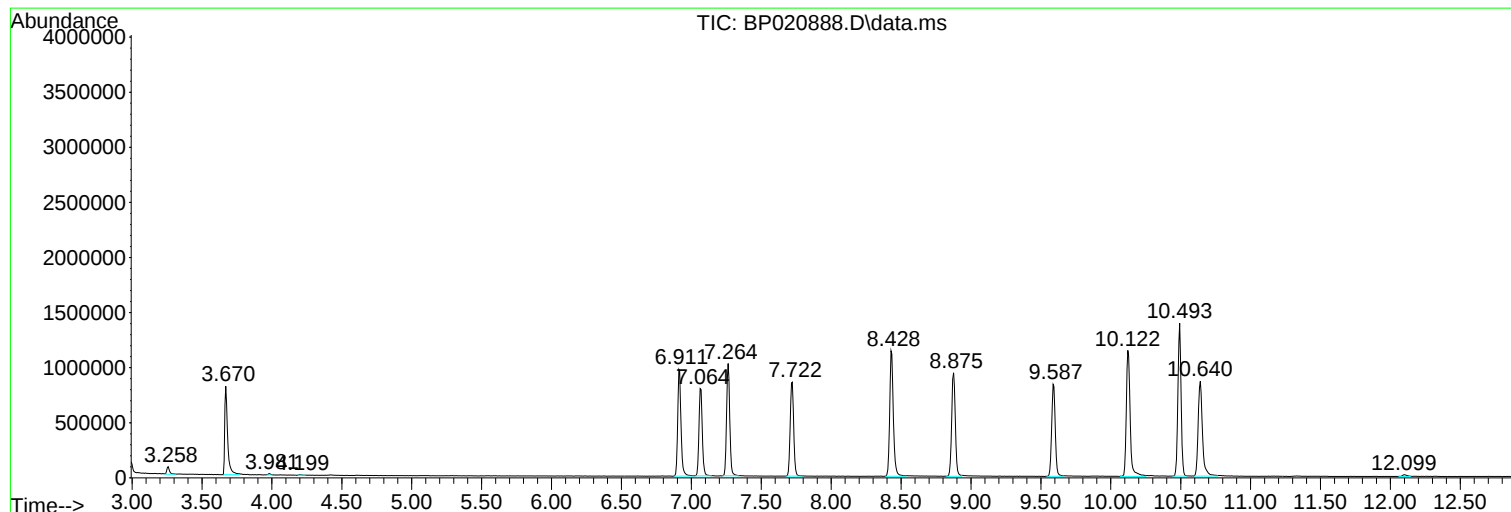

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071024\
Data File : BP020888.D
Acq On : 10 Jul 2024 20:20
Operator : MA/JU
Sample : PB161825BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK825

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071024\
Data File : BP020888.D
Acq On : 10 Jul 2024 20:20
Operator : MA/JU
Sample : PB161825BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK825

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc