

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071122\
 Data File : BP010947.D
 Acq On : 11 Jul 2022 12:35
 Operator : CG/JU
 Sample : PB146118TB 10X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLEB118

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010947.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	15	20	29	rVB	196305	261074	3.19%	0.248%
2	3.610	85	89	107	rBV	2053917	3000772	36.68%	2.845%
3	3.922	138	142	148	rVB	45646	61498	0.75%	0.058%
4	6.881	637	645	656	rBV	2405533	3642005	44.52%	3.453%
5	7.046	667	673	686	rVB	2096251	3128969	38.25%	2.966%
6	7.240	697	706	718	rBV	2483054	3813801	46.62%	3.616%
7	7.704	776	785	799	rBV	2064667	3160429	38.63%	2.996%
8	8.416	899	906	922	rBV	2828166	4453834	54.44%	4.222%
9	8.863	974	982	994	rBV	2157724	3452912	42.21%	3.273%
10	9.587	1095	1105	1117	rBV	1500264	2434971	29.76%	2.308%
11	10.122	1187	1196	1210	rBV	2540179	4022662	49.17%	3.814%
12	10.498	1251	1260	1270	rBV	2711693	4479321	54.75%	4.247%
13	10.639	1276	1284	1300	rBV	2142914	3593358	43.92%	3.407%
14	12.092	1525	1531	1540	rVB2	51284	82913	1.01%	0.079%
15	12.310	1562	1568	1573	rBV9	6915	15481	0.19%	0.015%
16	13.086	1693	1700	1703	rBV8	4942	9398	0.11%	0.009%
17	13.322	1737	1740	1746	rVB4	8401	10378	0.13%	0.010%
18	13.780	1811	1818	1829	rBV	3799501	5092826	62.25%	4.828%
19	14.051	1855	1864	1877	rBV	4600010	6424692	78.53%	6.091%
20	14.357	1910	1916	1926	rBV	3499344	4989646	60.99%	4.730%
21	14.569	1946	1952	1972	rBV	1270789	2071844	25.33%	1.964%
22	15.357	2079	2086	2100	rBV	5496369	7701429	94.14%	7.301%
23	15.480	2101	2107	2123	rVV	1066722	1532042	18.73%	1.452%
24	15.598	2123	2127	2135	rVB2	67144	99755	1.22%	0.095%
25	15.927	2180	2183	2188	rBV7	5561	8273	0.10%	0.008%
26	16.057	2199	2205	2207	rBV7	6360	10241	0.13%	0.010%
27	16.151	2217	2221	2227	rVB4	20244	28823	0.35%	0.027%
28	16.798	2328	2331	2336	rBV6	10048	12849	0.16%	0.012%
29	16.910	2346	2350	2353	rVB2	7111	8866	0.11%	0.008%
30	17.121	2380	2386	2397	rBV	3377710	4909416	60.01%	4.654%
31	17.221	2397	2403	2426	rVB2	5135311	7402202	90.48%	7.018%
32	19.051	2710	2714	2720	rBV2	55881	84042	1.03%	0.080%
33	19.115	2722	2725	2729	rBV	49587	68880	0.84%	0.065%
34	19.474	2780	2786	2794	rBV	6012663	7560003	92.41%	7.167%
35	21.239	3081	3086	3092	rBV	3672600	4592011	56.13%	4.353%
36	23.445	3454	3461	3472	rBV2	4351536	8180832	100.00%	7.756%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071122\
Data File : BP010947.D
Acq On : 11 Jul 2022 12:35
Operator : CG/JU
Sample : PB146118TB 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB118

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Title : SVOA CALIBRATION

37 23.598 3481 3487 3501 rVB2 2604963 5078702 62.08% 4.815%




Sum of corrected areas: 105481150

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071122\
Data File : BP010947.D
Acq On : 11 Jul 2022 12:35
Operator : CG/JU
Sample : PB146118TB 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB118

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

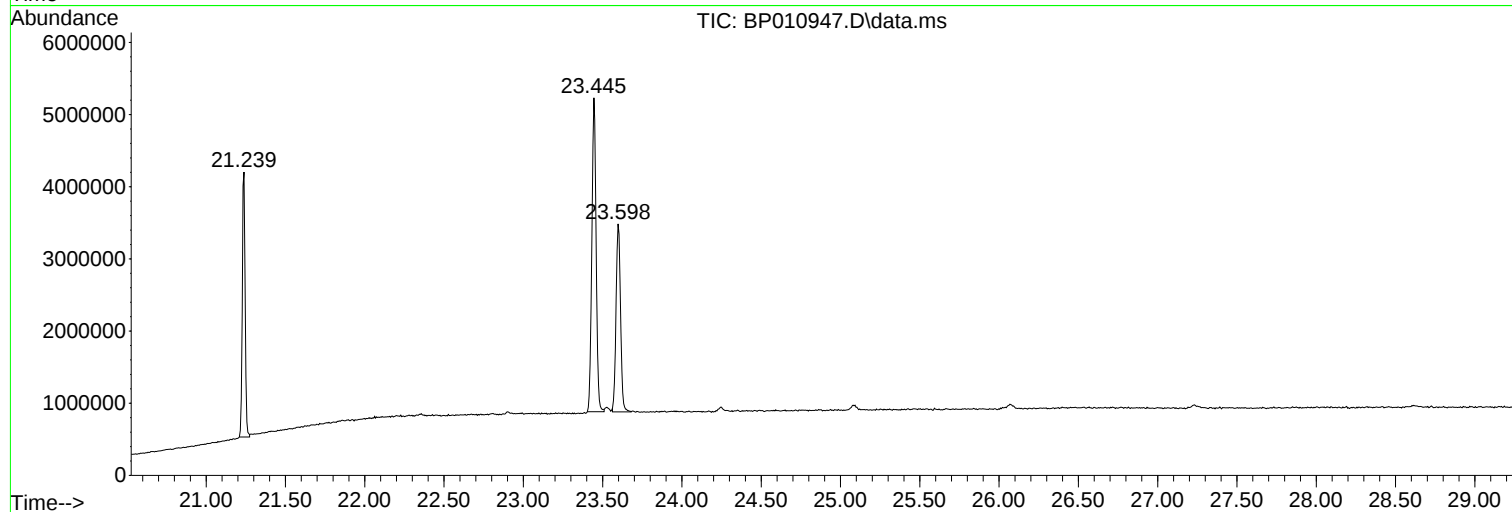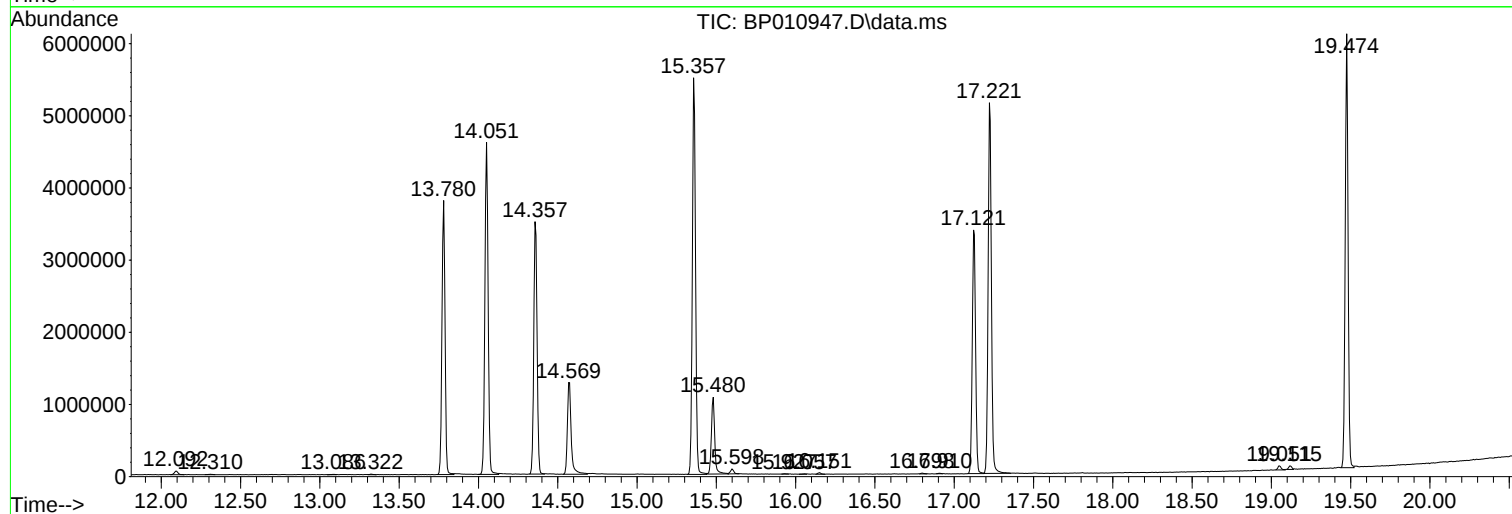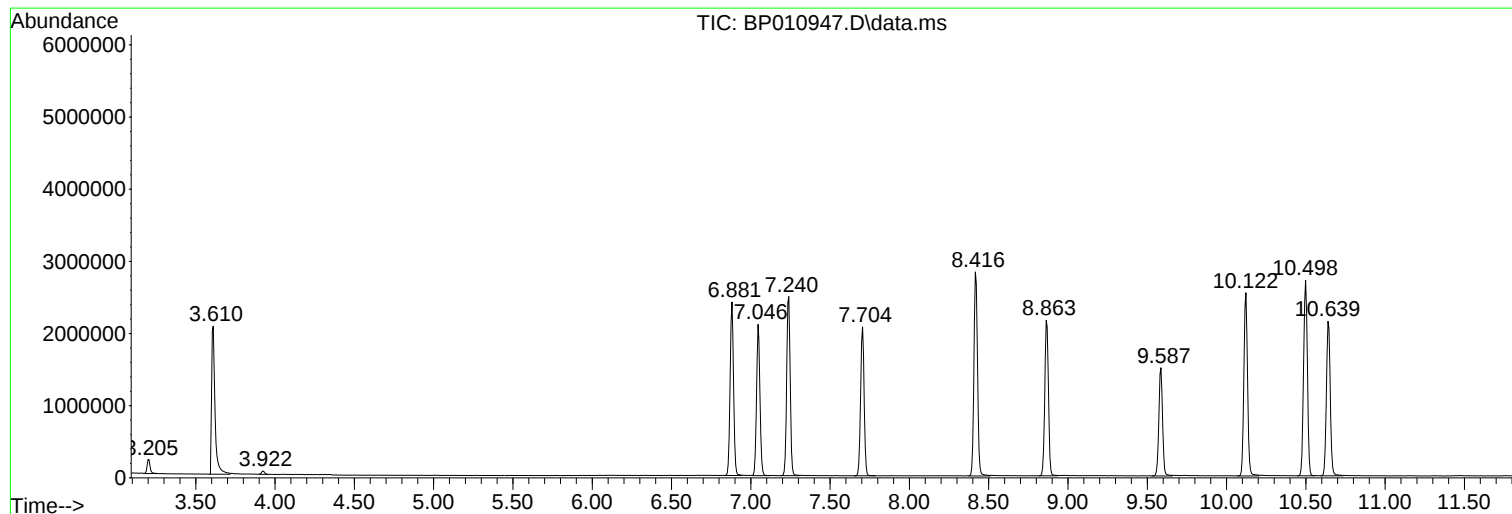

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071122\
Data File : BP010947.D
Acq On : 11 Jul 2022 12:35
Operator : CG/JU
Sample : PB146118TB 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB118

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071122\
Data File : BP010947.D
Acq On : 11 Jul 2022 12:35
Operator : CG/JU
Sample : PB146118TB 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB118

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------