

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071122\
 Data File : BP010948.D
 Acq On : 11 Jul 2022 13:09
 Operator : CG/JU
 Sample : N3639-01 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COL62

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010948.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.204	16	20	24	rBV	78359	95365	0.95%	0.111%
2	3.475	62	66	73	rBV	64139	93912	0.94%	0.109%
3	3.540	73	77	81	rVB	28131	34856	0.35%	0.040%
4	3.610	85	89	106	rBV	905335	1299155	12.95%	1.506%
5	3.834	122	127	133	rVB	63916	94287	0.94%	0.109%
6	3.922	139	142	148	rVB	23233	30405	0.30%	0.035%
7	4.298	202	206	210	rVB6	7056	11259	0.11%	0.013%
8	4.828	293	296	301	rBV	8992	13856	0.14%	0.016%
9	4.875	301	304	310	rVB	11210	18498	0.18%	0.021%
10	5.304	373	377	381	rVB2	7413	10666	0.11%	0.012%
11	5.422	394	397	404	rVB	14251	22416	0.22%	0.026%
12	5.669	435	439	445	rVB3	14401	20909	0.21%	0.024%
13	6.704	610	615	620	rBV6	10094	21516	0.21%	0.025%
14	6.875	637	644	655	rVB	626655	958113	9.55%	1.110%
15	7.045	666	673	682	rBV	2077369	3232060	32.21%	3.745%
16	7.116	682	685	693	rVB	25604	36458	0.36%	0.042%
17	7.234	698	705	717	rBV	2109600	3162533	31.52%	3.665%
18	7.322	717	720	725	rVB4	9668	12651	0.13%	0.015%
19	7.698	777	784	792	rBV	877062	1355813	13.51%	1.571%
20	7.769	792	796	805	rVB	62517	100408	1.00%	0.116%
21	8.298	879	886	889	rBV8	7610	16860	0.17%	0.020%
22	8.410	898	905	919	rBV	1563931	2532640	25.24%	2.935%
23	8.528	920	925	930	rVB	64669	99654	0.99%	0.115%
24	8.863	974	982	990	rBV	2316732	3594206	35.82%	4.165%
25	8.986	998	1003	1008	rBV	45790	71485	0.71%	0.083%
26	9.028	1008	1010	1017	rVB8	11320	17860	0.18%	0.021%
27	9.286	1050	1054	1059	rVB6	9417	17776	0.18%	0.021%
28	9.375	1059	1069	1071	rBV10	9882	22966	0.23%	0.027%
29	9.422	1074	1077	1086	rVB9	15405	34175	0.34%	0.040%
30	9.581	1095	1104	1118	rBV	1557074	2487251	24.79%	2.882%
31	10.033	1175	1181	1185	rBV8	7504	16786	0.17%	0.019%
32	10.116	1188	1195	1204	rBV	2402401	3817335	38.04%	4.424%
33	10.422	1242	1247	1251	rBV5	10381	16007	0.16%	0.019%
34	10.492	1251	1259	1267	rVB	1152590	1886755	18.80%	2.186%
35	10.639	1273	1284	1292	rBV	887576	1473862	14.69%	1.708%
36	11.051	1349	1354	1359	rBV	17139	26616	0.27%	0.031%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071122\
 Data File : BP010948.D
 Acq On : 11 Jul 2022 13:09
 Operator : CG/JU
 Sample : N3639-01 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COL62

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

37	11.110	1359	1364	1368	rBV	22862	33588	0.33%	0.039%
38	11.298	1391	1396	1399	rBV7	7194	12490	0.12%	0.014%
39	12.092	1523	1531	1536	rBV2	50806	81886	0.82%	0.095%
40	12.722	1633	1638	1642	rVB7	7939	14607	0.15%	0.017%
41	12.969	1674	1680	1684	rVB6	12812	19106	0.19%	0.022%
42	13.186	1712	1717	1721	rBV7	10509	14049	0.14%	0.016%
43	13.327	1736	1741	1745	rVV6	7630	11645	0.12%	0.013%
44	13.774	1810	1817	1830	rBV	3933809	5437154	54.18%	6.301%
45	14.045	1854	1863	1883	rBV	4713634	6812066	67.88%	7.894%
46	14.269	1896	1901	1905	rVB	18726	26186	0.26%	0.030%
47	14.351	1909	1915	1924	rVV	1365466	2046877	20.40%	2.372%
48	14.439	1928	1930	1937	rVB7	8514	12282	0.12%	0.014%
49	14.569	1946	1952	1964	rBV2	273353	465499	4.64%	0.539%
50	14.716	1974	1977	1983	rVV6	8373	11947	0.12%	0.014%
51	14.786	1984	1989	1993	rVB8	8602	14388	0.14%	0.017%
52	14.886	2003	2006	2012	rVB8	7332	13127	0.13%	0.015%
53	15.174	2051	2055	2056	rBV	13455	15772	0.16%	0.018%
54	15.221	2060	2063	2068	rVB	33276	43422	0.43%	0.050%
55	15.357	2079	2086	2100	rBV	5641115	8340374	83.11%	9.665%
56	15.474	2100	2106	2119	rVV	1191213	1632840	16.27%	1.892%
57	15.598	2122	2127	2131	rBV2	60772	89421	0.89%	0.104%
58	15.727	2146	2149	2154	rVB7	9965	16358	0.16%	0.019%
59	15.921	2179	2182	2187	rBV7	7434	12539	0.12%	0.015%
60	16.092	2207	2211	2217	rVV	52153	87470	0.87%	0.101%
61	16.145	2217	2220	2227	rVB4	24332	37645	0.38%	0.044%
62	16.792	2324	2330	2335	rBV10	13357	24994	0.25%	0.029%
63	16.892	2343	2347	2351	rBV	57105	66986	0.67%	0.078%
64	16.939	2353	2355	2359	rVB4	17474	24516	0.24%	0.028%
65	17.115	2379	2385	2395	rBV	1405902	2019494	20.12%	2.340%
66	17.221	2396	2403	2416	rVV	5856822	8490247	84.61%	9.839%
67	17.321	2417	2420	2424	rVB6	26084	38492	0.38%	0.045%
68	17.639	2471	2474	2480	rVB	45976	49271	0.49%	0.057%
69	17.815	2500	2504	2507	rVB	85905	97972	0.98%	0.114%
70	18.315	2586	2589	2594	rBV2	43971	57954	0.58%	0.067%
71	18.927	2691	2693	2700	rBV	26690	34798	0.35%	0.040%
72	19.045	2709	2713	2718	rBV2	72771	97939	0.98%	0.113%
73	19.115	2721	2725	2729	rVV	58031	76317	0.76%	0.088%
74	19.468	2780	2785	2793	rBV	6602651	8880843	88.50%	10.292%
75	20.968	3037	3040	3044	rBV2	114275	151815	1.51%	0.176%
76	21.233	3080	3085	3090	rBV	1571193	1975225	19.68%	2.289%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071122\
Data File : BP010948.D
Acq On : 11 Jul 2022 13:09
Operator : CG/JU
Sample : N3639-01 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0L62

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Title : SVOA CALIBRATION

77	23.445	3454	3461	3469	rVB	5335144	10034928	100.00%	11.629%
78	23.592	3481	3486	3496	rVB	1115460	2110024	21.03%	2.445%


Sum of corrected areas: 86291923

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071122\
Data File : BP010948.D
Acq On : 11 Jul 2022 13:09
Operator : CG/JU
Sample : N3639-01 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COL62

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

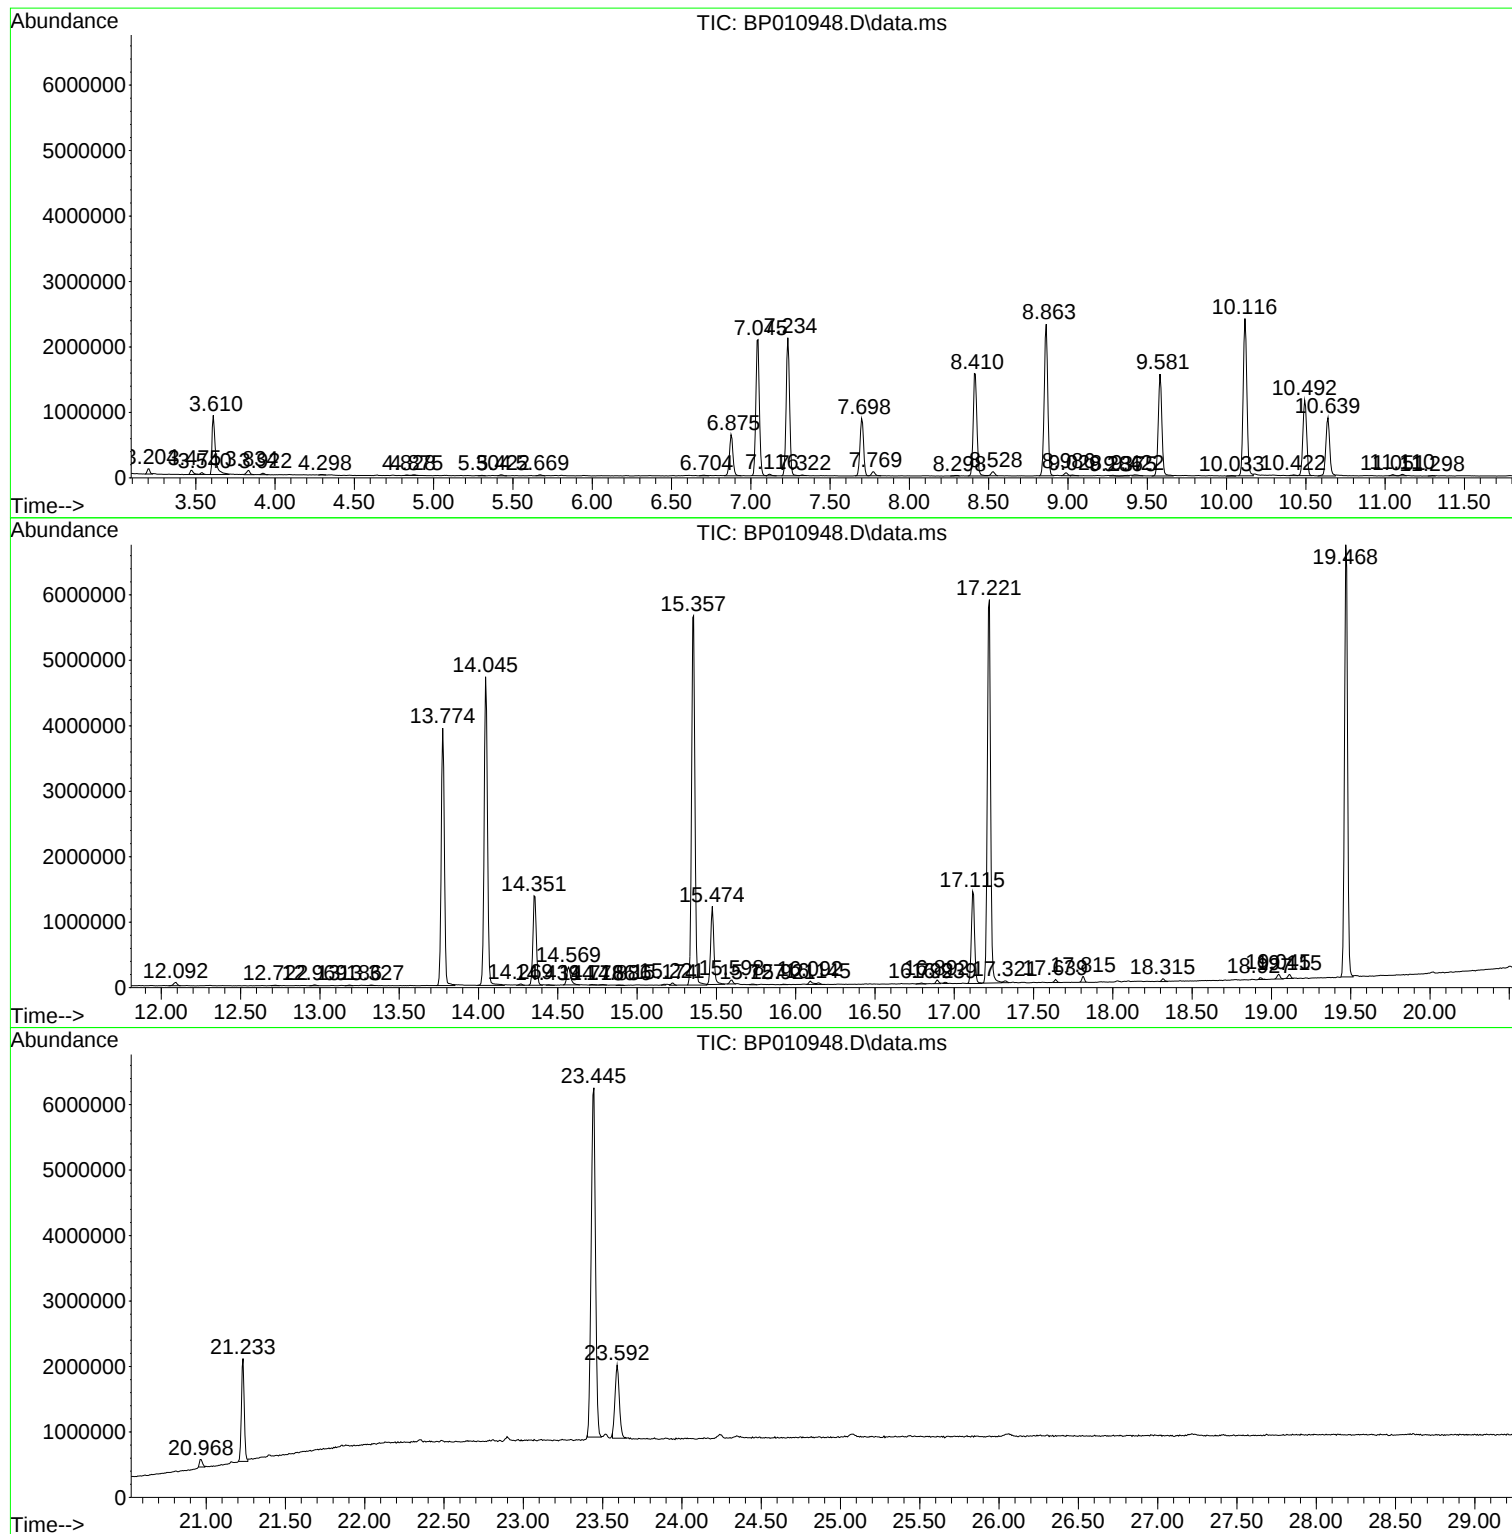

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071122\
Data File : BP010948.D
Acq On : 11 Jul 2022 13:09
Operator : CG/JU
Sample : N3639-01 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0L62

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071122\
Data File : BP010948.D
Acq On : 11 Jul 2022 13:09
Operator : CG/JU
Sample : N3639-01 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0L62

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc