

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071124\
 Data File : BP020903.D
 Acq On : 11 Jul 2024 14:29
 Operator : MA/JU
 Sample : P3088-03MS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4CC5MS

Quant Time: Jul 11 23:03:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 10 18:38:19 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.716	152	272086	20.000	ng/ul	0.00
20) Naphthalene-d8	10.487	136	1180027	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.357	164	769853	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.169	188	1401088	20.000	ng/ul	-0.01
79) Chrysene-d12	21.633	240	982487	20.000	ng/ul	0.01
88) Perylene-d12	24.992	264	1217044	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	24970	4.176	ng/uL	0.00
4) Pyridine-d5	3.670	84	375703	21.704	ng/ul	0.00
7) Phenol-d5	6.911	99	625000	28.176	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.063	67	377154	28.056	ng/ul	0.00
11) 2-Chlorophenol-d4	7.263	132	515157	28.187	ng/ul	0.00
15) 4-Methylphenol-d8	8.434	113	509846	27.674	ng/ul	0.00
21) Nitrobenzene-d5	8.875	128	258149	28.166	ng/ul	0.00
24) 2-Nitrophenol-d4	9.581	143	297142	28.325	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.128	165	546320	28.801	ng/ul	0.00
31) 4-Chloroaniline-d4	10.634	131	639253	25.438	ng/ul	0.00
46) Dimethylphthalate-d6	13.757	166	1523579	27.224	ng/ul	-0.01
49) Acenaphthylene-d8	14.045	160	1729333	27.520	ng/ul	0.00
54) 4-Nitrophenol-d4	14.604	143	204048	25.626	ng/ul	0.00
60) Fluorene-d10	15.369	176	1254785	27.330	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.522	200	232901	27.473	ng/ul	0.01
73) Anthracene-d10	17.275	188	1716375	27.581	ng/ul	0.00
81) Pyrene-d10	19.663	212	1664116	27.397	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.751	264	1727142	28.774	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.287	88	81117	12.335	ng/uL	98
5) Pyridine	3.687	79	509647	28.545	ng/ul	97
6) Benzaldehyde	6.887	77	256350	22.923	ng/ul	98
8) Phenol	6.940	94	838509	37.356	ng/ul	98
10) Bis(2-Chloroethyl)ether	7.158	93	653302	35.232	ng/ul	99
12) 2-Chlorophenol	7.293	128	663972	36.248	ng/ul	99
13) 2-Methylphenol	8.169	108	618188	35.611	ng/ul	98
14) 2,2'-oxybis(1-Chloropr...	8.234	45	941148	35.131	ng/ul	98
16) Acetophenone	8.540	105	1034439	36.379	ng/ul	99
17) N-Nitroso-di-n-propyla...	8.528	70	523890	35.163	ng/ul	99
18) 4-Methylphenol	8.499	108	685583	36.864	ng/ul	100
19) Hexachloroethane	8.775	117	279545	33.961	ng/ul	98
22) Nitrobenzene	8.916	77	773301	35.221	ng/ul	100
23) Isophorone	9.440	82	1484323	34.007	ng/ul	99
25) 2-Nitrophenol	9.616	139	406284	37.135	ng/ul	98
26) 2,4-Dimethylphenol	9.681	107	537868	24.931	ng/ul	98
27) Bis(2-Chloroethoxy)met...	9.904	93	917406	34.578	ng/ul	100
29) 2,4-Dichlorophenol	10.152	162	678979	36.320	ng/ul	98
30) Naphthalene	10.534	128	2122495	34.195	ng/ul	99
32) 4-Chloroaniline	10.657	127	649675	27.074	ng/ul	98
33) Hexachlorobutadiene	10.804	225	470951	33.598	ng/ul	99
34) Caprolactam	11.475	113	119651	20.777	ng/ul	97
35) 4-Chloro-3-methylphenol	11.799	107	741469	36.488	ng/ul	98
36) 2-Methylnaphthalene	12.157	142	1497912	35.156	ng/ul	99


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071124\
 Data File : BP020903.D
 Acq On : 11 Jul 2024 14:29
 Operator : MA/JU
 Sample : P3088-03MS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4CC5MS

Quant Time: Jul 11 23:03:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 10 18:38:19 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.369	142	1531088	34.940	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	12.522	216	884282	35.369	ng/ul	98
40) Hexachlorocyclopentadiene	12.493	237	373764	28.578	ng/ul	100
41) 2,4,6-Trichlorophenol	12.775	196	551407	34.903	ng/ul	98
42) 2,4,5-Trichlorophenol	12.857	196	600606	35.932	ng/ul	100
43) 1,1'-Biphenyl	13.175	154	1971722	35.045	ng/ul	99
44) 2-Chloronaphthalene	13.222	162	1551635	34.546	ng/ul	99
45) 2-Nitroaniline	13.440	65	451453	36.346	ng/ul	99
47) Dimethylphthalate	13.804	163	1899550	33.452	ng/ul	100
48) 2,6-Dinitrotoluene	13.951	165	402027	35.412	ng/ul	97
50) Acenaphthylene	14.075	152	2346299	32.977	ng/ul	100
51) 3-Nitroaniline	14.281	138	356510	36.087	ng/ul	99
52) Acenaphthene	14.416	153	1557123	32.974	ng/ul	98
53) 2,4-Dinitrophenol	14.492	184	214101	35.911	ng/ul	100
55) 4-Nitrophenol	14.616	109	231370	35.721	ng/ul	95
56) Dibenzofuran	14.769	168	2178814	33.693	ng/ul	99
57) 2,4-Dinitrotoluene	14.745	165	543029	34.844	ng/ul	95
58) 2,3,4,6-Tetrachlorophenol	15.004	232	467085	32.633	ng/ul	98
59) Diethylphthalate	15.198	149	1843277	32.481	ng/ul	99
61) Fluorene	15.428	166	1725426	32.697	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.422	204	929062	32.445	ng/ul	97
63) 4-Nitroaniline	15.469	138	326998	39.969	ng/ul	98
66) 4,6-Dinitro-2-methylph...	15.534	198	324438	36.089	ng/ul#	97
67) N-Nitrosodiphenylamine	15.645	169	1495366	36.651	ng/ul	99
68) 4-Bromophenyl-phenylether	16.339	248	587867	35.797	ng/ul	97
69) Hexachlorobenzene	16.451	284	654817	34.775	ng/ul	98
70) Atrazine	16.634	200	345745	23.252	ng/ul	100
71) Pentachlorophenol	16.816	266	324575	31.737	ng/ul	99
72) Phenanthrene	17.216	178	2558120	35.196	ng/ul	99
74) Anthracene	17.316	178	2481224	33.486	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.134	216	931058	41.518	ng/uL	99
76) Pentachlorobenzene	14.675	250	756906	33.968	ng/uL	100
77) Carbazole	17.598	167	2044660	33.756	ng/ul	100
78) Di-n-butylphthalate	18.175	149	2744069	32.836	ng/ul	100
80) Fluoranthene	19.316	202	2557959	34.871	ng/ul	100
82) Pyrene	19.692	202	2642303	35.398	ng/ul	100
83) Butylbenzylphthalate	20.639	149	1020901	32.826	ng/ul	96
84) 3,3'-Dichlorobenzidine	21.533	252	715462	31.869	ng/ul	99
85) Benzo(a)anthracene	21.610	228	2374913	34.507	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.533	149	1422239	31.777	ng/ul	99
87) Chrysene	21.680	228	2269916	35.494	ng/ul	100
89) Di-n-octyl phthalate	22.816	149	2594824	32.275	ng/ul	100
90) Benzo(b)fluoranthene	23.921	252	2625386	35.547	ng/ul	99
91) Benzo(k)fluoranthene	23.998	252	2524321	34.248	ng/ul	99
93) Benzo(a)pyrene	24.827	252	2222364	31.842	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	28.815	276	3322530	36.944	ng/ul	99
95) Dibenzo(a,h)anthracene	28.874	278	2680264	35.990	ng/ul	99
96) Benzo(g,h,i)perylene	29.998	276	2604240	35.556	ng/ul	99





(#) = qualifier out of range (m) = manual integration (+) = signals summed

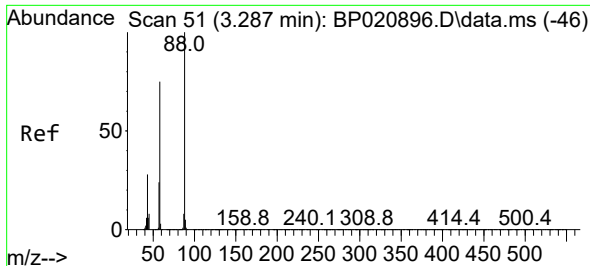

#2
 1,4-Dioxane
 Concen: 12.335 ng/uL
 RT: 3.287 min Scan# 51
 Delta R.T. 0.000 min
 Lab File: BP020903.D
 Acq: 11 Jul 2024 14:29




Instrument :
 BNA_P
 ClientSampleId :
 A4CC5MS


Tgt Ion: 88	Resp: 81117
Ion Ratio	Lower Upper
88	100
43	31.9 25.4 38.0
58	76.1 59.2 88.8

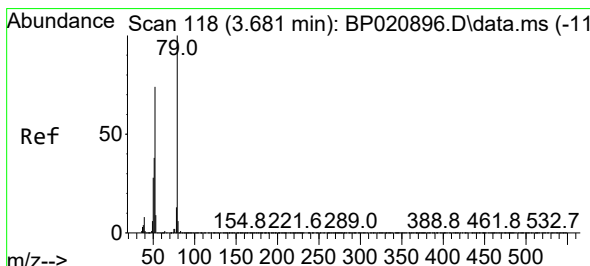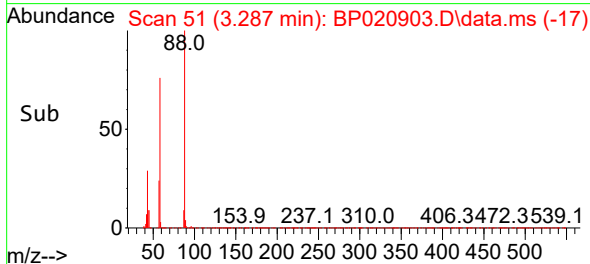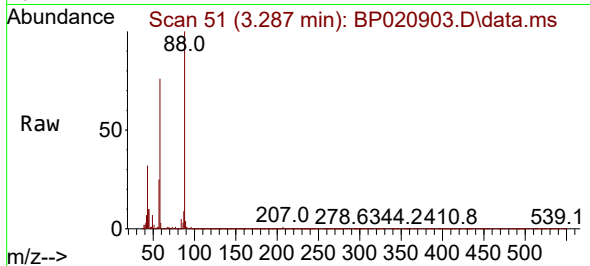

#5
 Pyridine
 Concen: 28.545 ng/uL
 RT: 3.687 min Scan# 119
 Delta R.T. 0.000 min
 Lab File: BP020903.D
 Acq: 11 Jul 2024 14:29

Tgt Ion: 79	Resp: 509647
Ion Ratio	Lower Upper
79	100
52	77.1 64.9 97.3
51	37.8 30.5 45.7


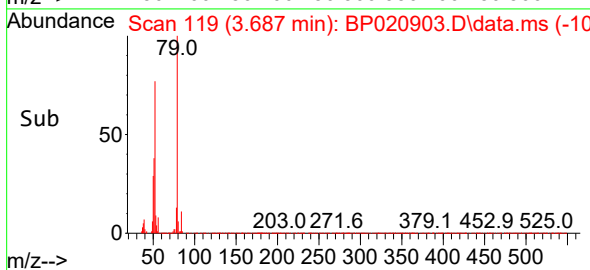

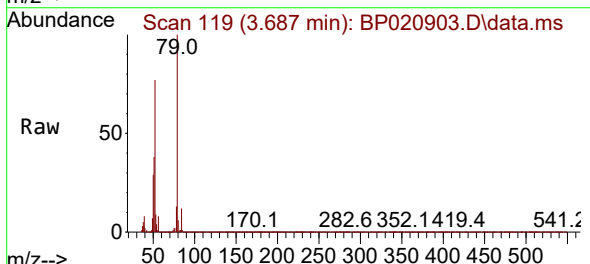




#6
Benzaldehyde
Concen: 22.923 ng/ul
RT: 6.887 min Scan# 661
Delta R.T. 0.000 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29




Instrument :
BNA_P
ClientSampleId :
A4CC5MS


Tgt Ion: 77 Resp: 256350
Ion Ratio Lower Upper
77 100
105 97.9 79.3 118.9
106 90.3 74.6 112.0

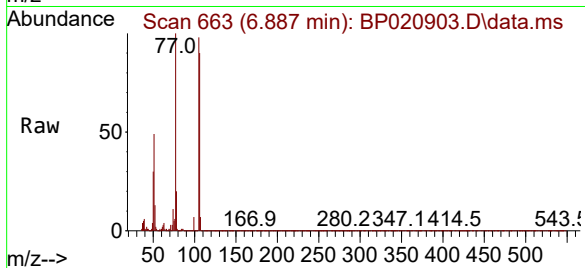

#8
Phenol
Concen: 37.356 ng/ul
RT: 6.940 min Scan# 672
Delta R.T. 0.000 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29

Tgt Ion: 94 Resp: 838509
Ion Ratio Lower Upper
94 100
65 28.8 23.4 35.0
66 40.4 33.9 50.9


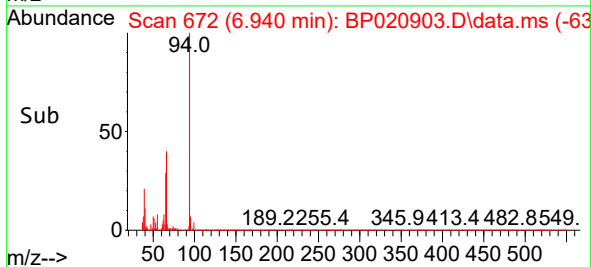

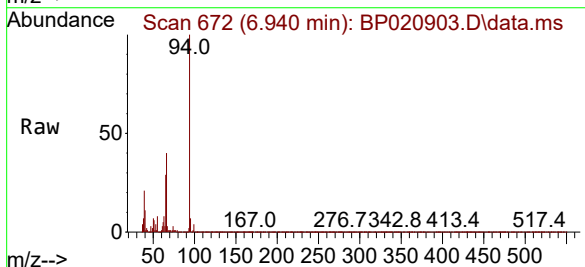




#10
Bis(2-Chloroethyl)ether
Concen: 35.232 ng/ul
RT: 7.158 min Scan# 709
Delta R.T. 0.006 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29




Instrument :
BNA_P
ClientSampleId :
A4CC5MS


Tgt Ion: 93 Resp: 653302
Ion Ratio Lower Upper
93 100
63 76.8 61.5 92.3
95 33.1 25.1 37.7



#12
2-Chlorophenol
Concen: 36.248 ng/ul
RT: 7.293 min Scan# 732
Delta R.T. -0.006 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29

Tgt Ion: 128 Resp: 663972
Ion Ratio Lower Upper
128 100
64 47.3 37.9 56.9
130 32.8 25.6 38.4

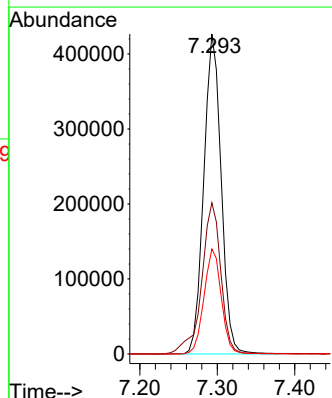



#13

2-Methylphenol

Concen: 35.611 ng/ul

RT: 8.169 min Scan# 880

Delta R.T. 0.000 min

Lab File: BP020903.D

Acq: 11 Jul 2024 14:29

Instrument :

BNA_P

ClientSampleId :





A4CC5MS

Tgt Ion:108 Resp: 618188

Ion Ratio Lower Upper

108 100

107 90.1 73.8 110.8

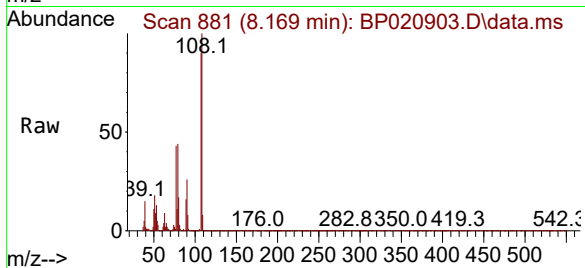

#14

2,2'-oxybis(1-Chloropropane)

Concen: 35.131 ng/ul

RT: 8.234 min Scan# 892

Delta R.T. -0.006 min

Lab File: BP020903.D

Acq: 11 Jul 2024 14:29




Tgt Ion: 45 Resp: 941148


Ion Ratio Lower Upper

45 100

77 14.5 10.9 16.3

79 10.5 8.1 12.1


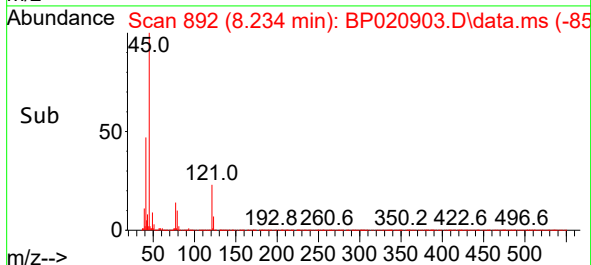
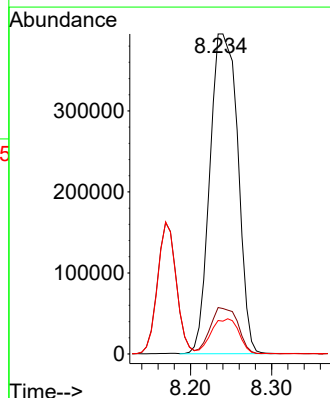
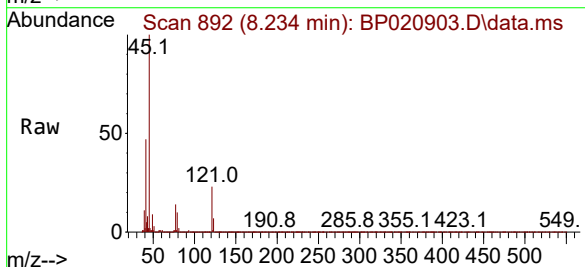




#16
Acetophenone
Concen: 36.379 ng/ul
RT: 8.540 min Scan# 941
Delta R.T. 0.000 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29




Instrument :
BNA_P
ClientSampleId :
A4CC5MS


Tgt Ion:105 Resp: 1034439
Ion Ratio Lower Upper
105 100
77 77.7 61.8 92.8
51 28.0 21.5 32.3



#17
N-Nitroso-di-n-propylamine
Concen: 35.163 ng/ul
RT: 8.528 min Scan# 942
Delta R.T. 0.012 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29

Tgt Ion: 70 Resp: 523890
Ion Ratio Lower Upper
70 100
42 57.6 46.6 69.8
101 10.4 7.4 11.0
130 21.5 17.2 25.8









#18
4-Methylphenol
Concen: 36.864 ng/ul
RT: 8.499 min Scan# 91
Delta R.T. 0.000 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29




Instrument :
BNA_P
ClientSampleId :
A4CC5MS


Tgt Ion:108 Resp: 685583
Ion Ratio Lower Upper
108 100
107 109.7 87.8 131.8



#19
Hexachloroethane
Concen: 33.961 ng/ul
RT: 8.775 min Scan# 984
Delta R.T. -0.006 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29

Tgt Ion:117 Resp: 279545
Ion Ratio Lower Upper
117 100
201 108.7 88.2 132.2
199 67.0 55.8 83.6









#22
Nitrobenzene
Concen: 35.221 ng/ul
RT: 8.916 min Scan# 1007
Delta R.T. 0.006 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29




Instrument :
BNA_P
ClientSampleId :
A4CC5MS


Tgt Ion: 77 Resp: 773301
Ion Ratio Lower Upper
77 100
123 45.9 36.7 55.1
65 13.8 11.1 16.7

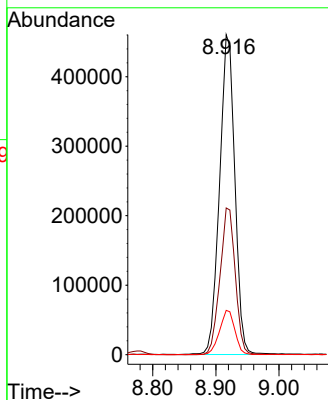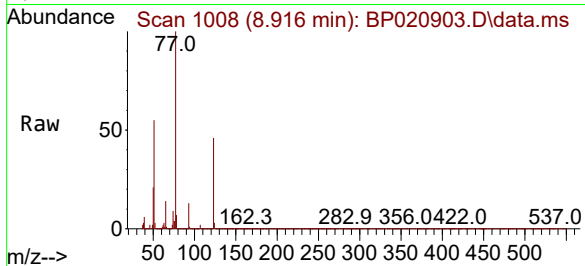

#23
Isophorone
Concen: 34.007 ng/ul
RT: 9.440 min Scan# 1097
Delta R.T. 0.000 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29

Tgt Ion: 82 Resp: 1484323
Ion Ratio Lower Upper
82 100
95 7.9 6.1 9.1
138 18.3 14.4 21.6



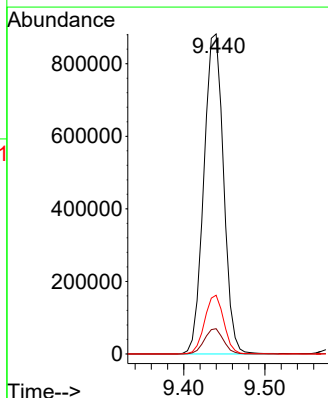
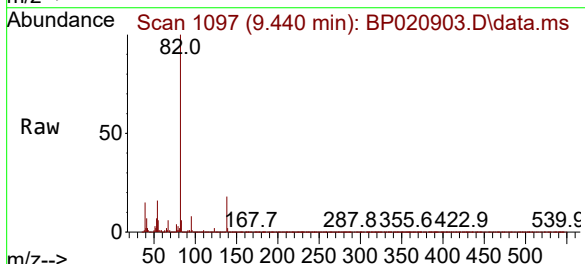




#25
2-Nitrophenol
Concen: 37.135 ng/ul
RT: 9.616 min Scan# 1127
Delta R.T. 0.000 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29




Instrument :
BNA_P
ClientSampleId :
A4CC5MS


Tgt Ion:139 Resp: 406284
Ion Ratio Lower Upper
139 100
65 51.4 42.9 64.3
109 33.0 26.2 39.4



#26
2,4-Dimethylphenol
Concen: 24.931 ng/ul
RT: 9.681 min Scan# 1138
Delta R.T. 0.006 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29

Tgt Ion:107 Resp: 537868
Ion Ratio Lower Upper
107 100
121 49.2 39.6 59.4
122 80.9 66.3 99.5

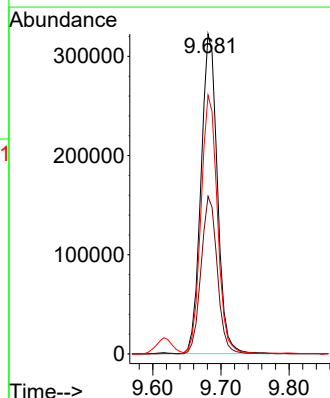



#27

Bis(2-Chloroethoxy)methane

Concen: 34.578 ng/ul

RT: 9.904 min Scan# 1176

Delta R.T. -0.006 min

Lab File: BP020903.D

Acq: 11 Jul 2024 14:29

Instrument :

BNA_P

ClientSampleId :

A4CC5MS





Tgt Ion: 93 Resp: 917406

Ion Ratio Lower Upper

93 100

95 31.8 25.5 38.3

123 11.3 9.0 13.4

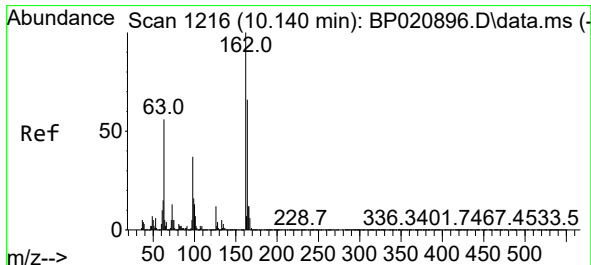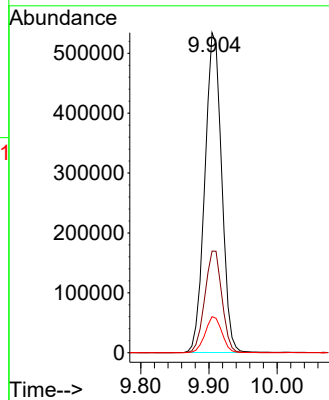

#29

2,4-Dichlorophenol

Concen: 36.320 ng/ul

RT: 10.152 min Scan# 1218

Delta R.T. 0.000 min

Lab File: BP020903.D

Acq: 11 Jul 2024 14:29




Tgt Ion:162 Resp: 678979


Ion Ratio Lower Upper

162 100

164 65.8 53.3 79.9

98 37.3 28.7 43.1

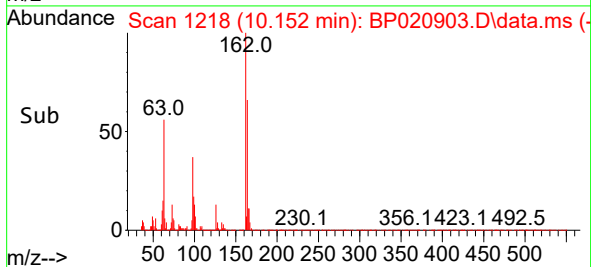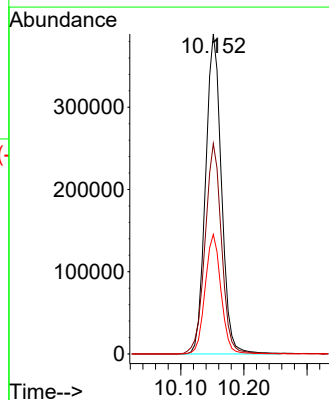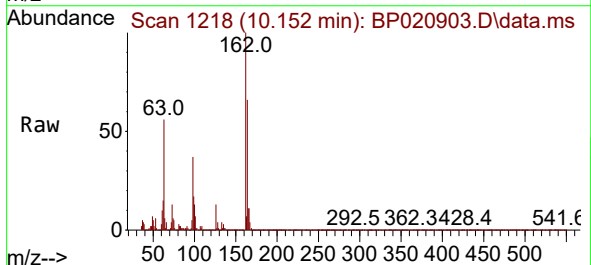



#30

Naphthalene

Concen: 34.195 ng/ul

RT: 10.534 min Scan# 1282

Delta R.T. -0.012 min

Lab File: BP020903.D

Acq: 11 Jul 2024 14:29

Instrument :

BNA_P

ClientSampleId :

A4CC5MS





Tgt Ion:128 Resp: 2122495

Ion Ratio Lower Upper

128 100

129 11.0 8.6 13.0

127 13.2 10.8 16.2

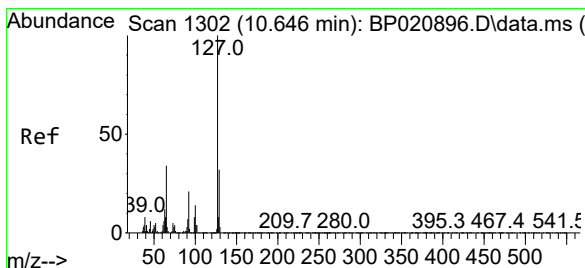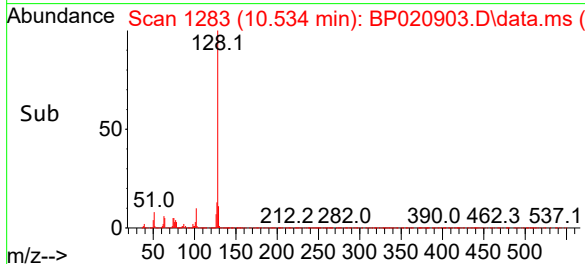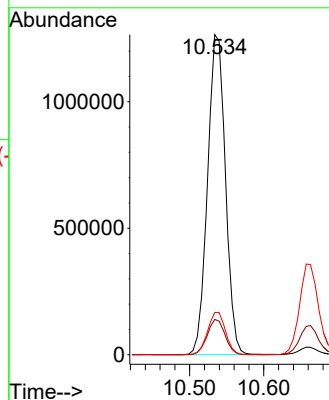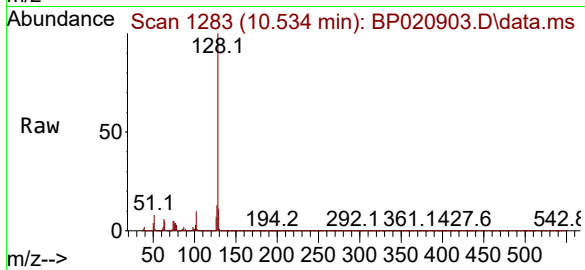

#32

4-Chloroaniline

Concen: 27.074 ng/ul

RT: 10.657 min Scan# 1304

Delta R.T. -0.006 min

Lab File: BP020903.D




Acq: 11 Jul 2024 14:29


Tgt Ion:127 Resp: 649675

Ion Ratio Lower Upper

127 100

129 31.3 26.1 39.1


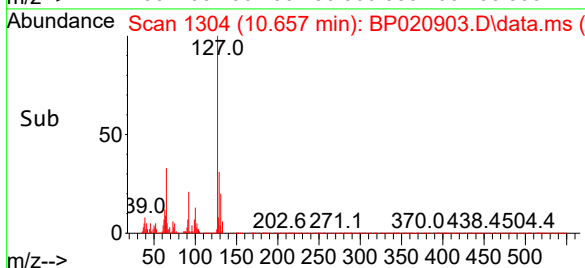
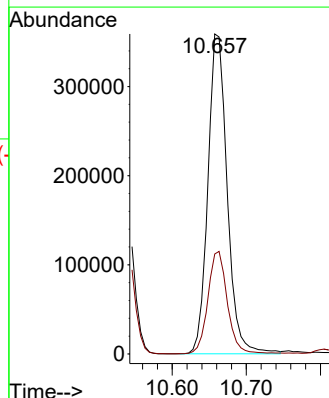
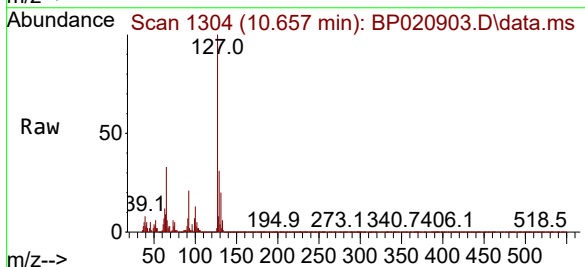




#33
Hexachlorobutadiene
Concen: 33.598 ng/ul
RT: 10.804 min Scan# 11
Delta R.T. 0.000 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29




Instrument :
BNA_P
ClientSampleId :
A4CC5MS


Tgt Ion:225 Resp: 470951
Ion Ratio Lower Upper
225 100
223 62.1 50.2 75.2
227 64.0 50.6 75.8

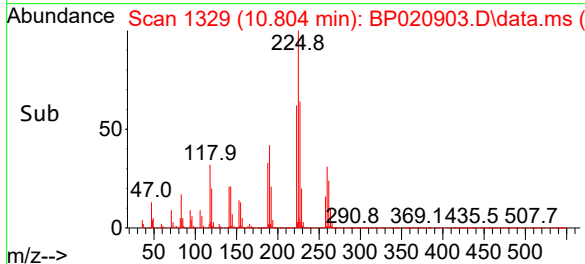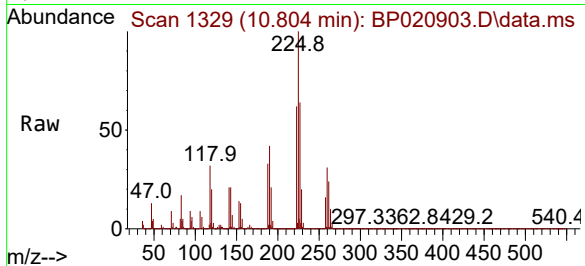

#34
Caprolactam
Concen: 20.777 ng/ul
RT: 11.475 min Scan# 1443
Delta R.T. 0.018 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29

Tgt Ion:113 Resp: 119651
Ion Ratio Lower Upper
113 100
55 172.3 140.2 210.4
56 126.4 105.5 158.3


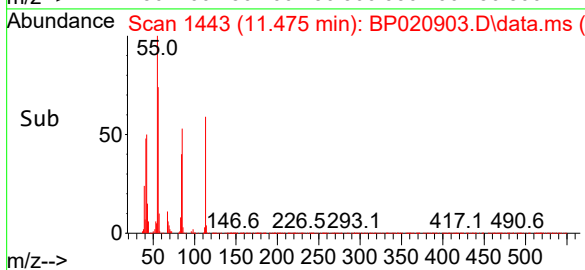

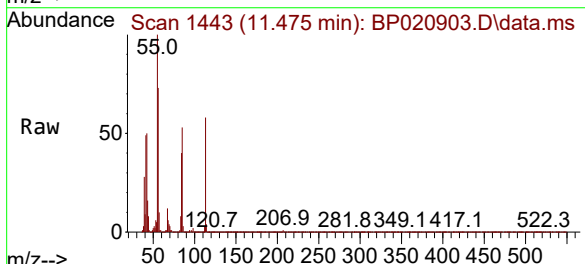




#35
4-Chloro-3-methylphenol
Concen: 36.488 ng/ul
RT: 11.799 min Scan# 1498
Delta R.T. 0.006 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29




Instrument :
BNA_P
ClientSampleId :
A4CC5MS


Tgt Ion:107 Resp: 741469
Ion Ratio Lower Upper
107 100
144 24.8 19.3 28.9
142 74.0 60.7 91.1

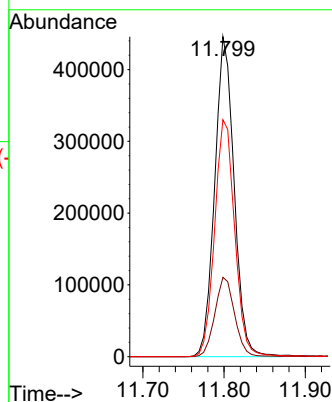

#36
2-Methylnaphthalene
Concen: 35.156 ng/ul
RT: 12.157 min Scan# 1559
Delta R.T. 0.012 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29

Tgt Ion:142 Resp: 1497912
Ion Ratio Lower Upper
142 100
141 90.0 72.6 108.8









#37
1-Methylnaphthalene
Concen: 34.940 ng/ul
RT: 12.369 min Scan# 1593
Delta R.T. -0.012 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29




Instrument :
BNA_P
ClientSampleId :
A4CC5MS


Tgt Ion:142 Resp: 1531088
Ion Ratio Lower Upper
142 100
141 93.8 75.0 112.6
116 4.0 3.2 4.8

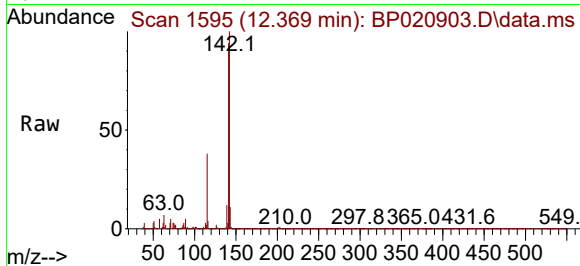

#39
1,2,4,5-Tetrachlorobenzene
Concen: 35.369 ng/ul
RT: 12.522 min Scan# 1621
Delta R.T. 0.006 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29

Tgt Ion:216 Resp: 884282
Ion Ratio Lower Upper
216 100
214 78.3 64.2 96.4
179 21.2 16.6 24.8
108 15.9 13.4 20.2




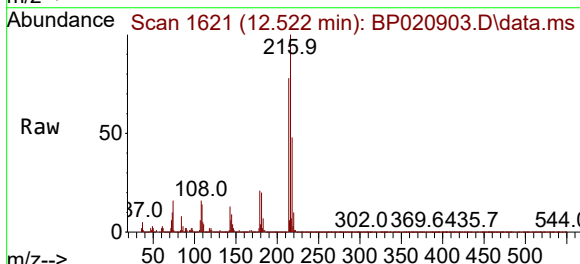




#40
Hexachlorocyclopentadiene
Concen: 28.578 ng/ul
RT: 12.493 min Scan# 1614
Delta R.T. 0.006 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29




Instrument :
BNA_P
ClientSampleId :
A4CC5MS


Tgt Ion:237 Resp: 373764
Ion Ratio Lower Upper
237 100
235 62.5 49.7 74.5
272 12.7 10.2 15.2



#41
2,4,6-Trichlorophenol
Concen: 34.903 ng/ul
RT: 12.775 min Scan# 1664
Delta R.T. -0.006 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29

Tgt Ion:196 Resp: 551407
Ion Ratio Lower Upper
196 100
198 93.9 76.6 115.0
200 30.9 26.0 39.0





#42

2,4,5-Trichlorophenol

Concen: 35.932 ng/ul

RT: 12.857 min Scan# 1

Delta R.T. -0.006 min

Lab File: BP020903.D

Acq: 11 Jul 2024 14:29

Instrument :

BNA_P

ClientSampleId :

A4CC5MS





Tgt Ion:196 Resp: 600606

Ion Ratio Lower Upper

196 100

198 96.1 77.1 115.7

200 31.4 25.3 37.9

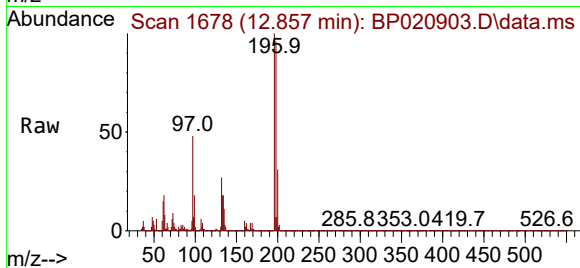

#43

1,1'-Biphenyl

Concen: 35.045 ng/ul

RT: 13.175 min Scan# 1732

Delta R.T. 0.000 min

Lab File: BP020903.D

Acq: 11 Jul 2024 14:29




Tgt Ion:154 Resp: 1971722


Ion Ratio Lower Upper

154 100

153 40.4 32.7 49.1

76 12.3 9.4 14.2

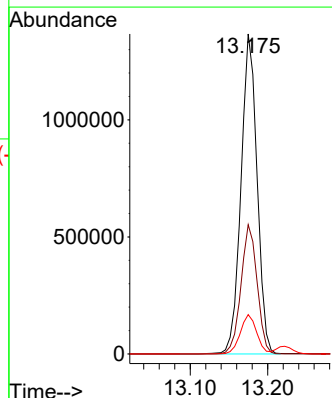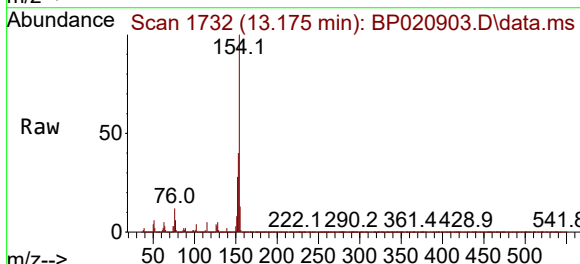



#44

2-Chloronaphthalene

Concen: 34.546 ng/ul

RT: 13.222 min Scan# 1740

Delta R.T. 0.006 min

Lab File: BP020903.D

Acq: 11 Jul 2024 14:29

Instrument :

BNA_P

ClientSampleId :

A4CC5MS





Tgt Ion:162 Resp: 1551635

Ion Ratio Lower Upper

162 100

164 32.9 26.3 39.5

127 40.7 31.8 47.8

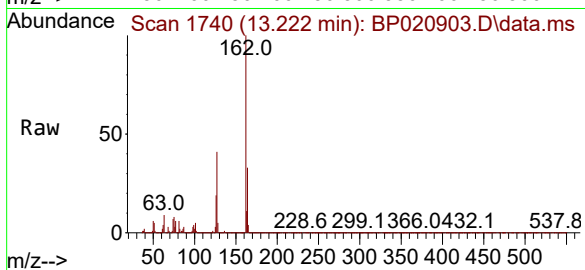

#45

2-Nitroaniline

Concen: 36.346 ng/ul

RT: 13.440 min Scan# 1777

Delta R.T. 0.000 min

Lab File: BP020903.D

Acq: 11 Jul 2024 14:29




Tgt Ion: 65 Resp: 451453


Ion Ratio Lower Upper

65 100

92 69.4 56.7 85.1

138 107.0 85.6 128.4




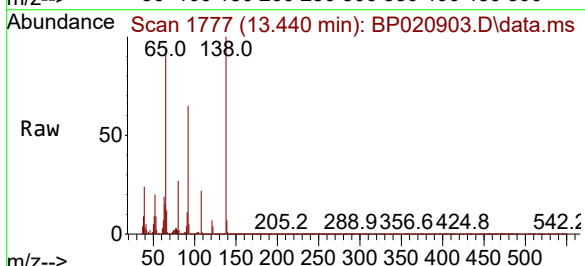


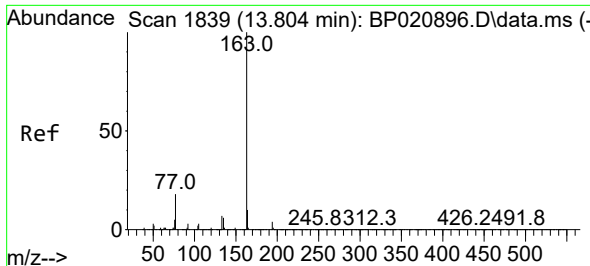

#47
Dimethylphthalate
Concen: 33.452 ng/ul
RT: 13.804 min Scan# 1839
Delta R.T. -0.012 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29




Instrument :
BNA_P
ClientSampleId :
A4CC5MS


Tgt Ion:163 Resp: 1899550
Ion Ratio Lower Upper
163 100
194 4.2 3.4 5.0
164 10.2 8.1 12.1

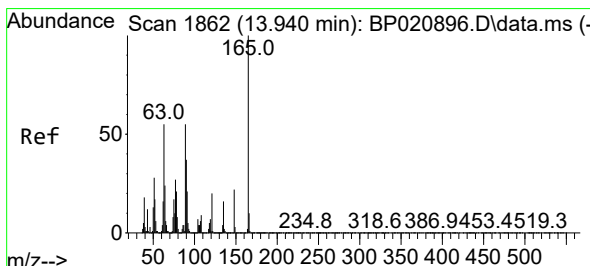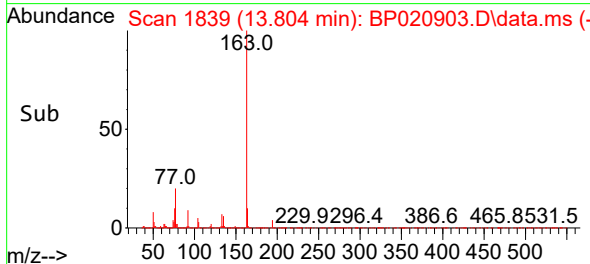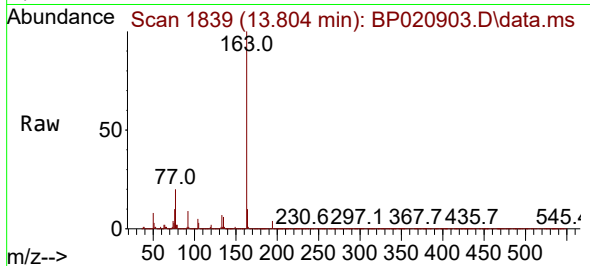

#48
2,6-Dinitrotoluene
Concen: 35.412 ng/ul
RT: 13.951 min Scan# 1864
Delta R.T. 0.012 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29

Tgt Ion:165 Resp: 402027
Ion Ratio Lower Upper
165 100
89 53.0 44.7 67.1
121 20.1 16.5 24.7


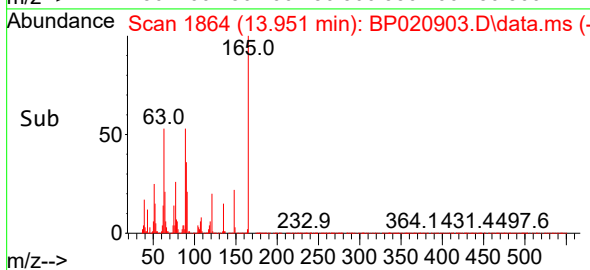

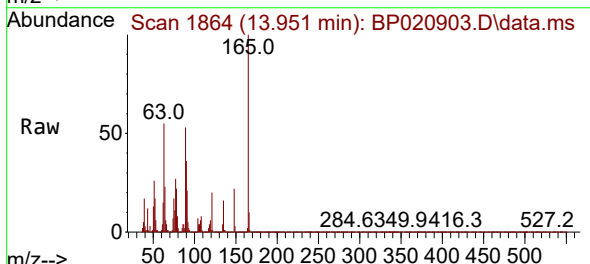




#50
Acenaphthylene
Concen: 32.977 ng/ul
RT: 14.075 min Scan# 1885
Delta R.T. -0.006 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29




Instrument :
BNA_P
ClientSampleId :
A4CC5MS


Tgt Ion:152 Resp: 2346299
Ion Ratio Lower Upper
152 100
151 20.3 16.2 24.2
153 12.9 10.3 15.5

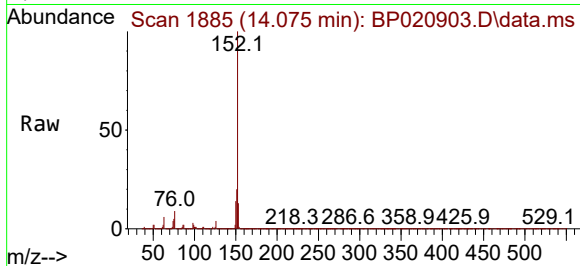

#51
3-Nitroaniline
Concen: 36.087 ng/ul
RT: 14.281 min Scan# 1920
Delta R.T. 0.000 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29

Tgt Ion:138 Resp: 356510
Ion Ratio Lower Upper
138 100
108 12.4 9.8 14.8
92 123.3 98.0 147.0

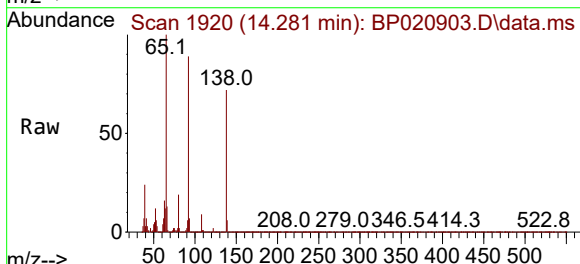



#52

Acenaphthene

Concen: 32.974 ng/ul

RT: 14.416 min Scan# 1943

Delta R.T. -0.006 min

Lab File: BP020903.D

Acq: 11 Jul 2024 14:29

Instrument :

BNA_P

ClientSampleId :

A4CC5MS





Tgt Ion:153 Resp: 1557123

Ion Ratio Lower Upper

153 100

152 46.2 37.8 56.6

154 87.0 71.8 107.6



#53

2,4-Dinitrophenol

Concen: 35.911 ng/ul

RT: 14.492 min Scan# 1956

Delta R.T. -0.012 min

Lab File: BP020903.D

Acq: 11 Jul 2024 14:29




Tgt Ion:184 Resp: 214101


Ion Ratio Lower Upper

184 100

63 62.8 50.3 75.5

154 66.4 53.0 79.6









#55
4-Nitrophenol
Concen: 35.721 ng/ul
RT: 14.616 min Scan# 1976
Delta R.T. -0.006 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29




Instrument :
BNA_P
ClientSampleId :
A4CC5MS


Tgt Ion	109	Resp	231370
Ion	Ratio	Lower	Upper
109	100		
139	127.6	98.0	147.0
65	125.4	106.0	159.0

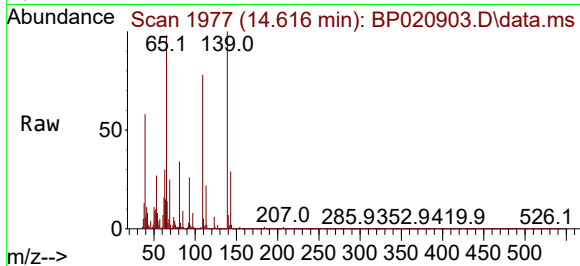

#56
Dibenzofuran
Concen: 33.693 ng/ul
RT: 14.769 min Scan# 2003
Delta R.T. 0.006 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29

Tgt Ion	168	Resp	2178814
Ion	Ratio	Lower	Upper
168	100		
139	38.3	31.1	46.7









#57
2,4-Dinitrotoluene
Concen: 34.844 ng/ul
RT: 14.745 min Scan# 1999
Delta R.T. -0.006 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29




Instrument :
BNA_P
ClientSampleId :
A4CC5MS


Tgt Ion:165 Resp: 543029
Ion Ratio Lower Upper
165 100
63 47.2 41.0 61.4
182 2.9 2.2 3.4

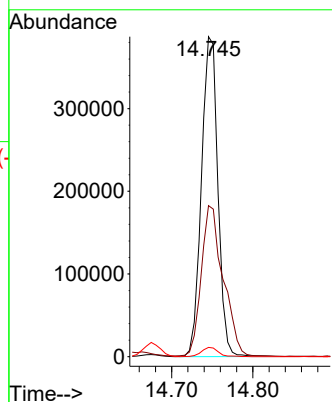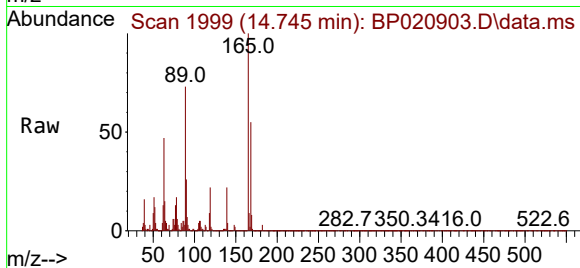

#58
2,3,4,6-Tetrachlorophenol
Concen: 32.633 ng/ul
RT: 15.004 min Scan# 2043
Delta R.T. 0.000 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29

Tgt Ion:232 Resp: 467085
Ion Ratio Lower Upper
232 100
131 41.3 34.4 51.6
130 2.2 2.0 3.0
166 29.8 24.4 36.6




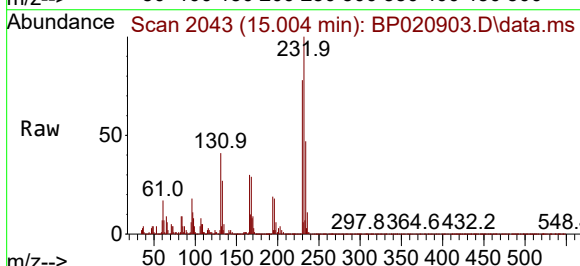




#59
Diethylphthalate
Concen: 32.481 ng/ul
RT: 15.198 min Scan# 2076
Delta R.T. 0.006 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29




Instrument :
BNA_P
ClientSampleId :
A4CC5MS


Tgt Ion:149 Resp: 1843277
Ion Ratio Lower Upper
149 100
177 22.7 17.7 26.5
150 12.6 10.2 15.2

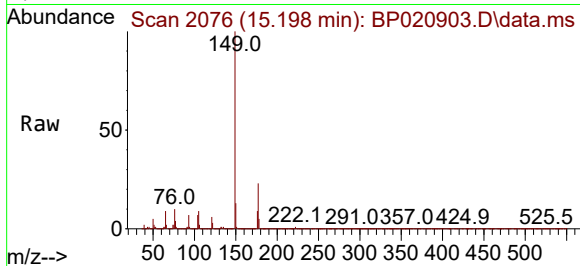

#61
Fluorene
Concen: 32.697 ng/ul
RT: 15.428 min Scan# 2115
Delta R.T. 0.000 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29

Tgt Ion:166 Resp: 1725426
Ion Ratio Lower Upper
166 100
165 98.2 78.1 117.1
167 13.5 10.9 16.3




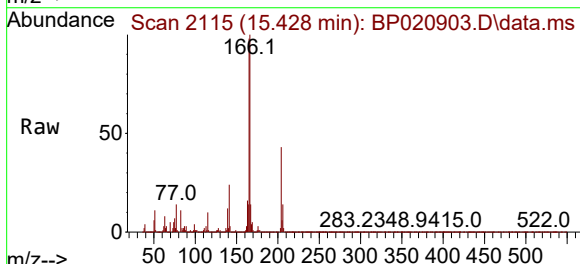




#62
4-Chlorophenyl-phenylether
Concen: 32.445 ng/ul
RT: 15.422 min Scan# 2114
Delta R.T. 0.000 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29




Instrument :
BNA_P
ClientSampleId :
A4CC5MS


Tgt Ion:204 Resp: 929062
Ion Ratio Lower Upper
204 100
206 32.9 26.4 39.6
141 57.1 48.5 72.7

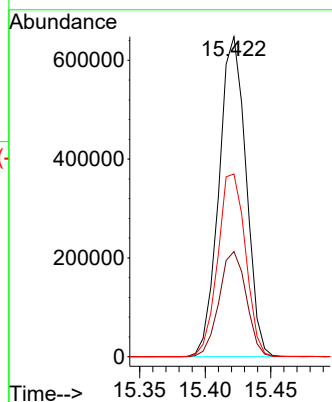

#63
4-Nitroaniline
Concen: 39.969 ng/ul
RT: 15.469 min Scan# 2122
Delta R.T. 0.000 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29

Tgt Ion:138 Resp: 326998
Ion Ratio Lower Upper
138 100
92 50.6 40.9 61.3
108 84.0 64.7 97.1









#66
4,6-Dinitro-2-methylphenol
Concen: 36.089 ng/ul
RT: 15.534 min Scan# 2133
Delta R.T. 0.012 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29




Instrument :
BNA_P
ClientSampleId :
A4CC5MS


Tgt Ion:198 Resp: 324438
Ion Ratio Lower Upper
198 100
182 3.8 3.8 5.6#
77 23.4 20.0 30.0

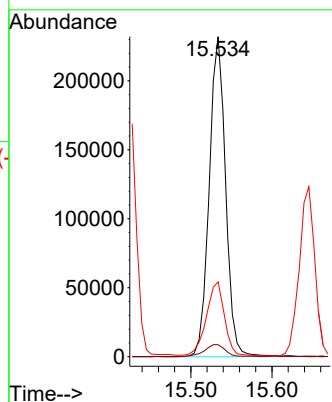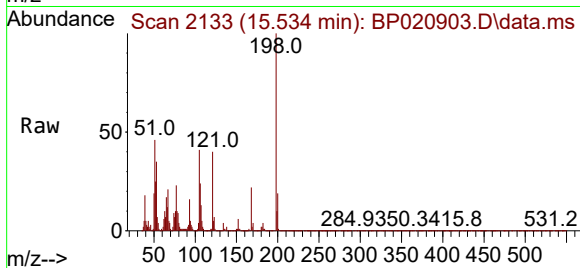

#67
N-Nitrosodiphenylamine
Concen: 36.651 ng/ul
RT: 15.645 min Scan# 2152
Delta R.T. 0.000 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29

Tgt Ion:169 Resp: 1495366
Ion Ratio Lower Upper
169 100
168 67.1 53.4 80.2
167 36.3 28.4 42.6




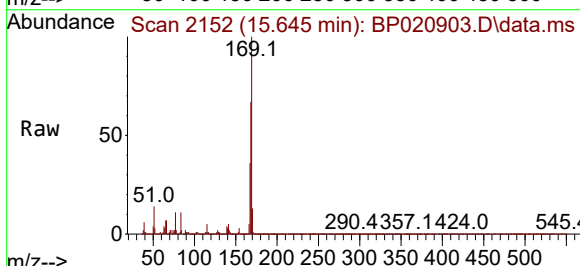




#68
4-Bromophenyl-phenylether
Concen: 35.797 ng/ul
RT: 16.339 min Scan# 21
Delta R.T. 0.000 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29




Instrument :
BNA_P
ClientSampleId :
A4CC5MS


Tgt Ion:248 Resp: 587867
Ion Ratio Lower Upper
248 100
250 97.7 79.3 118.9
141 66.8 57.4 86.0

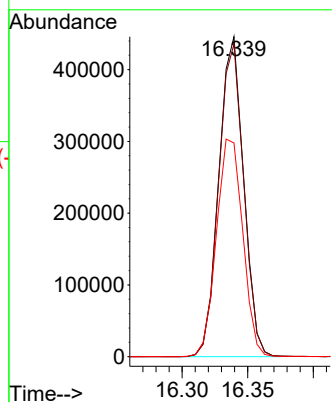

#69
Hexachlorobenzene
Concen: 34.775 ng/ul
RT: 16.451 min Scan# 2289
Delta R.T. 0.000 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29

Tgt Ion:284 Resp: 654817
Ion Ratio Lower Upper
284 100
142 31.2 25.8 38.8
249 32.7 25.1 37.7









#70
 Atrazine
 Concen: 23.252 ng/ul
 RT: 16.634 min Scan# 21
 Delta R.T. 0.012 min
 Lab File: BP020903.D
 Acq: 11 Jul 2024 14:29




Instrument :
 BNA_P
 ClientSampleId :
 A4CC5MS


Tgt Ion:200 Resp: 345745
 Ion Ratio Lower Upper
 200 100
 173 26.3 20.8 31.2
 215 48.2 38.7 58.1



#71
 Pentachlorophenol
 Concen: 31.737 ng/ul
 RT: 16.816 min Scan# 2351
 Delta R.T. -0.006 min
 Lab File: BP020903.D
 Acq: 11 Jul 2024 14:29

Tgt Ion:266 Resp: 324575
 Ion Ratio Lower Upper
 266 100
 264 64.3 52.3 78.5
 268 65.4 52.3 78.5





#72

Phenanthrene

Concen: 35.196 ng/ul

RT: 17.216 min Scan# 2419

Delta R.T. -0.006 min

Lab File: BP020903.D

Acq: 11 Jul 2024 14:29

Instrument :

BNA_P

ClientSampleId :

A4CC5MS





Tgt Ion:178 Resp: 2558120

Ion Ratio Lower Upper

178 100

179 15.2 12.2 18.4

176 19.2 15.0 22.4



#74

Anthracene

Concen: 33.486 ng/ul

RT: 17.316 min Scan# 2436

Delta R.T. 0.012 min

Lab File: BP020903.D

Acq: 11 Jul 2024 14:29




Tgt Ion:178 Resp: 2481224


Ion Ratio Lower Upper

178 100

179 15.7 12.5 18.7

176 18.7 14.8 22.2


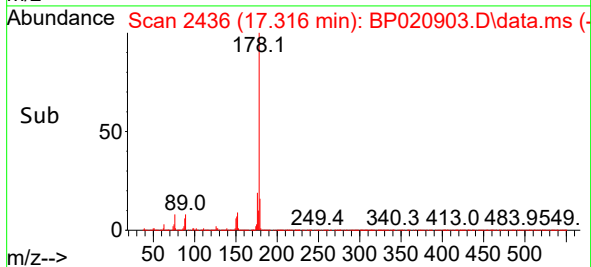

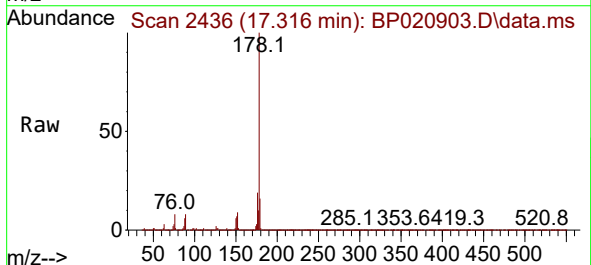




#75
1,2,3,4-Tetrachlorobenzene
Concen: 41.518 ng/uL
RT: 13.134 min Scan# 1725
Delta R.T. -0.006 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29




Instrument :
BNA_P
ClientSampleId :
A4CC5MS


Tgt Ion:216 Resp: 931058
Ion Ratio Lower Upper
216 100
214 78.0 63.2 94.8
218 49.1 38.2 57.4



#76
Pentachlorobenzene
Concen: 33.968 ng/uL
RT: 14.675 min Scan# 1987
Delta R.T. -0.006 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29

Tgt Ion:250 Resp: 756906
Ion Ratio Lower Upper
250 100
248 63.3 50.8 76.2
252 64.0 51.6 77.4





#77

Carbazole

Concen: 33.756 ng/ul

RT: 17.598 min Scan# 2483

Delta R.T. 0.000 min

Lab File: BP020903.D

Acq: 11 Jul 2024 14:29

Instrument :

BNA_P

ClientSampleId :

A4CC5MS





Tgt Ion:167 Resp: 2044660

Ion Ratio Lower Upper

167 100

166 21.7 17.3 25.9

139 13.1 10.2 15.2



#78

Di-n-butylphthalate

Concen: 32.836 ng/ul

RT: 18.175 min Scan# 2582

Delta R.T. -0.006 min

Lab File: BP020903.D

Acq: 11 Jul 2024 14:29




Tgt Ion:149 Resp: 2744069


Ion Ratio Lower Upper

149 100

150 9.3 7.4 11.0

104 5.0 3.9 5.9









#80
Fluoranthene
Concen: 34.871 ng/ul
RT: 19.316 min Scan# 21
Delta R.T. 0.006 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29




Instrument :
BNA_P
ClientSampleId :
A4CC5MS


Tgt Ion:202 Resp: 2557959
Ion Ratio Lower Upper
202 100
101 9.8 8.0 12.0
100 7.8 6.1 9.1

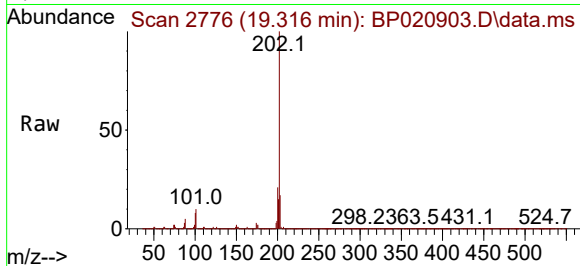

#82
Pyrene
Concen: 35.398 ng/ul
RT: 19.692 min Scan# 2840
Delta R.T. 0.000 min
Lab File: BP020903.D
Acq: 11 Jul 2024 14:29

Tgt Ion:202 Resp: 2642303
Ion Ratio Lower Upper
202 100
101 11.8 9.4 14.2
100 9.9 7.8 11.6





#83

Butylbenzylphthalate

Concen: 32.826 ng/ul

RT: 20.639 min Scan# 3001

Delta R.T. 0.000 min

Lab File: BP020903.D

Acq: 11 Jul 2024 14:29

Instrument :

BNA_P

ClientSampleId :

A4CC5MS





Tgt Ion:149 Resp: 1020901

Ion Ratio Lower Upper

149 100

91 64.2 54.1 81.1

206 22.4 17.0 25.6

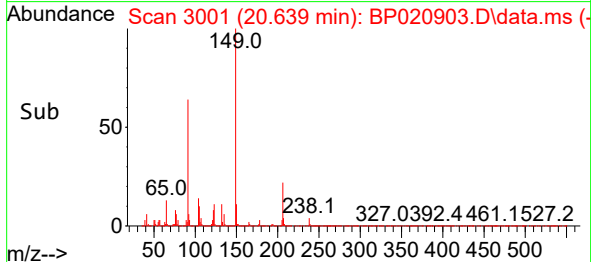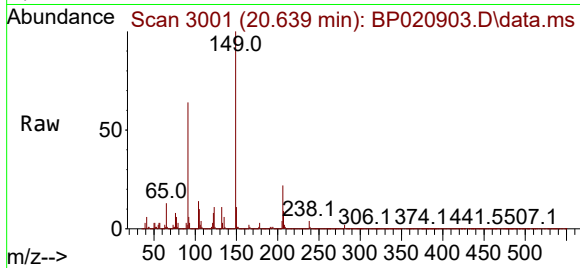

#84

3,3'-Dichlorobenzidine

Concen: 31.869 ng/ul

RT: 21.533 min Scan# 3153

Delta R.T. -0.006 min

Lab File: BP020903.D

Acq: 11 Jul 2024 14:29




Tgt Ion:252 Resp: 715462


Ion Ratio Lower Upper

252 100

254 65.0 51.5 77.3

126 10.1 8.0 12.0

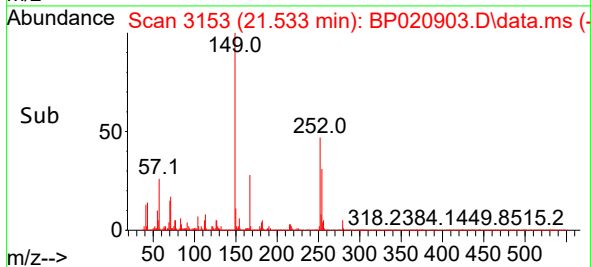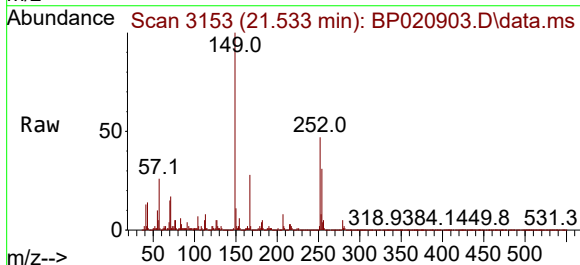



#85

Benzo(a)anthracene

Concen: 34.507 ng/ul

RT: 21.610 min Scan# 3166

Delta R.T. 0.000 min

Lab File: BP020903.D

Acq: 11 Jul 2024 14:29

Instrument :

BNA_P

ClientSampleId :

A4CC5MS





Tgt Ion:228 Resp: 2374913

Ion Ratio Lower Upper

228 100

229 19.8 15.5 23.3

226 27.4 21.4 32.2

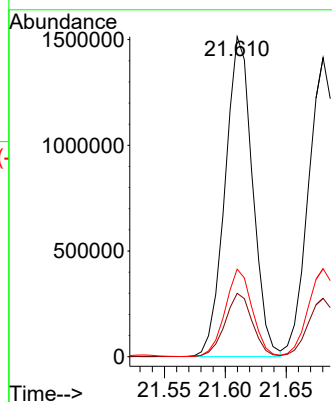

#86

Bis(2-ethylhexyl)phthalate

Concen: 31.777 ng/ul

RT: 21.533 min Scan# 3153

Delta R.T. -0.006 min

Lab File: BP020903.D

Acq: 11 Jul 2024 14:29




Tgt Ion:149 Resp: 1422239


Ion Ratio Lower Upper

149 100

167 28.0 22.1 33.1

279 4.8 3.7 5.5





#87

Chrysene

Concen: 35.494 ng/ul

RT: 21.680 min Scan# 3177

Delta R.T. 0.006 min

Lab File: BP020903.D

Acq: 11 Jul 2024 14:29

Instrument :

BNA_P

ClientSampleId :

A4CC5MS





Tgt Ion:228 Resp: 2269916

Ion Ratio Lower Upper

228 100

226 29.4 23.6 35.4

229 19.5 15.5 23.3



#89

Di-n-octyl phthalate

Concen: 32.275 ng/ul




RT: 22.816 min Scan# 3371


Delta R.T. 0.012 min

Lab File: BP020903.D

Acq: 11 Jul 2024 14:29

Tgt Ion:149 Resp: 2594824

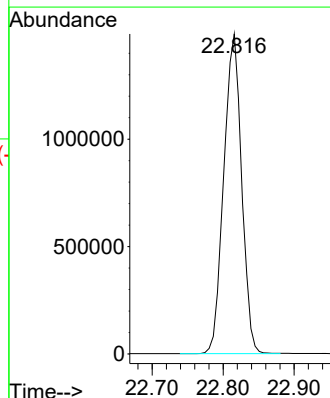



#90

Benzo(b)fluoranthene

Concen: 35.547 ng/ul

RT: 23.921 min Scan# 3559

Delta R.T. 0.000 min

Lab File: BP020903.D

Acq: 11 Jul 2024 14:29

Instrument :

BNA_P

ClientSampleId :

A4CC5MS





Tgt Ion:252 Resp: 2625386

Ion Ratio Lower Upper

252 100

253 21.7 17.1 25.7

125 8.8 7.0 10.4

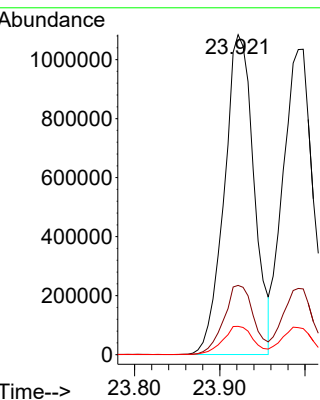

#91

Benzo(k)fluoranthene

Concen: 34.248 ng/ul

RT: 23.998 min Scan# 3572

Delta R.T. 0.006 min

Lab File: BP020903.D

Acq: 11 Jul 2024 14:29




Tgt Ion:252 Resp: 2524321


Ion Ratio Lower Upper

252 100

253 21.5 17.4 26.2

125 8.5 7.4 11.0

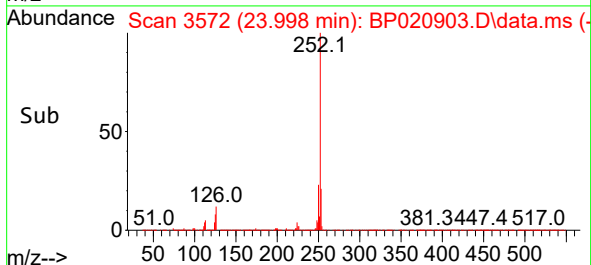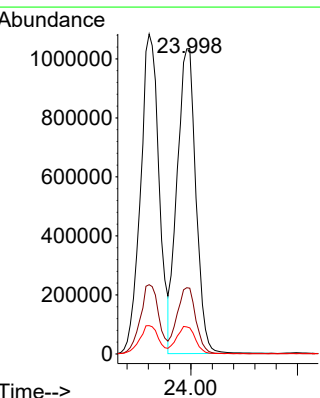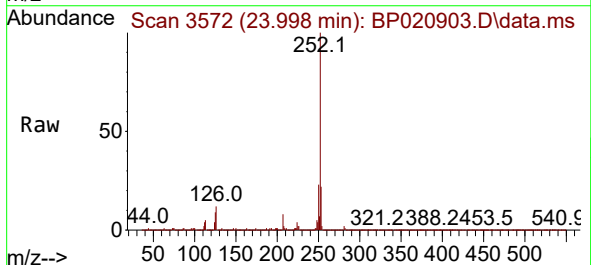



#93

Benzo(a)pyrene

Concen: 31.842 ng/ul

RT: 24.827 min Scan# 31

Delta R.T. 0.000 min

Lab File: BP020903.D

Acq: 11 Jul 2024 14:29

Instrument :

BNA_P

ClientSampleId :

A4CC5MS





Tgt Ion:252 Resp: 2222364

Ion Ratio Lower Upper

252 100

253 21.9 17.4 26.0

125 9.3 7.7 11.5

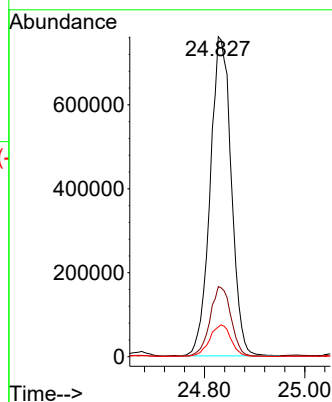

#94

Indeno(1,2,3-cd)pyrene

Concen: 36.944 ng/ul

RT: 28.815 min Scan# 4391

Delta R.T. 0.029 min

Lab File: BP020903.D

Acq: 11 Jul 2024 14:29




Tgt Ion:276 Resp: 3322530


Ion Ratio Lower Upper

276 100

138 17.3 14.3 21.5

277 24.7 19.2 28.8





#95

Dibenzo(a,h)anthracene

Concen: 35.990 ng/ul

RT: 28.874 min Scan# 4401

Delta R.T. 0.012 min

Lab File: BP020903.D

Acq: 11 Jul 2024 14:29

Instrument :

BNA_P

ClientSampleId :

A4CC5MS





Tgt Ion:278 Resp: 2680264

Ion Ratio Lower Upper

278 100

139 13.2 10.9 16.3

279 23.7 19.4 29.0



#96

Benzo(g,h,i)perylene

Concen: 35.556 ng/ul

RT: 29.998 min Scan# 4592

Delta R.T. 0.012 min

Lab File: BP020903.D

Acq: 11 Jul 2024 14:29

Tgt Ion:276 Resp: 2604240

Ion Ratio Lower Upper

276 100

138 18.6 15.3 22.9

277 23.2 18.2 27.2

